

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030168.D
 Acq On : 18 Mar 2019 12:59
 Operator : JC/SP
 Sample : K1936-21DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rVB	11618	11062	0.68%	0.077%
2	1.399	88	96	110	rBV	212265	215637	13.35%	1.502%
3	1.679	174	183	195	rBV	155852	210004	13.00%	1.462%
4	2.190	337	342	348	rBV6	4387	5206	0.32%	0.036%
5	2.270	356	367	381	rBV	350700	530264	32.83%	3.693%
6	2.444	416	421	432	rVB3	3578	5903	0.37%	0.041%
7	2.685	492	496	497	rBV	1712	1120	0.07%	0.008%
8	3.045	605	608	611	rBV	992	761	0.05%	0.005%
9	3.309	687	690	692	rBV	1044	774	0.05%	0.005%
10	3.424	721	726	729	rBV2	1128	1209	0.07%	0.008%
11	3.826	847	851	855	rBV	1367	1357	0.08%	0.009%
12	3.926	878	882	886	rBV	1380	1290	0.08%	0.009%
13	3.958	889	892	895	rBV	1376	935	0.06%	0.007%
14	4.087	929	932	935	rBV	1650	1194	0.07%	0.008%
15	4.174	947	959	983	rBV	173783	450970	27.92%	3.141%
16	4.508	1059	1063	1067	rBV2	1216	1214	0.08%	0.008%
17	4.646	1088	1106	1134	rBV	272602	656269	40.63%	4.570%
18	4.936	1192	1196	1203	rBV2	1489	1876	0.12%	0.013%
19	5.006	1214	1218	1221	rBV	1350	1306	0.08%	0.009%
20	5.058	1231	1234	1243	rVB	2002	2546	0.16%	0.018%
21	5.177	1267	1271	1274	rBV	1142	1051	0.07%	0.007%
22	5.338	1298	1321	1362	rBV2	539697	1615119	100.00%	11.248%
23	5.611	1403	1406	1412	rBV	1455	1319	0.08%	0.009%
24	5.646	1414	1417	1419	rBV	1150	810	0.05%	0.006%
25	5.884	1477	1491	1516	rBV	560631	1123522	69.56%	7.824%
26	6.328	1615	1629	1652	rVV	362321	727820	45.06%	5.069%
27	6.543	1691	1696	1699	rBV2	1854	1845	0.11%	0.013%
28	6.720	1745	1751	1754	rBV	1720	1914	0.12%	0.013%
29	6.768	1760	1766	1769	rBV3	1682	1560	0.10%	0.011%
30	6.784	1769	1771	1779	rVB2	925	1056	0.07%	0.007%
31	6.945	1816	1821	1825	rBV2	1122	1223	0.08%	0.009%
32	6.987	1829	1834	1835	rBV	820	811	0.05%	0.006%
33	7.022	1842	1845	1853	rVB2	2204	2407	0.15%	0.017%
34	7.061	1853	1857	1859	rBV	1850	1426	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030168.D
 Acq On : 18 Mar 2019 12:59
 Operator : JC/SP
 Sample : K1936-21DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	7.106	1867	1871	1875	rBV2	942	1140	0.07%	0.008%
36	7.180	1889	1894	1897	rBV2	1085	1146	0.07%	0.008%
37	7.225	1897	1908	1925	rBV	199395	359091	22.23%	2.501%
38	7.389	1954	1959	1962	rBV2	1314	1479	0.09%	0.010%
39	7.563	2000	2013	2042	rBV	710109	1280536	79.28%	8.918%
40	7.846	2091	2101	2127	rBV	135291	244725	15.15%	1.704%
41	8.177	2195	2204	2207	rBV2	7364	10756	0.67%	0.075%
42	8.225	2208	2219	2235	rVV	507994	883832	54.72%	6.155%
43	8.309	2235	2245	2279	rVB	589691	1049496	64.98%	7.309%
44	8.643	2346	2349	2354	rVB2	1147	973	0.06%	0.007%
45	8.897	2426	2428	2433	rVB	1430	1125	0.07%	0.008%
46	9.019	2463	2466	2468	rBV	1320	865	0.05%	0.006%
47	9.087	2474	2487	2506	rBV	820665	1384719	85.73%	9.643%
48	9.280	2541	2547	2551	rBV2	941	1011	0.06%	0.007%
49	9.640	2656	2659	2665	rBV	1250	1034	0.06%	0.007%
50	9.804	2708	2710	2715	rVB2	1072	786	0.05%	0.005%
51	9.958	2754	2758	2762	rBV2	1514	1485	0.09%	0.010%
52	10.013	2770	2775	2777	rVV	1296	1162	0.07%	0.008%
53	10.116	2801	2807	2808	rBV	1467	1620	0.10%	0.011%
54	10.128	2808	2811	2815	rVB2	1275	1143	0.07%	0.008%
55	10.235	2840	2844	2848	rBV	849	862	0.05%	0.006%
56	10.334	2870	2875	2878	rBV2	1828	1819	0.11%	0.013%
57	10.427	2890	2904	2923	rBV	594291	956187	59.20%	6.659%
58	10.498	2923	2926	2933	rVV	1879	2079	0.13%	0.014%
59	10.543	2937	2940	2943	rVB	2276	1429	0.09%	0.010%
60	10.569	2943	2948	2951	rBV2	1839	2048	0.13%	0.014%
61	10.868	3033	3041	3046	rBV2	1016	1431	0.09%	0.010%
62	10.929	3055	3060	3065	rVV	1207	1384	0.09%	0.010%
63	10.955	3065	3068	3073	rVB2	1178	929	0.06%	0.006%
64	11.003	3078	3083	3088	rBV2	1263	1597	0.10%	0.011%
65	11.080	3104	3107	3108	rBV3	1454	811	0.05%	0.006%
66	11.132	3117	3123	3126	rBV2	1355	1595	0.10%	0.011%
67	11.276	3164	3168	3171	rBV	1399	1009	0.06%	0.007%
68	11.312	3176	3179	3183	rVB	995	824	0.05%	0.006%
69	11.341	3183	3188	3190	rBV	1019	923	0.06%	0.006%
70	11.405	3202	3208	3210	rBV3	1716	1731	0.11%	0.012%
71	11.482	3218	3232	3254	rBV	811456	1317491	81.57%	9.175%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030168.D
 Acq On : 18 Mar 2019 12:59
 Operator : JC/SP
 Sample : K1936-21DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	11.858	3337	3349	3373	rBV	732863	1218652	75.45%	8.487%
73	12.251	3468	3471	3481	rVB	2020	2564	0.16%	0.018%
74	12.292	3481	3484	3487	rBV	1851	1509	0.09%	0.011%
75	12.315	3488	3491	3496	rVV	925	1088	0.07%	0.008%
76	12.366	3503	3507	3511	rBV2	1219	1150	0.07%	0.008%
77	12.431	3524	3527	3529	rBV	1331	980	0.06%	0.007%
78	12.620	3582	3586	3589	rBV2	1561	1298	0.08%	0.009%
79	12.691	3604	3608	3613	rBV	1406	1339	0.08%	0.009%
80	12.755	3625	3628	3634	rBV2	1304	1418	0.09%	0.010%
81	12.855	3657	3659	3663	rVB	1569	995	0.06%	0.007%
82	12.877	3663	3666	3673	rVV2	1205	1247	0.08%	0.009%
83	12.971	3693	3695	3702	rVB	1367	1221	0.08%	0.009%
84	13.080	3724	3729	3734	rVB2	997	1187	0.07%	0.008%
85	13.148	3746	3750	3755	rVB	1504	1396	0.09%	0.010%
86	13.328	3802	3806	3808	rBV2	1528	1063	0.07%	0.007%
87	13.344	3808	3811	3818	rVB	1817	1951	0.12%	0.014%
88	13.379	3818	3822	3826	rBV2	1441	1515	0.09%	0.011%
89	13.514	3861	3864	3867	rBV	1326	929	0.06%	0.006%
90	13.697	3918	3921	3924	rBV	1150	960	0.06%	0.007%
91	13.742	3932	3935	3939	rBV2	1070	772	0.05%	0.005%
92	13.765	3939	3942	3946	rBV	956	982	0.06%	0.007%
93	13.852	3966	3969	3972	rBV	1644	1225	0.08%	0.009%
94	14.061	4031	4034	4037	rBV2	1068	878	0.05%	0.006%
95	14.083	4037	4041	4044	rBV	1517	1137	0.07%	0.008%
96	14.559	4186	4189	4196	rVB	1695	1894	0.12%	0.013%
97	14.591	4196	4199	4202	rBV3	1126	924	0.06%	0.006%
98	15.038	4336	4338	4345	rBV2	1371	1349	0.08%	0.009%
99	15.488	4475	4478	4480	rBV2	1478	1219	0.08%	0.008%
100	15.636	4521	4524	4527	rBV3	1951	1423	0.09%	0.010%


Sum of corrected areas: 14359318

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031819\
Data File : VU030168.D
Acq On : 18 Mar 2019 12:59
Operator : JC/SP
Sample : K1936-21DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

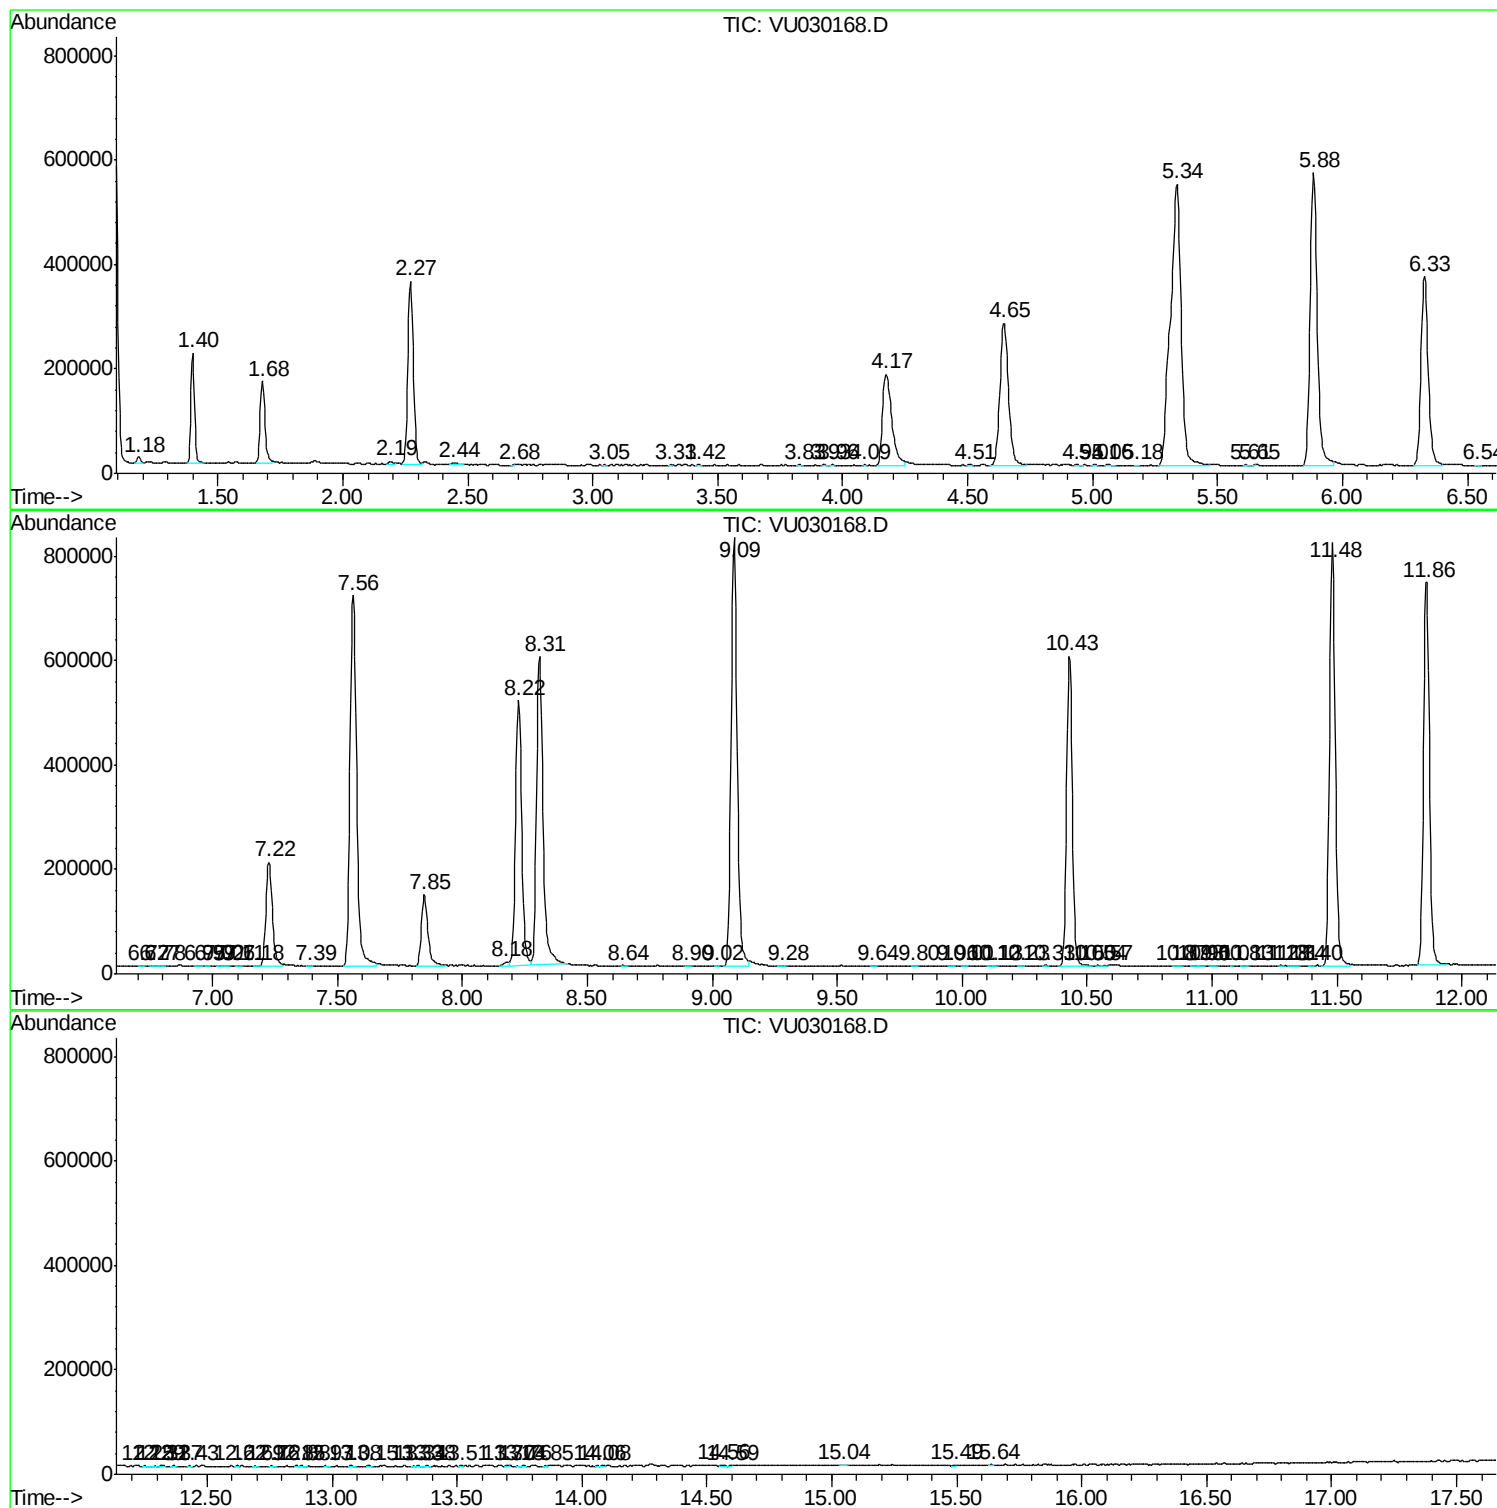

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031819\
Data File : VU030168.D
Acq On : 18 Mar 2019 12:59
Operator : JC/SP
Sample : K1936-21DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031819\
Data File : VU030168.D
Acq On : 18 Mar 2019 12:59
Operator : JC/SP
Sample : K1936-21DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc