

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030176.D
 Acq On : 18 Mar 2019 16:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	35	rVB	10631	8890	0.49%	0.064%
2	1.399	89	96	107	rBV	265292	265206	14.58%	1.905%
3	1.678	176	183	200	rVB	195813	248038	13.64%	1.782%
4	2.270	356	367	381	rBV	422516	647950	35.62%	4.655%
5	2.370	394	398	401	rBV2	1419	1529	0.08%	0.011%
6	2.598	466	469	470	rBV	2000	1223	0.07%	0.009%
7	2.887	557	559	563	rBV	988	808	0.04%	0.006%
8	3.116	628	630	634	rBV	973	894	0.05%	0.006%
9	3.180	648	650	655	rVB	2073	1576	0.09%	0.011%
10	3.219	655	662	665	rBV	1494	1593	0.09%	0.011%
11	3.280	675	681	686	rBV	1517	2111	0.12%	0.015%
12	3.325	691	695	703	rVB3	1213	1293	0.07%	0.009%
13	3.389	712	715	720	rVB2	1070	857	0.05%	0.006%
14	3.485	741	745	747	rBV	1089	943	0.05%	0.007%
15	3.685	802	807	810	rBV	1572	1571	0.09%	0.011%
16	3.704	810	813	817	rVV	1361	1455	0.08%	0.010%
17	3.733	817	822	825	rVV	1591	1852	0.10%	0.013%
18	3.772	831	834	840	rVB	1602	1618	0.09%	0.012%
19	3.823	845	850	853	rBV	1374	1531	0.08%	0.011%
20	3.865	860	863	866	rBV	1569	1157	0.06%	0.008%
21	4.135	944	947	949	rBV	1420	814	0.04%	0.006%
22	4.177	949	960	986	rBV	83323	228791	12.58%	1.644%
23	4.460	1045	1048	1055	rVB	2370	1972	0.11%	0.014%
24	4.492	1055	1058	1063	rBV	1355	1439	0.08%	0.010%
25	4.646	1090	1106	1127	rVV	299451	705918	38.81%	5.072%
26	4.865	1170	1174	1176	rVV	1389	953	0.05%	0.007%
27	4.939	1194	1197	1201	rVB2	1448	1078	0.06%	0.008%
28	4.981	1206	1210	1216	rVB	1818	1623	0.09%	0.012%
29	5.009	1216	1219	1222	rBV2	1042	992	0.05%	0.007%
30	5.054	1230	1233	1235	rBV	1331	795	0.04%	0.006%
31	5.170	1264	1269	1272	rBV	1488	1516	0.08%	0.011%
32	5.254	1292	1295	1298	rBV	1711	1132	0.06%	0.008%
33	5.337	1298	1321	1353	rBV2	616508	1818990	100.00%	13.068%
34	5.640	1411	1415	1418	rBV	1385	1116	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030176.D
 Acq On : 18 Mar 2019 16:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	5.755	1447	1451	1456	rVB	1911	1474	0.08%	0.011%
36	5.884	1477	1491	1521	rBV	562332	1132504	62.26%	8.136%
37	6.087	1551	1554	1555	rBV	1465	839	0.05%	0.006%
38	6.164	1574	1578	1579	rBV2	2057	1417	0.08%	0.010%
39	6.328	1615	1629	1652	rBV	398082	804645	44.24%	5.781%
40	6.630	1718	1723	1725	rBV	1658	1117	0.06%	0.008%
41	6.662	1730	1733	1735	rVV	1520	1064	0.06%	0.008%
42	6.720	1744	1751	1753	rBV	1648	1526	0.08%	0.011%
43	6.794	1769	1774	1777	rBV	1773	1854	0.10%	0.013%
44	6.932	1814	1817	1822	rVB	1506	1160	0.06%	0.008%
45	7.022	1842	1845	1852	rBV2	1170	1290	0.07%	0.009%
46	7.225	1897	1908	1936	rVV	174447	324123	17.82%	2.329%
47	7.562	2000	2013	2041	rBV	811201	1469656	80.80%	10.558%
48	7.742	2065	2069	2072	rVV	1707	1444	0.08%	0.010%
49	7.762	2073	2075	2081	rVB2	1891	1660	0.09%	0.012%
50	7.849	2091	2102	2119	rBV	122344	216855	11.92%	1.558%
51	8.080	2167	2174	2179	rBV3	1458	1901	0.10%	0.014%
52	8.144	2188	2194	2195	rBV2	1434	1169	0.06%	0.008%
53	8.173	2197	2203	2211	rVV2	7311	11815	0.65%	0.085%
54	8.228	2212	2220	2229	rVB5	11646	20778	1.14%	0.149%
55	8.308	2234	2245	2271	rBV	523154	937311	51.53%	6.734%
56	8.652	2349	2352	2357	rBV2	1160	1175	0.06%	0.008%
57	8.678	2357	2360	2361	rBV	1568	821	0.05%	0.006%
58	8.903	2425	2430	2433	rBV	1155	1183	0.07%	0.008%
59	9.006	2459	2462	2465	rVB	1396	949	0.05%	0.007%
60	9.025	2465	2468	2471	rBV	1608	1218	0.07%	0.009%
61	9.086	2474	2487	2516	rBV	818903	1408080	77.41%	10.116%
62	9.360	2566	2572	2575	rBV	1588	1749	0.10%	0.013%
63	9.427	2587	2593	2596	rBV2	1693	1681	0.09%	0.012%
64	9.678	2668	2671	2674	rBV	1213	806	0.04%	0.006%
65	9.713	2679	2682	2686	rVV2	1094	904	0.05%	0.006%
66	9.848	2721	2724	2731	rVB	1430	1620	0.09%	0.012%
67	10.064	2789	2791	2794	rVB	1431	872	0.05%	0.006%
68	10.154	2816	2819	2824	rVB	1440	1332	0.07%	0.010%
69	10.247	2845	2848	2854	rVB	2008	1744	0.10%	0.013%
70	10.279	2854	2858	2862	rVB	1704	1281	0.07%	0.009%
71	10.308	2863	2867	2871	rBV	977	937	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030176.D
 Acq On : 18 Mar 2019 16:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.427	2887	2904	2926	rBV	599691	978229	53.78%	7.028%
73	10.839	3029	3032	3034	rBV	1163	883	0.05%	0.006%
74	10.887	3044	3047	3051	rBV	1187	898	0.05%	0.006%
75	11.080	3104	3107	3111	rBV	962	935	0.05%	0.007%
76	11.151	3125	3129	3132	rBV2	932	796	0.04%	0.006%
77	11.241	3154	3157	3163	rVB	1447	1121	0.06%	0.008%
78	11.318	3177	3181	3184	rBV	1243	1153	0.06%	0.008%
79	11.430	3207	3216	3220	rBV	1719	2681	0.15%	0.019%
80	11.482	3220	3232	3254	rBV	780317	1268975	69.76%	9.117%
81	11.710	3300	3303	3306	rBV	1329	1053	0.06%	0.008%
82	11.858	3336	3349	3370	rBV	781234	1312115	72.13%	9.427%
83	12.649	3593	3595	3601	rBV2	1014	865	0.05%	0.006%
84	13.089	3728	3732	3736	rBV2	1597	1986	0.11%	0.014%
85	13.273	3783	3789	3792	rBV2	1206	1500	0.08%	0.011%
86	13.546	3871	3874	3876	rBV2	1278	908	0.05%	0.007%
87	13.752	3932	3938	3945	rBV	2253	3474	0.19%	0.025%
88	13.829	3959	3962	3965	rBV2	1561	960	0.05%	0.007%
89	13.942	3993	3997	4003	rBV2	2088	2279	0.13%	0.016%
90	14.151	4058	4062	4066	rBV	2351	2210	0.12%	0.016%
91	14.215	4080	4082	4090	rVB2	1674	1555	0.09%	0.011%
92	14.311	4110	4112	4115	rBV	1363	829	0.05%	0.006%
93	14.562	4187	4190	4196	rBV	1521	1897	0.10%	0.014%
94	14.662	4218	4221	4227	rVB	2002	2053	0.11%	0.015%
95	15.173	4377	4380	4382	rBV2	1563	1149	0.06%	0.008%
96	15.385	4443	4446	4450	rBV3	1652	1180	0.06%	0.008%
97	15.424	4455	4458	4461	rBV2	1315	1048	0.06%	0.008%
98	15.594	4507	4511	4516	rBV2	2417	2647	0.15%	0.019%
99	15.642	4523	4526	4529	rVB	1910	996	0.05%	0.007%
100	16.112	4669	4672	4675	rBV2	2364	1667	0.09%	0.012%


Sum of corrected areas: 13919220

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031819\
Data File : VU030176.D
Acq On : 18 Mar 2019 16:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

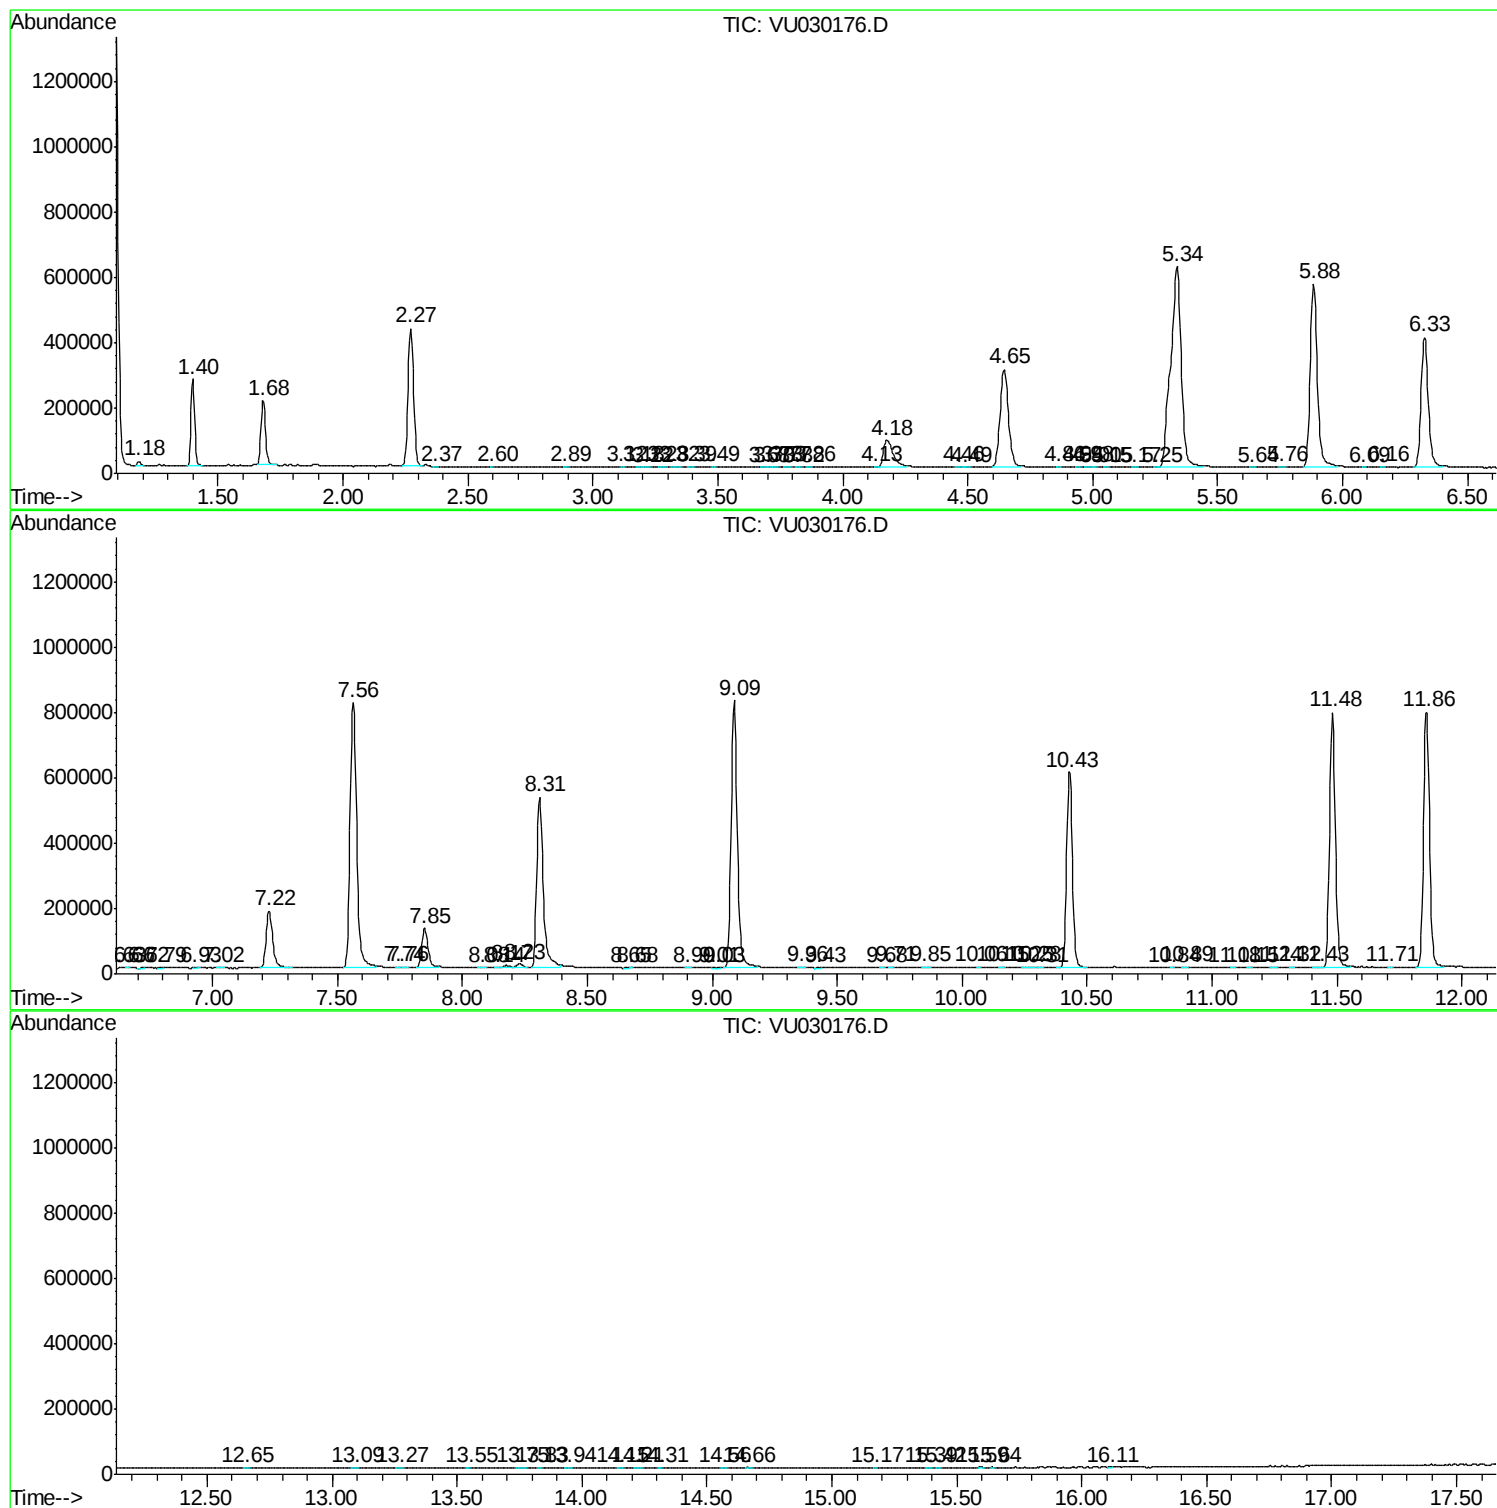

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031819\
Data File : VU030176.D
Acq On : 18 Mar 2019 16:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031819\
Data File : VU030176.D
Acq On : 18 Mar 2019 16:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc