


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031819\
Data File : VU030158.D
Acq On : 18 Mar 2019 08:51
Operator : JC/SP
Sample : BFB36
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Title : VOC Analysis
Last Update : Mon Mar 18 12:44:57 2019

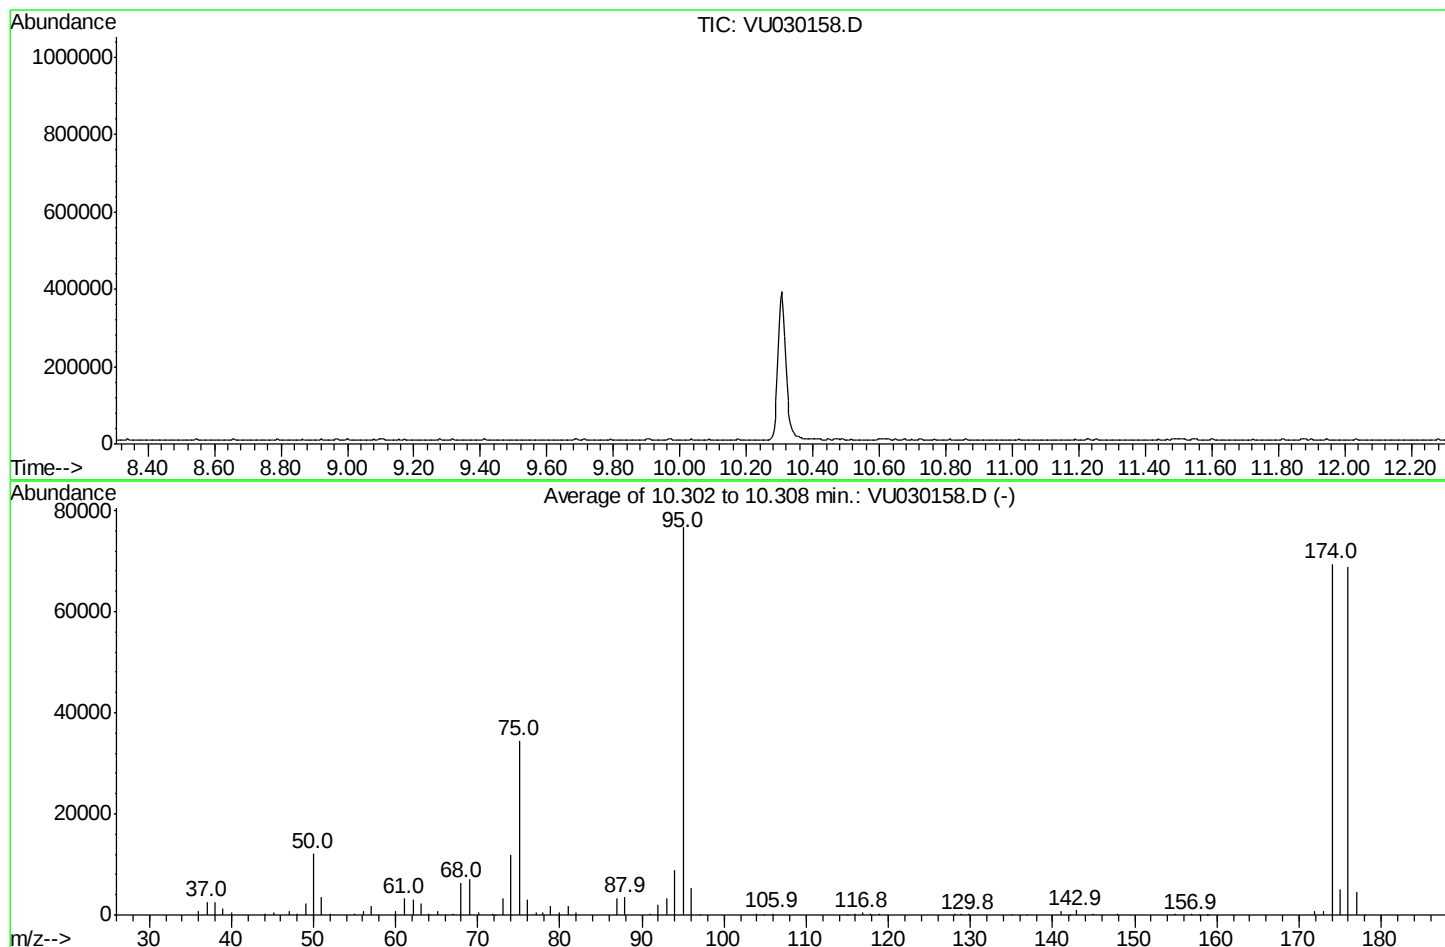

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	12051	PASS
75	95	30	80	45.1	34533	PASS
95	95	100	100	100.0	76642	PASS
96	95	5	9	6.9	5286	PASS
173	174	0.00	2	1.2	799	PASS
174	95	50	120	90.6	69440	PASS
175	174	5	9	7.3	5100	PASS
176	174	95	101	99.2	68882	PASS
177	176	5	9	6.5	4483	PASS

Scan 2853 (10.263 min): VU030158.D
BFB36

m/z	Abundance
40.00	10508.0
44.00	382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	608.0
37.00	2435.0
38.00	2378.0
39.00	1138.0
40.00	11279.0
44.00	631.0
45.10	502.0
47.00	834.0
47.90	288.0
49.00	2133.0
50.00	11961.0
51.00	3603.0
52.10	232.0
54.90	168.0
56.00	671.0
57.10	1750.0
60.00	658.0
61.00	3178.0
62.10	3033.0
63.00	2250.0
64.00	340.0
65.10	695.0
66.00	127.0
66.90	160.0
68.00	6315.0
69.00	7152.0
70.10	568.0
71.90	323.0
73.00	3456.0
74.00	11738.0
75.10	34696.0
76.00	3010.0
77.10	449.0
77.90	404.0
78.90	1779.0
80.00	488.0
80.90	1691.0
82.00	492.0
86.90	3105.0
87.90	3354.0
91.00	240.0
92.00	2042.0
93.00	3296.0
94.00	8625.0
95.10	74824.0
96.00	5523.0
97.00	148.0
104.00	288.0
104.80	101.0
105.90	365.0
115.00	113.0
116.00	206.0
116.90	459.0
117.70	269.0
118.90	305.0
128.10	160.0
128.80	134.0
129.80	261.0
134.90	117.0
136.80	119.0
141.00	688.0
142.90	866.0
144.80	142.0
147.80	166.0
155.00	169.0
156.90	131.0
158.80	118.0
171.90	886.0
173.00	730.0
174.00	66712.0
175.00	4767.0
176.00	65792.0
177.00	4156.0
178.00	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	721.0
37.00	2671.0
38.00	2497.0
39.00	1219.0
40.00	11268.0
44.00	660.0
45.10	635.0
47.00	884.0
47.90	302.0
49.00	2241.0
50.00	12445.0
51.00	3704.0
52.10	217.0
54.90	200.0
56.00	736.0
57.10	1842.0
60.00	720.0
61.00	3277.0
62.10	3220.0
63.00	2374.0
64.00	320.0
65.10	719.0
66.00	114.0
66.90	196.0
68.00	6613.0
69.00	7374.0
70.10	641.0
71.90	351.0
73.00	3445.0
74.00	12341.0
75.10	35600.0
76.00	3084.0
77.00	481.0
77.90	413.0
78.90	1920.0
79.90	553.0
80.90	1792.0
82.00	527.0
86.90	3440.0
87.90	3702.0
90.90	246.0
92.00	2083.0
93.00	3375.0
94.00	9314.0
95.10	79368.0
96.00	5468.0
97.00	133.0
104.00	275.0
105.90	362.0
114.90	105.0
116.00	242.0
116.90	516.0
117.80	313.0
118.90	312.0
128.00	231.0
128.90	179.0
129.80	263.0
134.90	111.0
136.80	110.0
141.00	723.0
142.90	1024.0
144.90	164.0
147.90	150.0
154.90	153.0
156.90	175.0
171.90	843.0
173.10	821.0
174.00	71608.0
175.00	5223.0
176.00	71120.0
177.00	4629.0
177.90	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	699.0
37.00	2630.0
38.00	2459.0
39.00	1202.0
40.00	10836.0
44.00	652.0
45.10	658.0
47.00	884.0
47.90	330.0
49.00	2276.0
50.00	11747.0
51.00	3673.0
52.00	176.0
55.00	216.0
56.10	753.0
57.00	1749.0
60.00	642.0
61.00	3073.0
62.10	3064.0
63.10	2321.0
64.00	330.0
65.00	706.0
66.00	107.0
67.00	208.0
68.00	6435.0
69.00	7135.0
70.00	652.0
71.80	326.0
72.20	291.0
73.00	3108.0
74.00	11628.0
75.00	33304.0
76.00	2770.0
77.00	536.0
77.90	366.0
78.90	1857.0
79.90	564.0
81.00	1892.0
82.00	539.0
86.90	3307.0
87.90	3466.0
90.90	251.0
92.00	1959.0
93.00	3047.0
94.00	8888.0
95.00	75736.0
96.00	4868.0
103.90	215.0
104.80	105.0
105.90	366.0
116.00	220.0
116.80	502.0
117.80	303.0
119.00	301.0
128.00	258.0
128.90	177.0
129.80	223.0
135.00	113.0
141.00	708.0
142.10	127.0
142.90	1022.0
145.00	185.0
147.90	122.0
154.90	138.0
156.90	216.0
157.90	102.0
159.00	114.0
171.90	810.0
173.10	847.0
174.00	70000.0
175.00	5310.0
176.00	69736.0
177.00	4666.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36