

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031821\
 Data File : VU042701.D
 Acq On : 18 Mar 2021 10:50
 Operator : SY/MD
 Sample : VU0318WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0318WBL01

Quant Time: Mar 19 02:18:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031721DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 18 07:25:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.128	96	15603	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.645	95	5653	0.81	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.00%	
68) 1,2-Dichlorobenzene-d4	12.201	152	6376	0.87	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031821\
Data File : VU042701.D
Acq On : 18 Mar 2021 10:50
Operator : SY/MD
Sample : VU0318WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Quant Time: Mar 19 02:18:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 18 07:25:09 2021
Response via : Initial Calibration

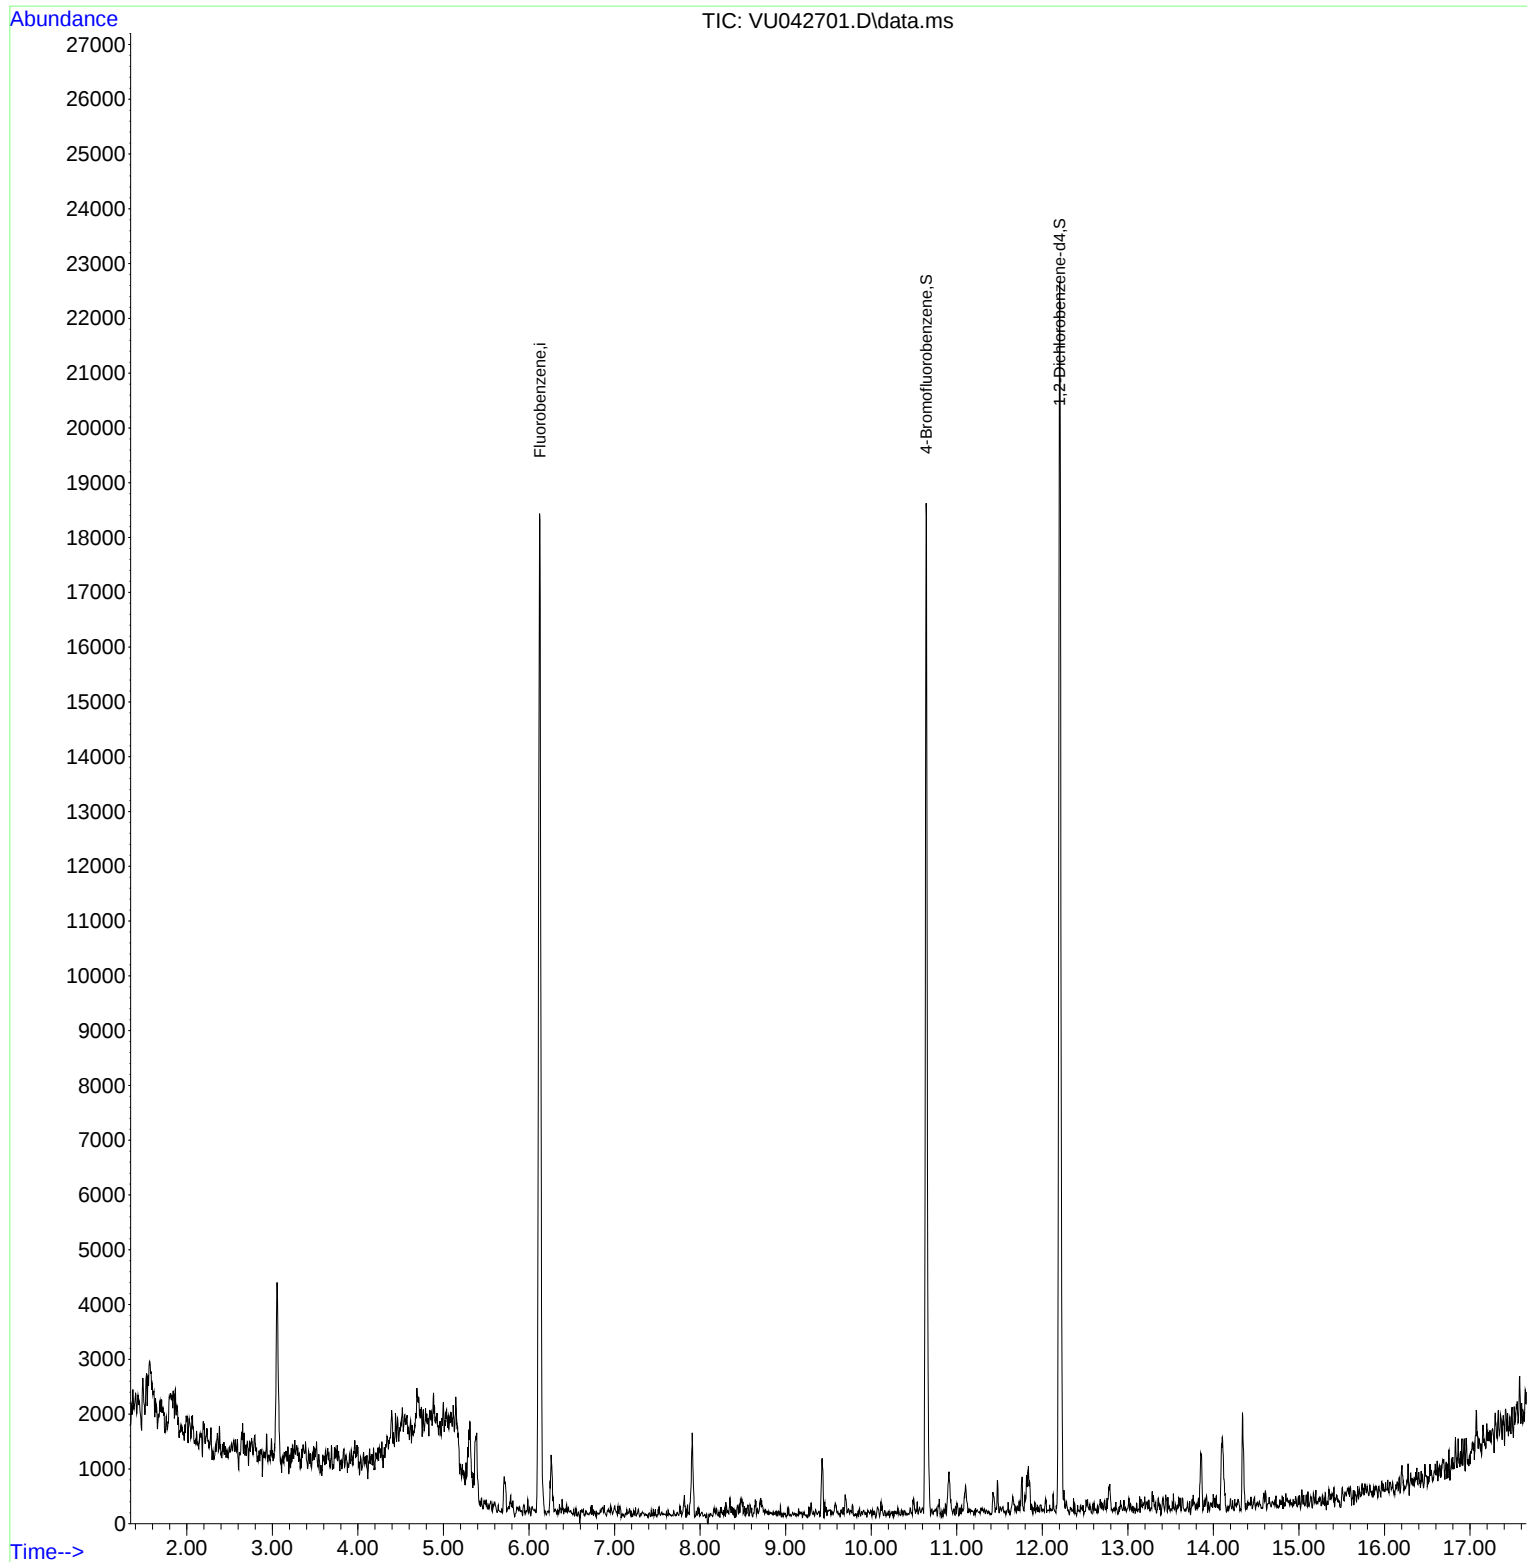




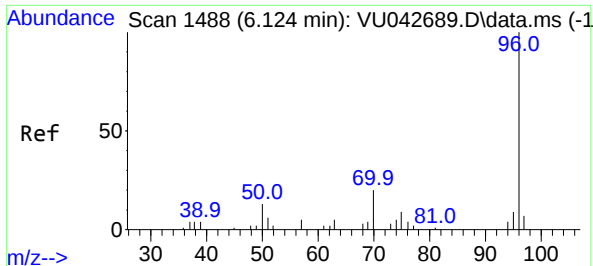


#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.128 min Scan# 1489
Delta R.T. 0.004 min
Lab File: VU042701.D
Acq: 18 Mar 2021 10:50

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Tgt Ion: 96 Resp: 15603




Ion	Ratio	Lower	Upper
96	100		
70	19.8	17.2	25.8
95	10.2	8.0	12.0
97	7.1	0.0	0.0

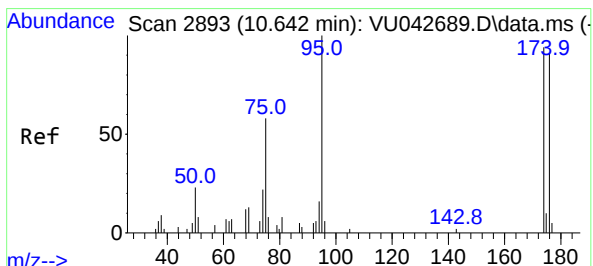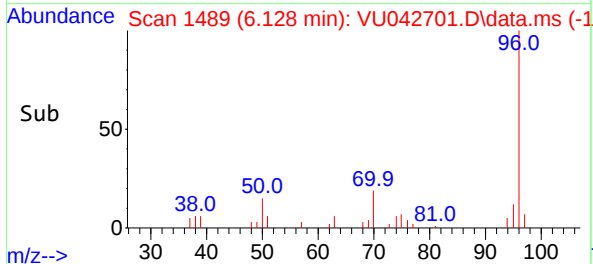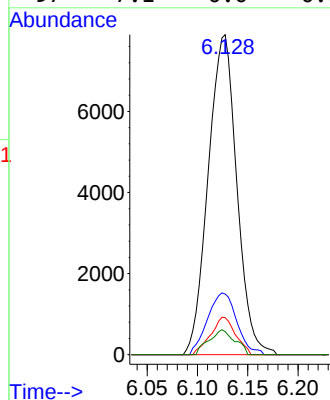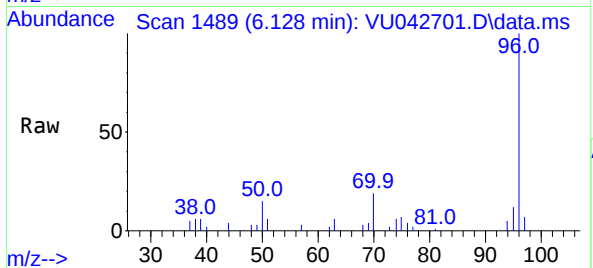


#57
4-Bromofluorobenzene
Concen: 0.81 ug/l
RT: 10.645 min Scan# 2894
Delta R.T. 0.003 min
Lab File: VU042701.D
Acq: 18 Mar 2021 10:50

Tgt Ion: 95 Resp: 5653

Ion	Ratio	Lower	Upper
95	100		
174	90.7	73.8	110.6
176	85.4	71.4	107.0

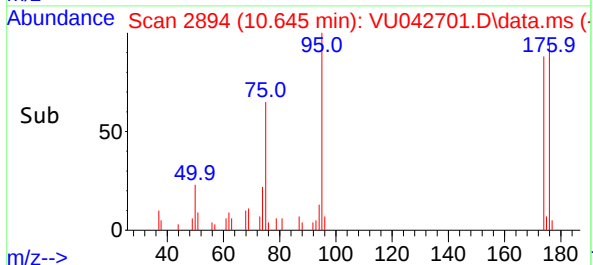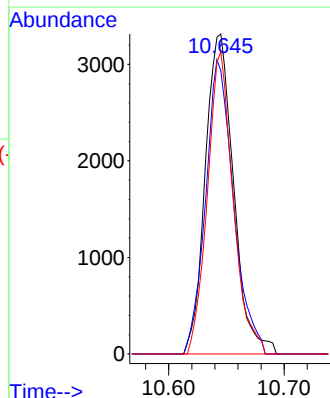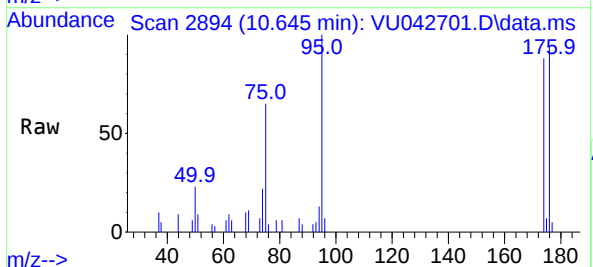

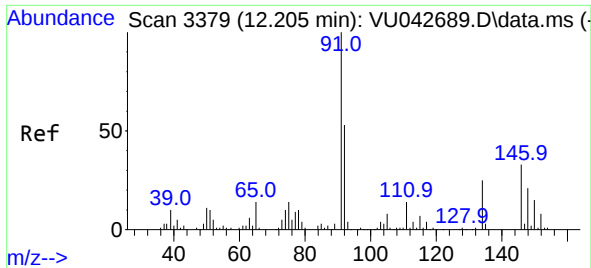

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.87 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. -0.004 min
 Lab File: VU042701.D
 Acq: 18 Mar 2021 10:50

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0318WBL01

Tgt Ion:	152	Resp:	6376
Ion	Ratio	Lower	Upper
152	100		
115	59.6	0.0	271.0
150	155.0	0.0	633.0

