
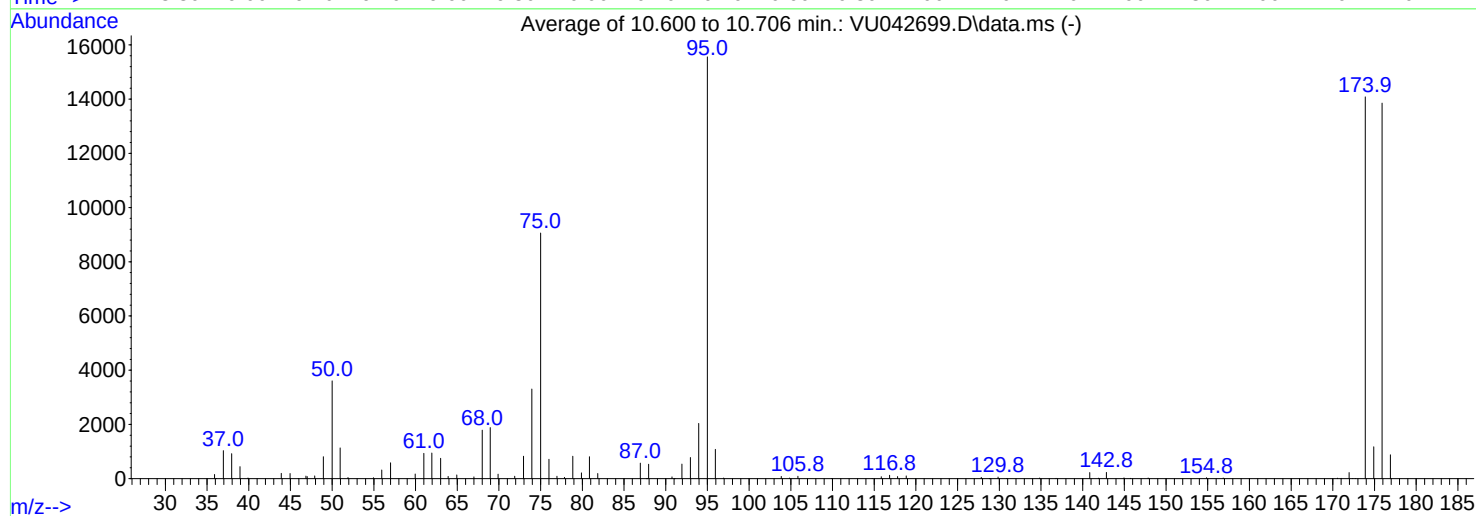


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031821\
 Data File : VU042699.D
 Acq On : 18 Mar 2021 09:34
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031721DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Mar 18 07:25:09 2021

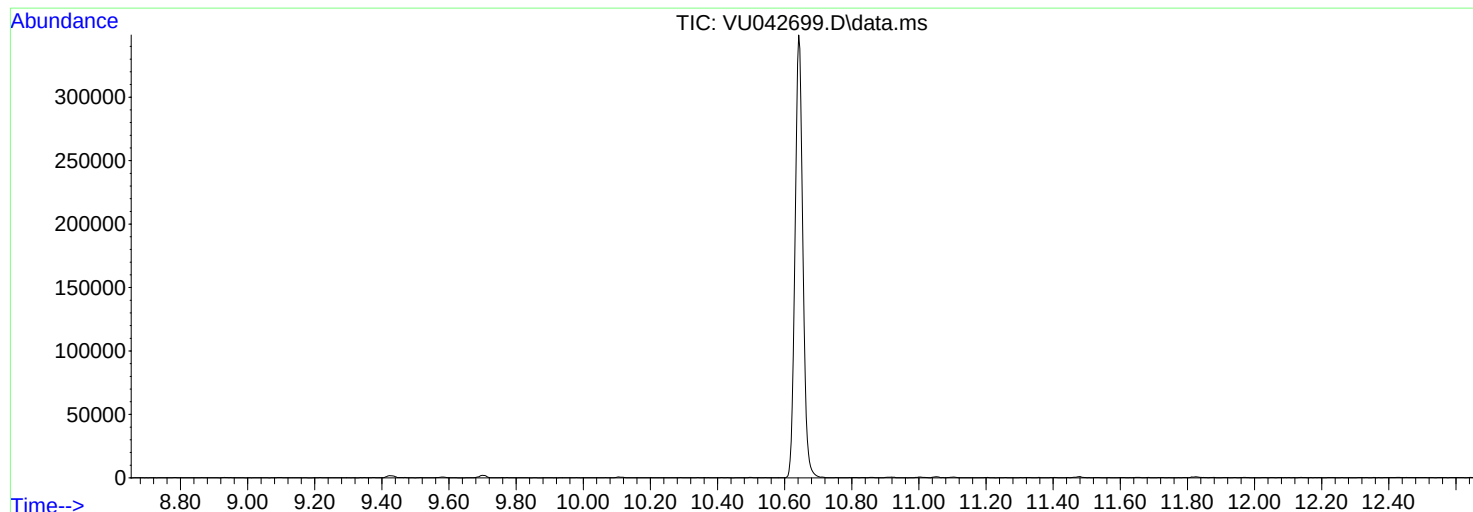

AutoFind: Averaged scan 2880 to 2913; Bkg corrected with scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	3606	PASS
75	95	30	60	58.2	9057	PASS
95	95	100	100	100.0	15559	PASS
96	95	5	9	7.0	1082	PASS
173	174	0.00	2	0.0	4	PASS
174	95	50	100	90.5	14081	PASS
175	174	5	9	8.3	1174	PASS
176	174	95	101	98.4	13854	PASS
177	176	5	9	6.3	878	PASS