

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
 Data File : VU047615.D
 Acq On : 18 Mar 2022 14:47
 Operator : SY/MD
 Sample : VU0318WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0318WBL01

Quant Time: Mar 19 05:12:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Mar 18 13:19:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	30055	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	9151	0.817	ug/l	0.00
Spiked Amount	1.000		Recovery	=	82.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	12585	0.927	ug/l	0.00
Spiked Amount	1.000		Recovery	=	93.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
Data File : VU047615.D
Acq On : 18 Mar 2022 14:47
Operator : SY/MD
Sample : VU0318WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Quant Time: Mar 19 05:12:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 18 13:19:37 2022
Response via : Initial Calibration




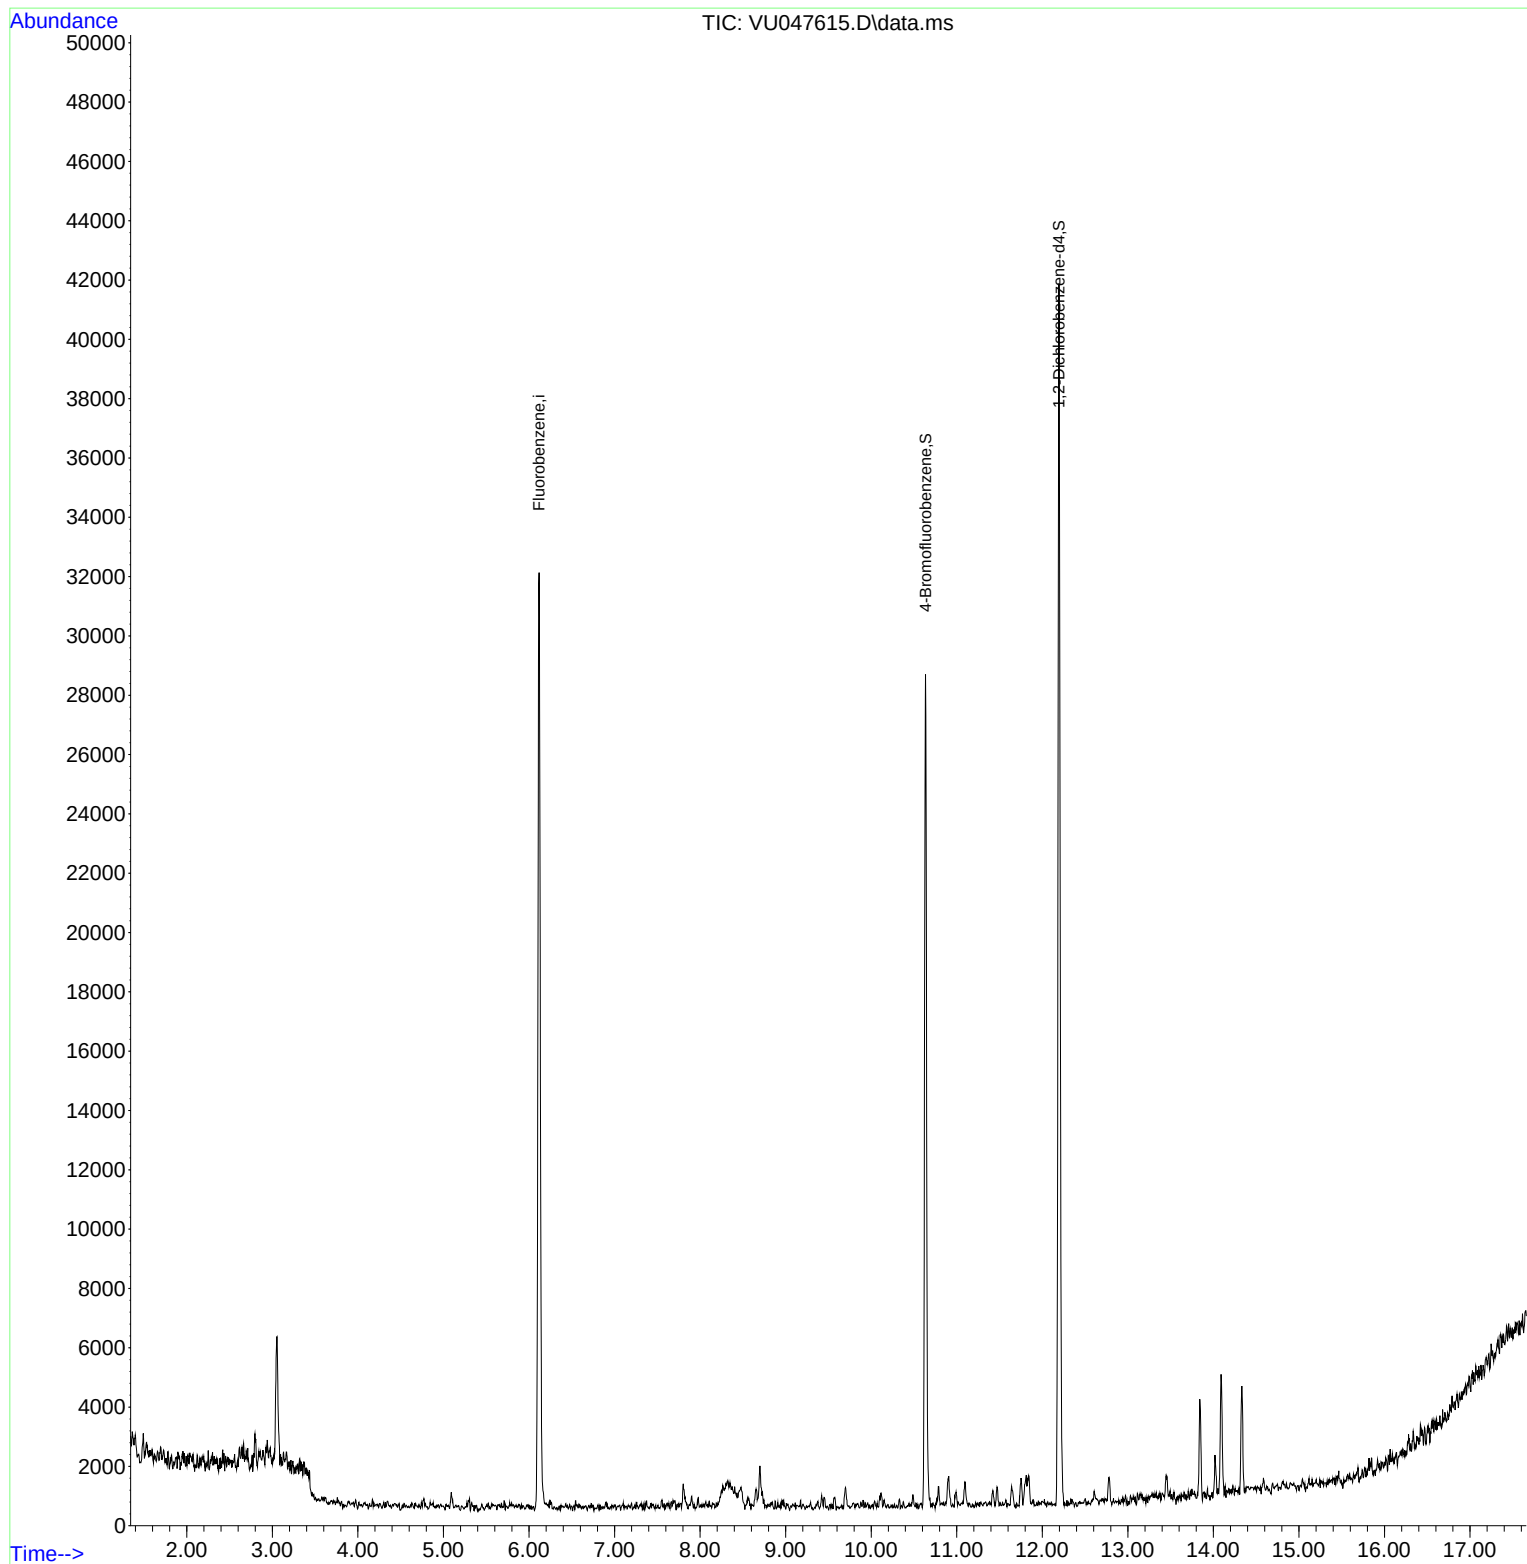


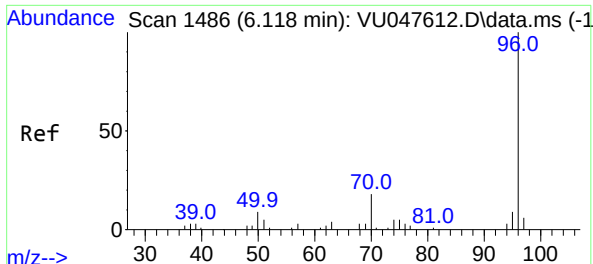

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047615.D
Acq: 18 Mar 2022 14:47




Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01


Tgt Ion: 96	Resp: 30055
Ion Ratio	Lower Upper
96 100	
70 18.8	16.8 25.2
95 9.6	7.3 10.9
97 6.7	0.0 0.0#

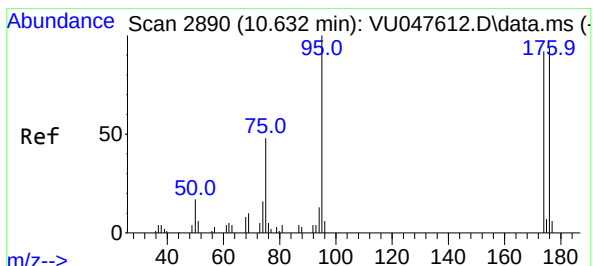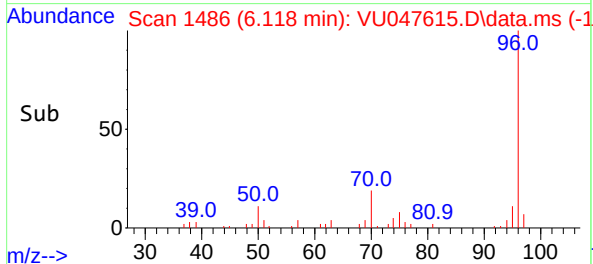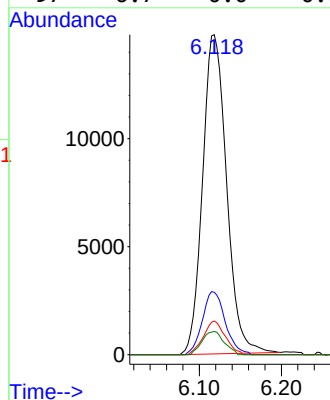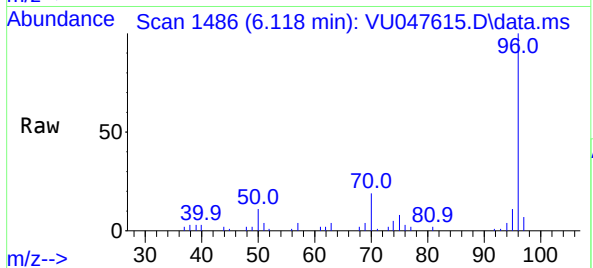

#57
4-Bromofluorobenzene
Concen: 0.817 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU047615.D
Acq: 18 Mar 2022 14:47

Tgt Ion: 95	Resp: 9151
Ion Ratio	Lower Upper
95 100	
174 100.7	56.6 84.8#
176 94.9	54.3 81.5#

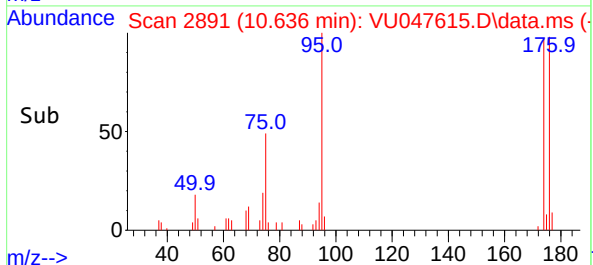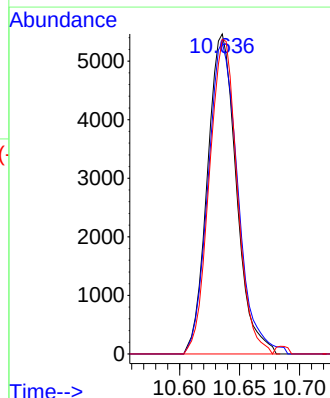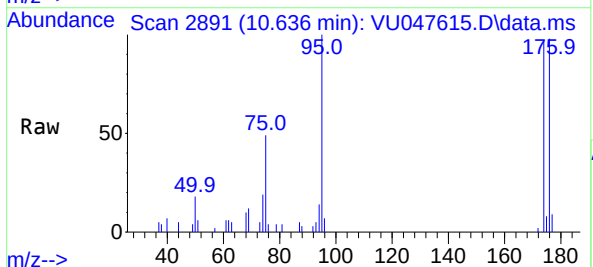

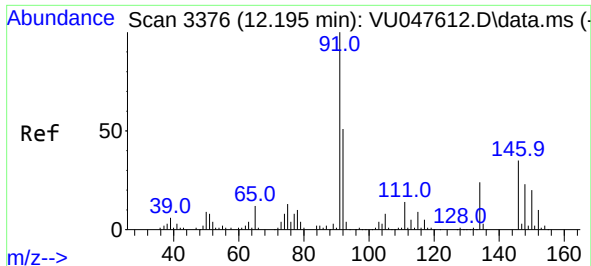

#68

1,2-Dichlorobenzene-d4

Concen: 0.927 ug/l

RT: 12.195 min Scan# 31

Delta R.T. -0.000 min

Lab File: VU047615.D


Acq: 18 Mar 2022 14:47

Instrument :

MSVOA_U

ClientSampleId :

VU0318WBL01

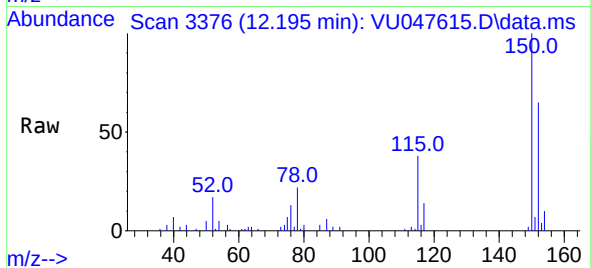

Tgt Ion:152 Resp: 12585

Ion Ratio Lower Upper

152 100

115 56.5 0.0 251.0

150 156.5 0.0 613.8

