

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
 Data File : VU047615.D
 Acq On : 18 Mar 2022 14:47
 Operator : SY/MD
 Sample : VU0318WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0318WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU047615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.617	392	397	401	rBV4	668	767	1.08%	0.345%
2	3.054	522	533	544	rVB6	4325	8233	11.59%	3.699%
3	5.092	1161	1167	1176	rBV5	543	738	1.04%	0.332%
4	6.118	1469	1486	1506	rBV	31624	60896	85.70%	27.359%
5	7.803	2004	2010	2012	rBV2	827	752	1.06%	0.338%
6	8.478	2209	2220	2234	rVB3	752	2299	3.24%	1.033%
7	8.655	2266	2275	2279	rBV4	587	925	1.30%	0.416%
8	8.700	2282	2289	2296	rVV3	1121	1558	2.19%	0.700%
9	9.700	2593	2600	2610	rBV3	707	1155	1.63%	0.519%
10	10.636	2879	2891	2905	rBV2	28103	45241	63.67%	20.325%
11	10.906	2965	2975	2986	rVB4	1039	1860	2.62%	0.836%
12	10.992	2995	3002	3007	rBV4	516	768	1.08%	0.345%
13	11.095	3028	3034	3046	rVB5	831	1279	1.80%	0.575%
14	11.472	3145	3151	3158	rVB3	644	849	1.19%	0.381%
15	11.642	3198	3204	3215	rVB2	688	1145	1.61%	0.514%
16	11.751	3231	3238	3245	rBV4	942	1341	1.89%	0.602%
17	11.812	3245	3257	3259	rBV5	1016	1643	2.31%	0.738%
18	12.195	3364	3376	3395	rVB	41220	71061	100.00%	31.925%
19	12.780	3552	3558	3564	rVB3	804	1133	1.59%	0.509%
20	13.841	3881	3888	3898	rVB4	3440	5058	7.12%	2.272%
21	14.018	3936	3943	3951	rBV6	1430	1881	2.65%	0.845%
22	14.089	3957	3965	3976	rVB	4082	6492	9.14%	2.917%
23	14.333	4033	4041	4050	rBV2	3654	5510	7.75%	2.475%




Sum of corrected areas: 222584

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
Data File : VU047615.D
Acq On : 18 Mar 2022 14:47
Operator : SY/MD
Sample : VU0318WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

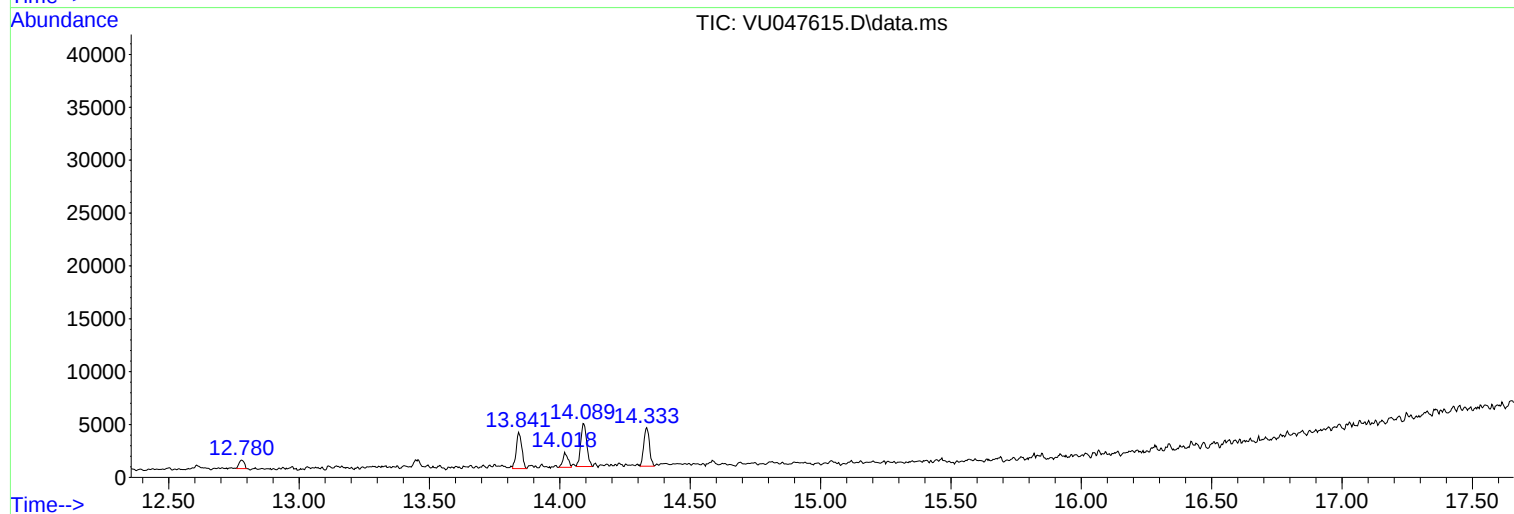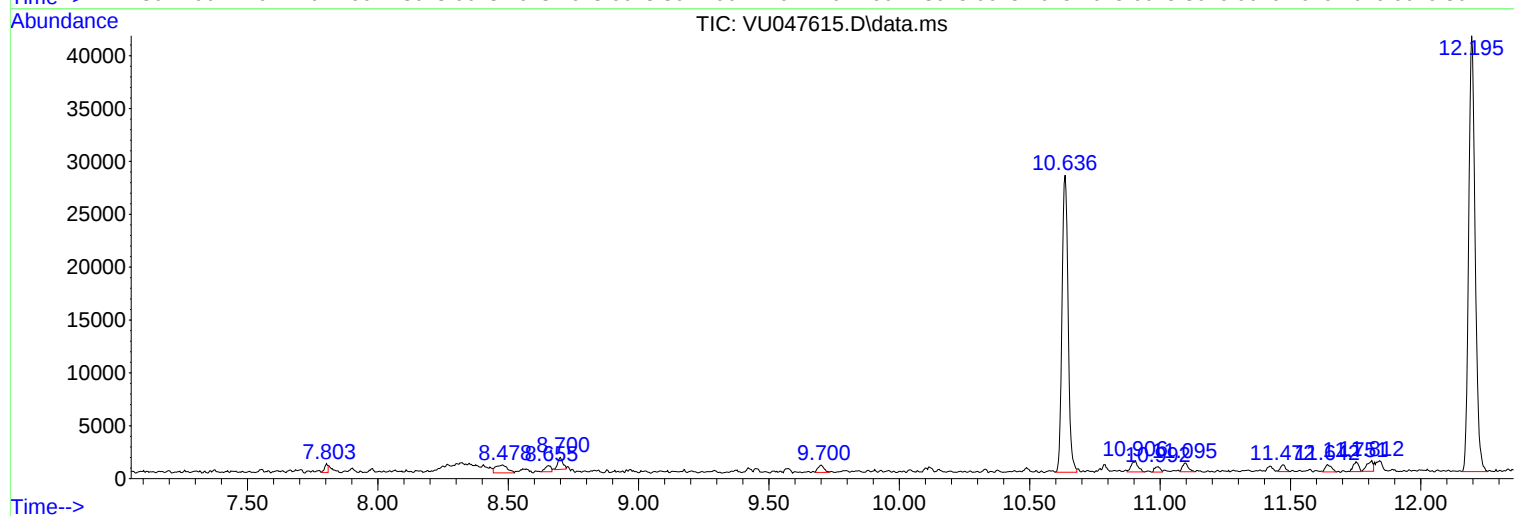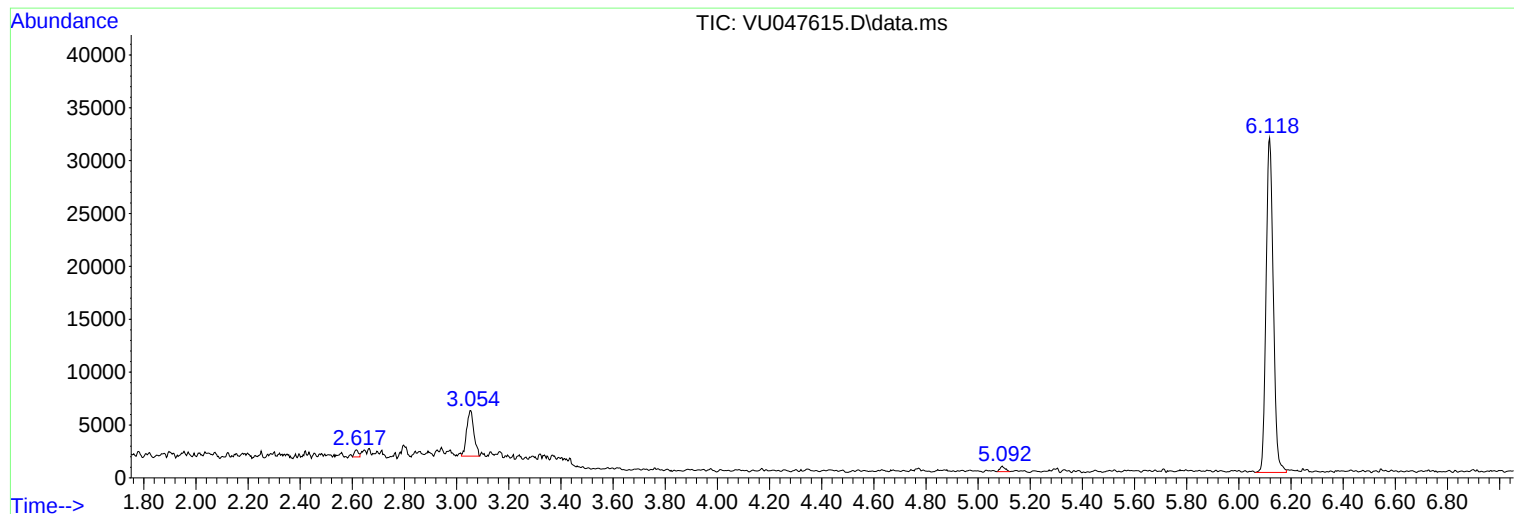

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
Data File : VU047615.D
Acq On : 18 Mar 2022 14:47
Operator : SY/MD
Sample : VU0318WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
Data File : VU047615.D
Acq On : 18 Mar 2022 14:47
Operator : SY/MD
Sample : VU0318WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0318WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------