


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031822\
 Data File : VU047607.D
 Acq On : 18 Mar 2022 09:16
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Mar 18 13:19:37 2022

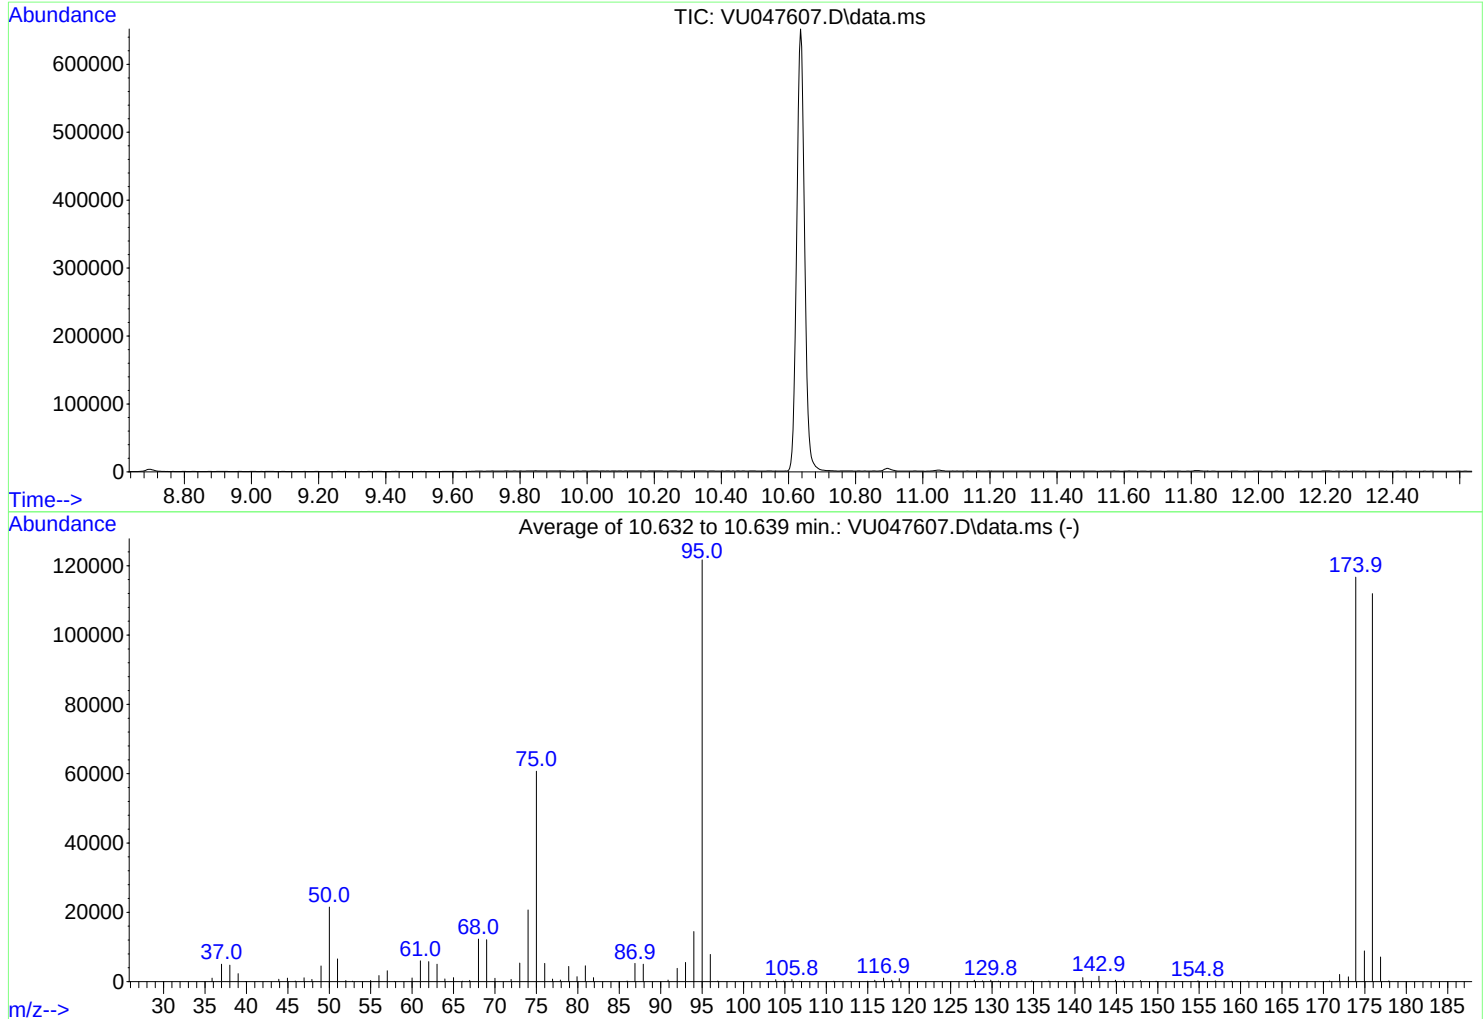

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	21539	PASS
75	95	30	60	49.9	60699	PASS
95	95	100	100	100.0	121709	PASS
96	95	5	9	6.5	7869	PASS
173	174	0.00	2	1.2	1376	PASS
174	95	50	100	95.9	116712	PASS
175	174	5	9	7.6	8853	PASS
176	174	95	101	95.9	111979	PASS
177	176	5	9	6.4	7113	PASS