

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031919\
 Data File : VU030196.D
 Acq On : 19 Mar 2019 16:00
 Operator : JC/SP
 Sample : K1918-21DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rBV2	11589	10830	0.48%	0.059%
2	1.399	89	96	112	rBV	305571	302465	13.28%	1.638%
3	1.679	174	183	198	rVB	209001	272439	11.97%	1.476%
4	1.884	243	247	254	rVB5	5261	5978	0.26%	0.032%
5	2.187	335	341	348	rBV3	6047	8318	0.37%	0.045%
6	2.270	356	367	380	rBV	476228	721300	31.68%	3.907%
7	2.447	413	422	430	rBV3	6346	13163	0.58%	0.071%
8	2.540	448	451	458	rVB3	1799	2079	0.09%	0.011%
9	2.572	458	461	464	rBV3	1129	919	0.04%	0.005%
10	2.688	491	497	498	rBV2	1076	928	0.04%	0.005%
11	2.839	538	544	548	rBV3	1175	1255	0.06%	0.007%
12	2.987	584	590	591	rBV2	1466	1339	0.06%	0.007%
13	3.058	607	612	615	rBV	1421	1402	0.06%	0.008%
14	3.212	656	660	664	rVB	1546	1210	0.05%	0.007%
15	3.277	677	680	684	rVB	1607	1223	0.05%	0.007%
16	3.302	684	688	691	rBV	1746	1413	0.06%	0.008%
17	3.383	710	713	719	rVV	1184	1077	0.05%	0.006%
18	3.588	773	777	781	rVV	1642	1745	0.08%	0.009%
19	3.633	787	791	796	rVB	1558	1518	0.07%	0.008%
20	3.669	796	802	805	rBV3	1052	1252	0.05%	0.007%
21	3.891	868	871	875	rVB	1503	1025	0.05%	0.006%
22	3.955	885	891	897	rVB	2168	3260	0.14%	0.018%
23	4.003	903	906	911	rVV	1158	1098	0.05%	0.006%
24	4.174	947	959	983	rBV	170520	442380	19.43%	2.396%
25	4.643	1087	1105	1128	rBV	319429	759718	33.37%	4.115%
26	4.900	1183	1185	1189	rVB	1989	1257	0.06%	0.007%
27	4.955	1199	1202	1203	rBV	1870	1034	0.05%	0.006%
28	5.338	1295	1321	1352	rBV2	667645	1977231	86.84%	10.709%
29	5.627	1406	1411	1415	rBV	1919	2179	0.10%	0.012%
30	5.884	1478	1491	1521	rBV	586004	1175411	51.62%	6.366%
31	6.167	1576	1579	1585	rBV	1921	1808	0.08%	0.010%
32	6.267	1607	1610	1614	rBV	1313	1013	0.04%	0.005%
33	6.328	1614	1629	1652	rBV	423502	853167	37.47%	4.621%
34	6.508	1681	1685	1691	rBV	1292	1646	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031919\
 Data File : VU030196.D
 Acq On : 19 Mar 2019 16:00
 Operator : JC/SP
 Sample : K1918-21DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.649	1725	1729	1733	rBV	1125	1066	0.05%	0.006%
36	6.707	1744	1747	1751	rVB	1322	972	0.04%	0.005%
37	6.826	1779	1784	1786	rBV	1302	1138	0.05%	0.006%
38	6.878	1796	1800	1805	rBV	1320	1228	0.05%	0.007%
39	6.926	1812	1815	1819	rVB2	1272	1066	0.05%	0.006%
40	6.952	1819	1823	1826	rBV	1631	1227	0.05%	0.007%
41	7.006	1836	1840	1843	rBV	2350	1795	0.08%	0.010%
42	7.225	1897	1908	1932	rBV	244666	435637	19.13%	2.359%
43	7.399	1959	1962	1968	rBV	1489	1253	0.06%	0.007%
44	7.463	1976	1982	1984	rBV2	1736	1906	0.08%	0.010%
45	7.563	2000	2013	2032	rBV	932287	1633604	71.75%	8.848%
46	7.845	2091	2101	2124	rVV	164389	290040	12.74%	1.571%
47	8.109	2178	2183	2187	rVB	1576	1771	0.08%	0.010%
48	8.135	2187	2191	2193	rBV2	1418	992	0.04%	0.005%
49	8.177	2194	2204	2213	rBV2	6975	11982	0.53%	0.065%
50	8.225	2213	2219	2223	rBV5	2100	2569	0.11%	0.014%
51	8.308	2232	2245	2284	rBV	592127	1062802	46.68%	5.756%
52	8.534	2312	2315	2326	rBV3	1519	2565	0.11%	0.014%
53	8.640	2344	2348	2350	rBV	1610	1020	0.04%	0.006%
54	8.656	2350	2353	2356	rBV	1278	1005	0.04%	0.005%
55	8.807	2398	2400	2406	rVB2	1343	1107	0.05%	0.006%
56	8.842	2406	2411	2414	rBV2	1055	1195	0.05%	0.006%
57	8.900	2424	2429	2434	rVB	1389	1570	0.07%	0.009%
58	8.958	2444	2447	2453	rVB	1229	1022	0.04%	0.006%
59	8.993	2453	2458	2461	rBV	1098	1214	0.05%	0.007%
60	9.087	2475	2487	2516	rBV2	877389	1665143	73.13%	9.019%
61	9.553	2629	2632	2636	rBV	1609	1265	0.06%	0.007%
62	9.749	2689	2693	2696	rBV	1418	1209	0.05%	0.007%
63	9.935	2747	2751	2755	rVB2	1714	1624	0.07%	0.009%
64	10.051	2783	2787	2790	rBV	1525	1065	0.05%	0.006%
65	10.427	2892	2904	2927	rBV	632343	1020513	44.82%	5.527%
66	10.659	2973	2976	2980	rBV	1176	1290	0.06%	0.007%
67	10.704	2984	2990	2994	rBV2	2032	2470	0.11%	0.013%
68	11.112	3113	3117	3122	rBV	1607	1747	0.08%	0.009%
69	11.260	3159	3163	3168	rVB2	1857	1757	0.08%	0.010%
70	11.414	3199	3211	3221	rBV	225577	355302	15.60%	1.924%
71	11.482	3221	3232	3262	rVB2	935874	2276953	100.00%	12.332%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031919\
 Data File : VU030196.D
 Acq On : 19 Mar 2019 16:00
 Operator : JC/SP
 Sample : K1918-21DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.749	3311	3315	3318	rBV	1485	1161	0.05%	0.006%
73	11.858	3333	3349	3382	rBV2	954823	1845519	81.05%	9.996%
74	12.160	3437	3443	3446	rBV3	1229	1615	0.07%	0.009%
75	12.395	3513	3516	3522	rVB	1637	1600	0.07%	0.009%
76	12.530	3552	3558	3561	rBV	1274	1443	0.06%	0.008%
77	12.646	3583	3594	3605	rBV7	5345	12453	0.55%	0.067%
78	12.800	3637	3642	3643	rBV2	1893	1688	0.07%	0.009%
79	12.890	3664	3670	3680	rVB4	7608	13033	0.57%	0.071%
80	12.942	3680	3686	3691	rBV	1916	2608	0.11%	0.014%
81	12.971	3691	3695	3698	rVB	1280	953	0.04%	0.005%
82	12.996	3698	3703	3707	rBV4	1275	1440	0.06%	0.008%
83	13.340	3806	3810	3815	rVB	1712	1811	0.08%	0.010%
84	13.498	3848	3859	3892	rBV	624645	1093024	48.00%	5.920%
85	13.746	3930	3936	3944	rBV4	3584	6140	0.27%	0.033%
86	13.987	4001	4011	4024	rBV2	50856	93798	4.12%	0.508%
87	14.176	4068	4070	4076	rBV	1271	926	0.04%	0.005%
88	14.389	4133	4136	4142	rBV	1297	1234	0.05%	0.007%
89	14.524	4175	4178	4181	rBV	1600	950	0.04%	0.005%
90	14.543	4181	4184	4187	rBV	1674	1387	0.06%	0.008%
91	14.585	4194	4197	4201	rVB2	1737	1185	0.05%	0.006%
92	14.607	4201	4204	4209	rBV	1692	1793	0.08%	0.010%
93	14.717	4235	4238	4242	rBV	1692	1553	0.07%	0.008%
94	14.797	4261	4263	4266	rVB	2256	1143	0.05%	0.006%
95	14.868	4281	4285	4289	rBV	2197	2118	0.09%	0.011%
96	15.080	4348	4351	4354	rBV2	1883	1178	0.05%	0.006%
97	15.154	4371	4374	4378	rBV3	1447	962	0.04%	0.005%
98	15.591	4506	4510	4512	rBV3	1616	1321	0.06%	0.007%
99	15.745	4555	4558	4561	rBV	1526	1119	0.05%	0.006%
100	15.835	4580	4586	4588	rBV	1797	2067	0.09%	0.011%


Sum of corrected areas: 18463386

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031919\
Data File : VU030196.D
Acq On : 19 Mar 2019 16:00
Operator : JC/SP
Sample : K1918-21DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

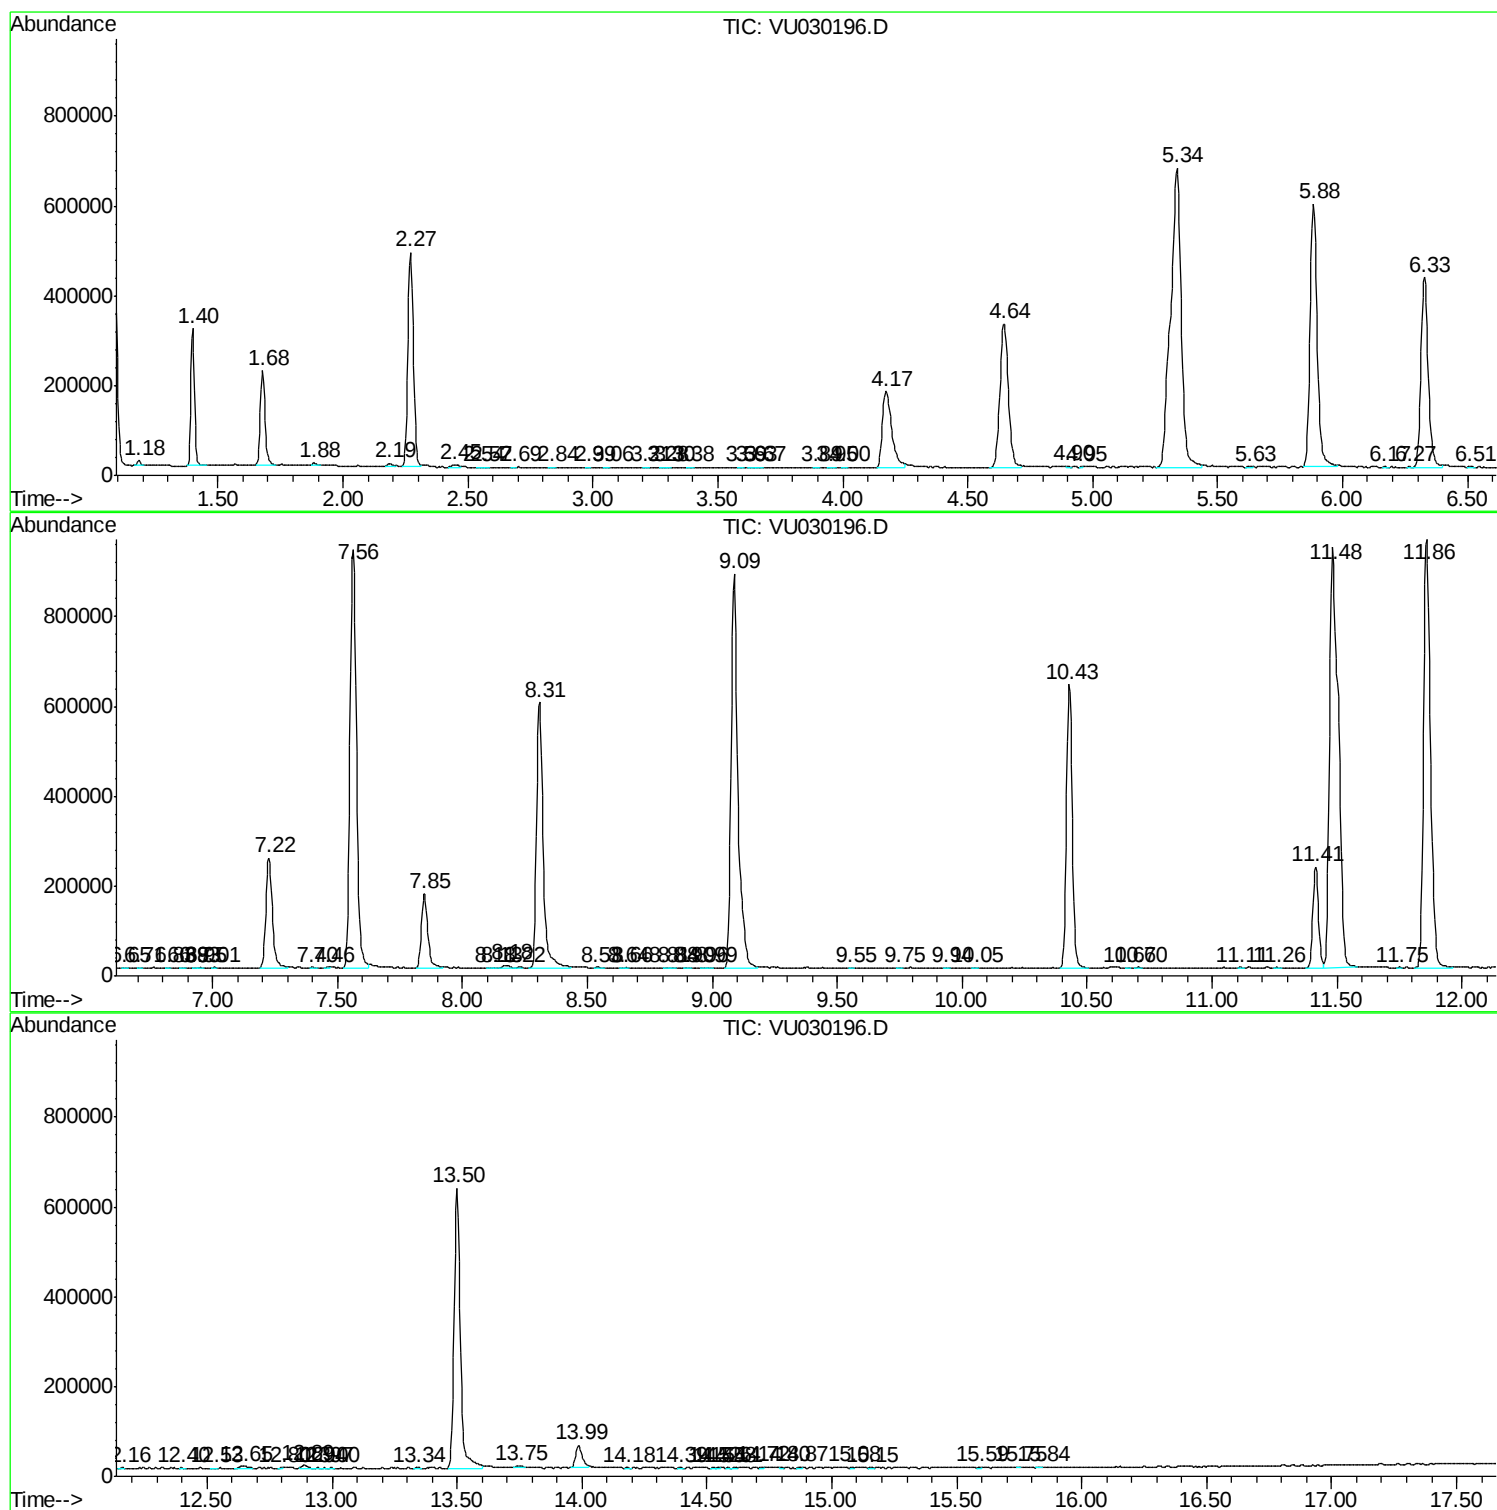

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031919\
Data File : VU030196.D
Acq On : 19 Mar 2019 16:00
Operator : JC/SP
Sample : K1918-21DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031919\
Data File : VU030196.D
Acq On : 19 Mar 2019 16:00
Operator : JC/SP
Sample : K1918-21DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc