

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042712.D
 Acq On : 19 Mar 2021 11:04
 Operator : SY/MD
 Sample : VU0319WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK29

Quant Time: Mar 20 05:43:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 16 01:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	78756	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	78822	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	38269	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	27620	5.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.20%
7) Chloroethane-d5	1.919	69	25244	6.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	127.00%
11) 1,1-Dichloroethene-d2	2.568	63	50267	4.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.80%
20) 2-Butanone-d5	4.652	46	76705	44.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.00%
24) Chloroform-d	5.073	84	52890	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.713	65	33675	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.735	84	98493	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.700	67	31364	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.906	98	89718	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloroprop...	8.185	79	12140	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.655	63	64602	46.32	ug/L	0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.64%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	26388	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	36197	5.22	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.40%
Target Compounds						Qvalue
16) Methylene chloride	3.060	84	1233	0.19	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042712.D
Acq On : 19 Mar 2021 11:04
Operator : SY/MD
Sample : VU0319WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK29


Quant Time: Mar 20 05:43:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 16 01:32:07 2021
Response via : Initial Calibration

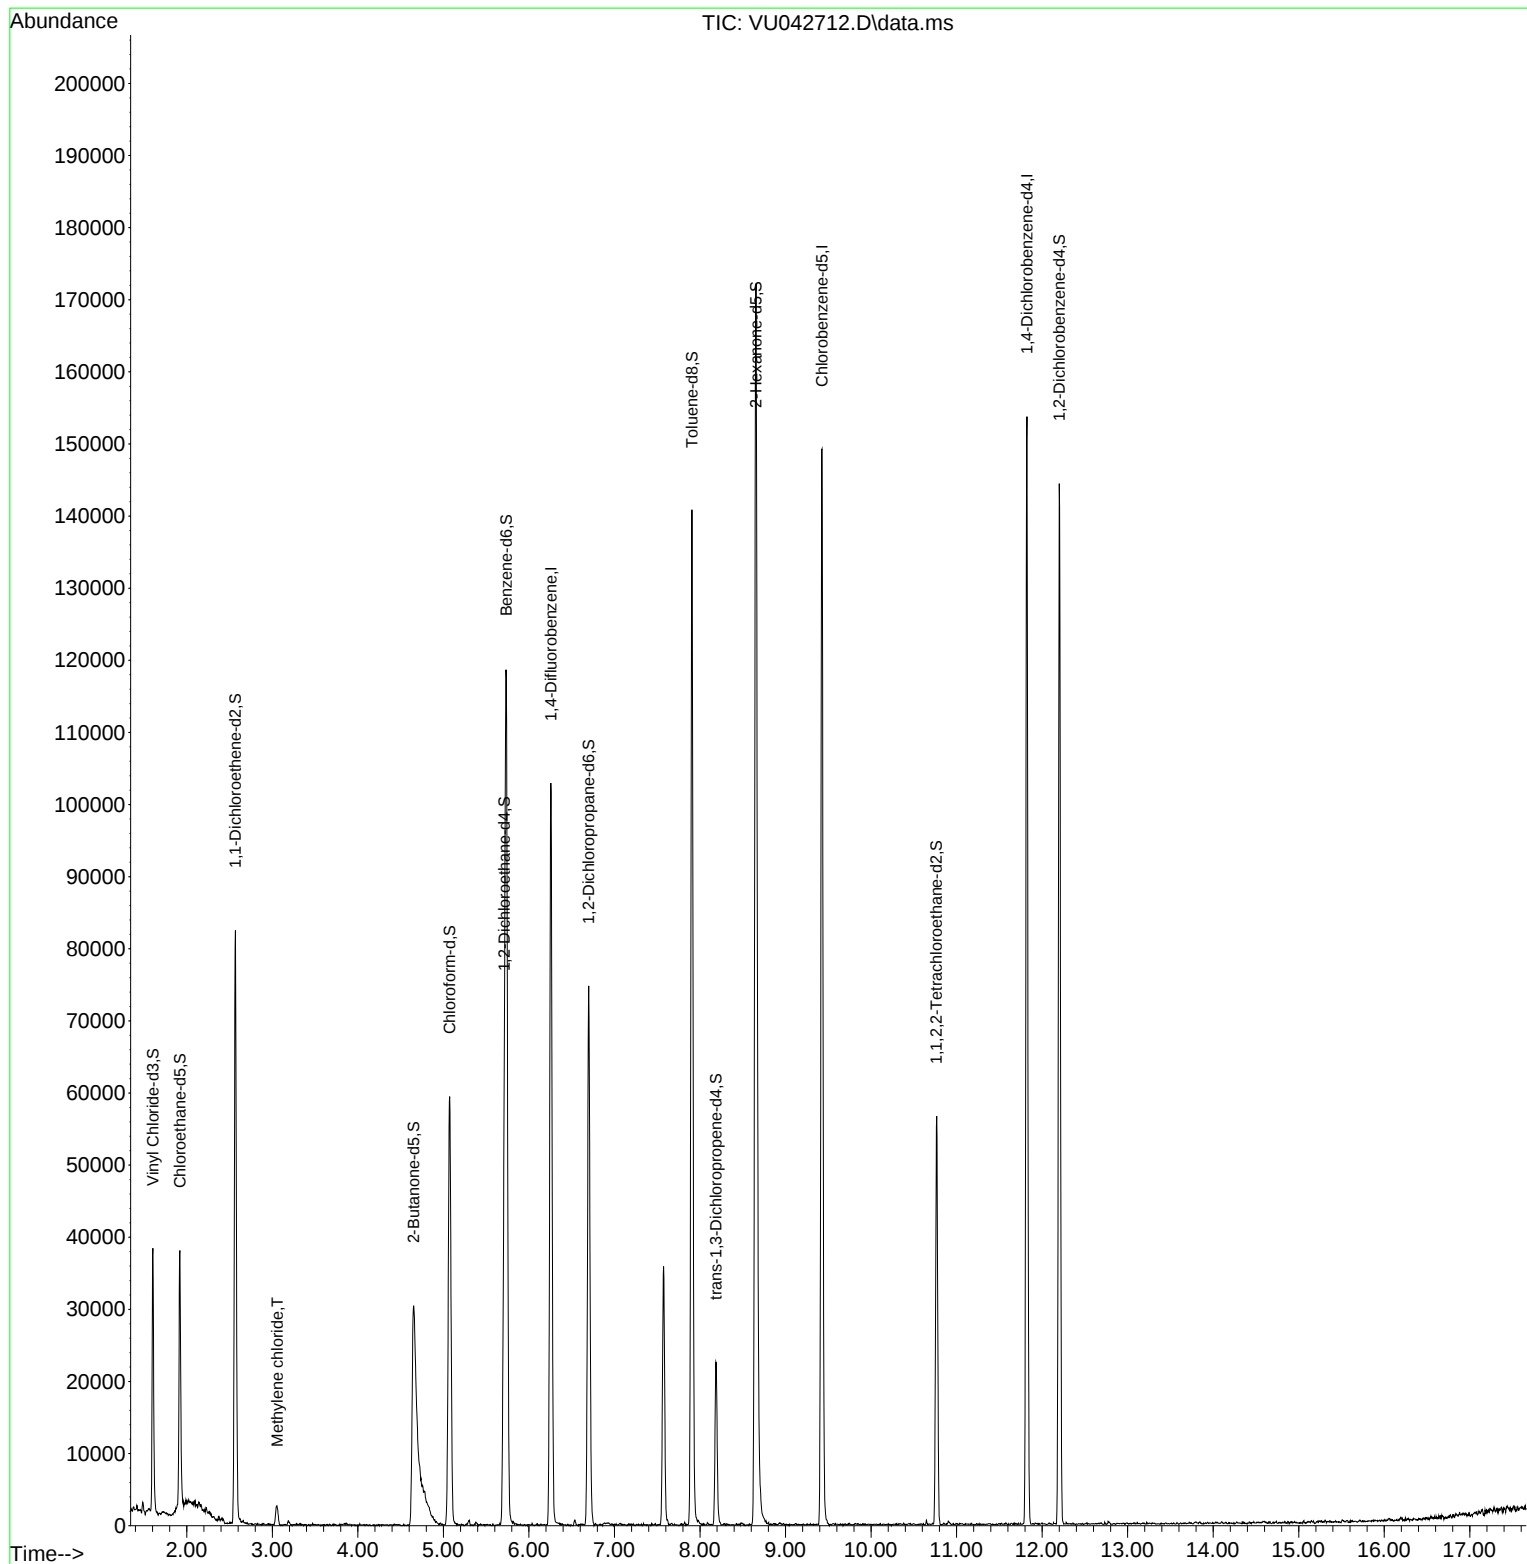

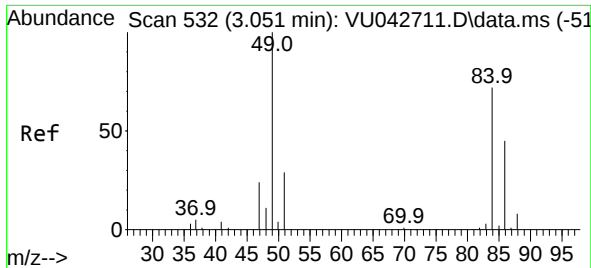

#16
Methylene chloride
Concen: 0.19 ug/L
RT: 3.060 min Scan# 535
Delta R.T. 0.006 min
Lab File: VU042712.D
Acq: 19 Mar 2021 11:04

Instrument :
MSVOA_U
ClientSampleId :
VBLK29

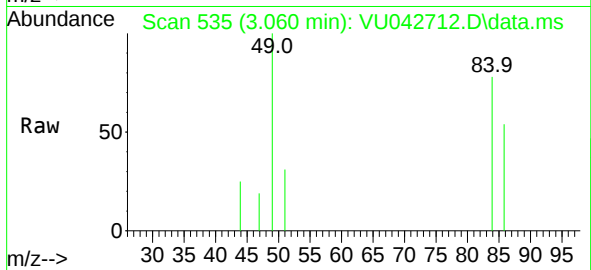

Tgt Ion:	84	Resp:	1233
Ion	Ratio	Lower	Upper
84	100		
86	69.3	44.1	81.9
49	127.9	95.0	176.4

