

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042717.D
 Acq On : 19 Mar 2021 13:49
 Operator : SY/MD
 Sample : M1699-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Mar 20 05:49:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 20 05:47:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	71298	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	72014	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	34743	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	26582	5.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.80%
7) Chloroethane-d5	1.919	69	21221	5.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.00%
11) 1,1-Dichloroethene-d2	2.575	63	44194	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	4.652	46	61280	39.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.54%
24) Chloroform-d	5.073	84	50367	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
26) 1,2-Dichloroethane-d4	5.710	65	31095	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
32) Benzene-d6	5.735	84	92385	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
36) 1,2-Dichloropropane-d6	6.700	67	29470	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.906	98	84239	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
43) trans-1,3-Dichloroprop...	8.189	79	11860	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.648	63	60497	47.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.96%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	25735	5.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.40%
64) 1,2-Dichlorobenzene-d4	12.201	152	33918	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%
Target Compounds						
16) Methylene chloride	3.050	84	1206	0.20	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042717.D
Acq On : 19 Mar 2021 13:49
Operator : SY/MD
Sample : M1699-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Mar 20 05:49:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 20 05:47:33 2021
Response via : Initial Calibration

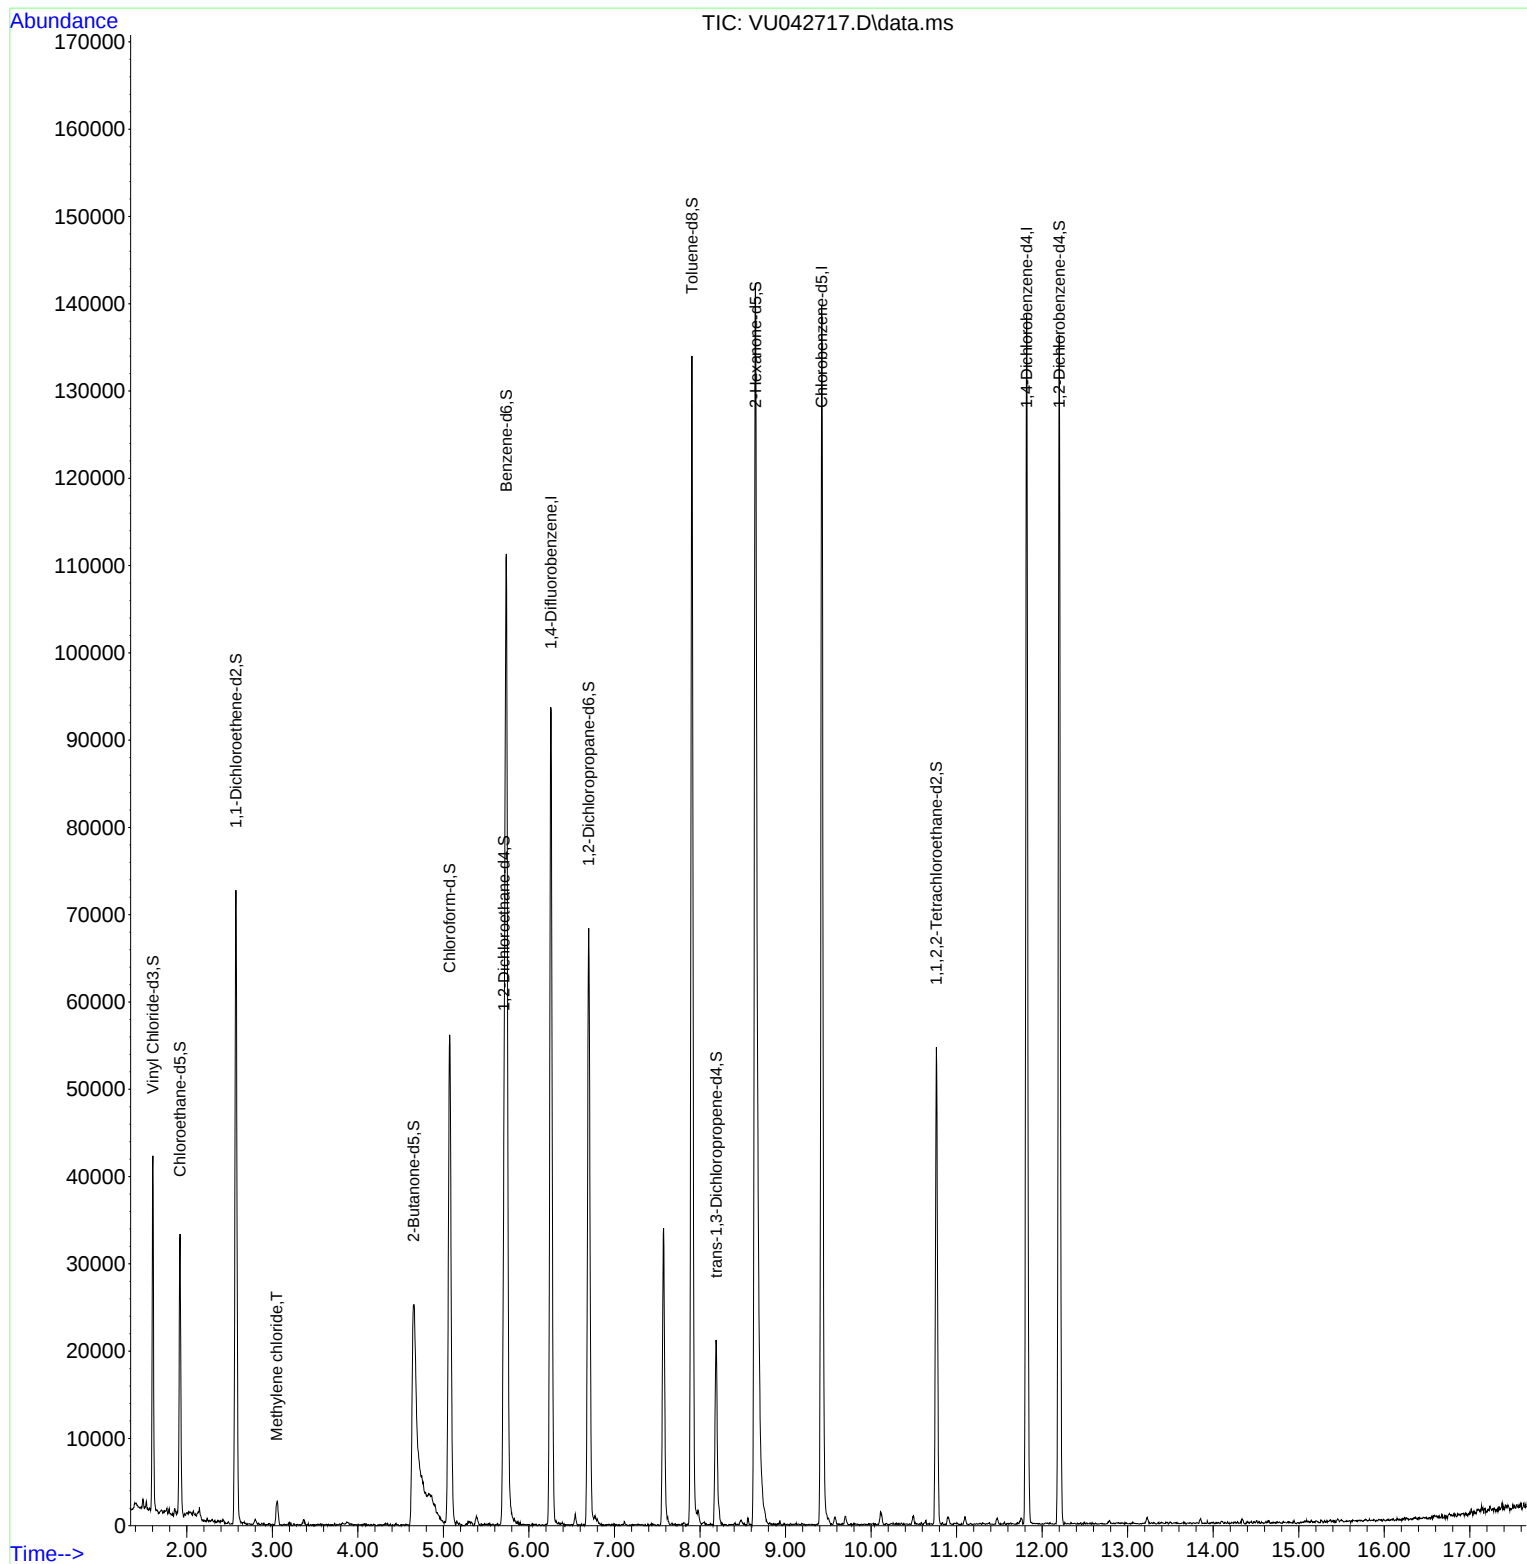

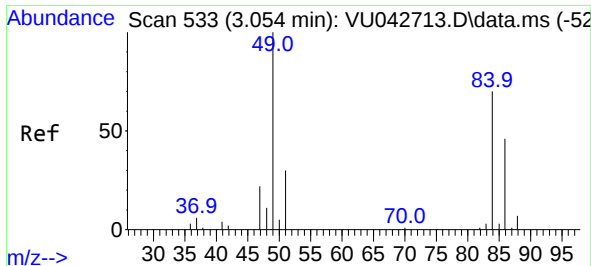

#16
Methylene chloride
Concen: 0.20 ug/L
RT: 3.050 min Scan# 532
Delta R.T. -0.003 min
Lab File: VU042717.D
Acq: 19 Mar 2021 13:49

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Tgt Ion: 84 Resp: 1206
Ion Ratio Lower Upper
84 100
86 46.6 44.1 81.9
49 120.2 95.0 176.4

