

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042718.D
 Acq On : 19 Mar 2021 14:14
 Operator : SY/MD
 Sample : M1744-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZF2

Quant Time: Mar 20 05:49:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 20 05:47:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	73307	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	74846	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	36187	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24970	5.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.20%
7) Chloroethane-d5	1.919	69	20708	5.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.00%
11) 1,1-Dichloroethene-d2	2.575	63	42404	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.80%
20) 2-Butanone-d5	4.652	46	64590	40.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.50%
24) Chloroform-d	5.073	84	49495	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.713	65	31256	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.20%
32) Benzene-d6	5.735	84	88724	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.700	67	29624	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.906	98	80874	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloroprop...	8.189	79	11047	3.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.80%
46) 2-Hexanone-d5	8.648	63	58681	44.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.62%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	24278	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	32396	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%
Target Compounds						
22) cis-1,2-Dichloroethene	4.677	96	1307	0.23	ug/L	Qvalue 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042718.D
Acq On : 19 Mar 2021 14:14
Operator : SY/MD
Sample : M1744-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZF2


Quant Time: Mar 20 05:49:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 20 05:47:33 2021
Response via : Initial Calibration

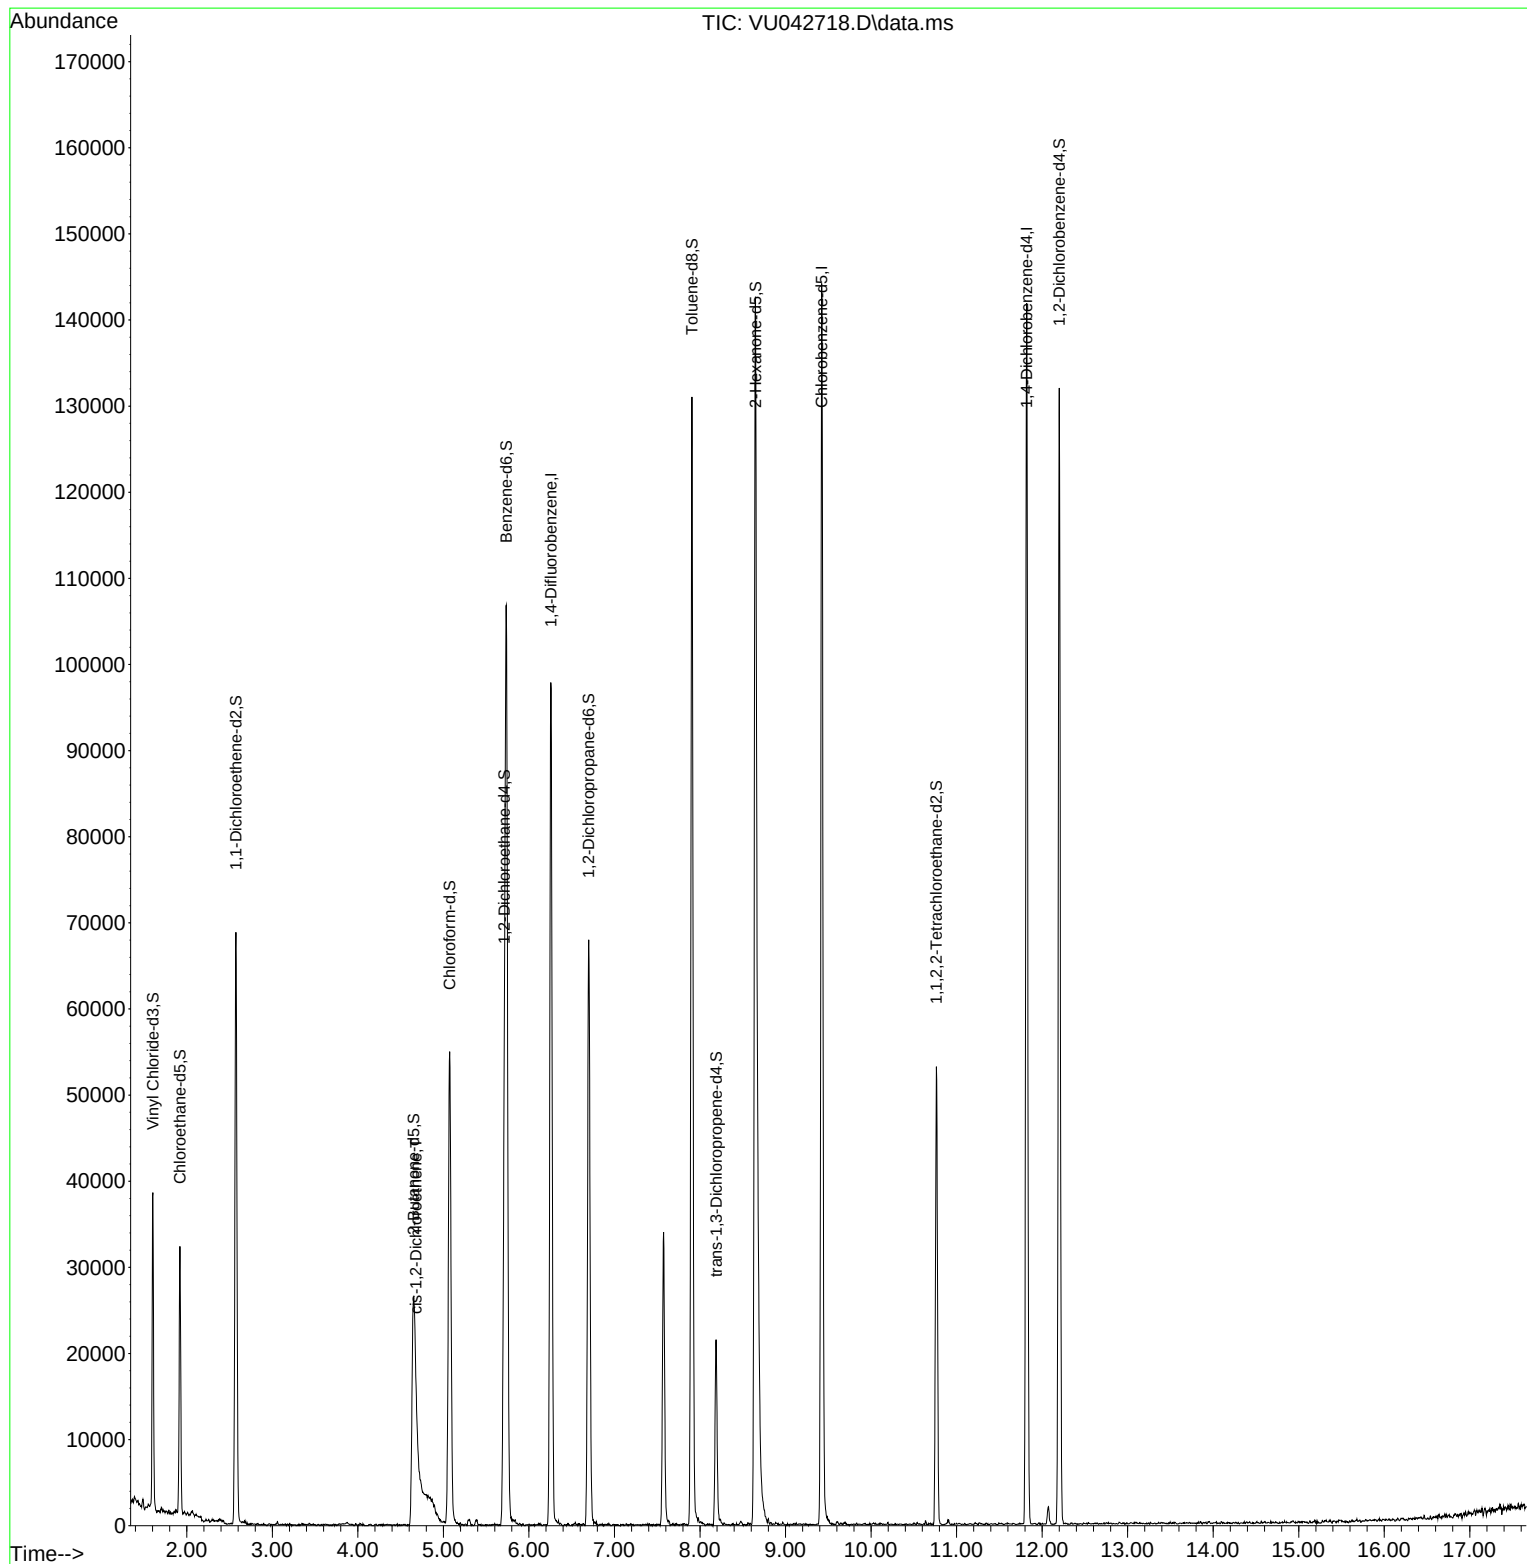

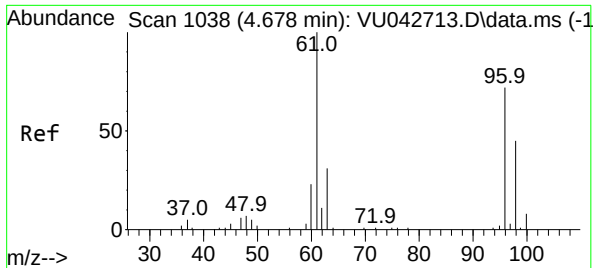

#22
 cis-1,2-Dichloroethene
 Concen: 0.23 ug/L
 RT: 4.677 min Scan# 1038
 Delta R.T. -0.000 min
 Lab File: VU042718.D
 Acq: 19 Mar 2021 14:14

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZF2

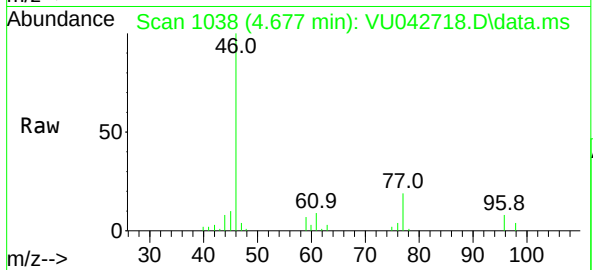

Tgt Ion:	96	Resp:	1307
Ion	Ratio	Lower	Upper
96	100		
61	111.9	97.8	181.6
68	0.0	0.0	0.0

