

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042719.D
 Acq On : 19 Mar 2021 14:38
 Operator : SY/MD
 Sample : M1744-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZF3

Quant Time: Mar 20 05:50:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 20 05:47:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	70009	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	70183	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	33343	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	25626	5.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.80%
7) Chloroethane-d5	1.919	69	20401	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.40%
11) 1,1-Dichloroethene-d2	2.575	63	41826	3.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.40%
20) 2-Butanone-d5	4.655	46	55560	36.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.52%
24) Chloroform-d	5.073	84	48911	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	5.713	65	30989	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.735	84	87441	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.700	67	28319	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.906	98	80331	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
43) trans-1,3-Dichloroprop...	8.185	79	11293	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.645	63	57705	46.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.94%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	24376	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	32397	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%
Target Compounds					Qvalue	
42) Toluene	7.976	91	9009	0.38	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042719.D
Acq On : 19 Mar 2021 14:38
Operator : SY/MD
Sample : M1744-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZF3

Quant Time: Mar 20 05:50:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 20 05:47:33 2021
Response via : Initial Calibration

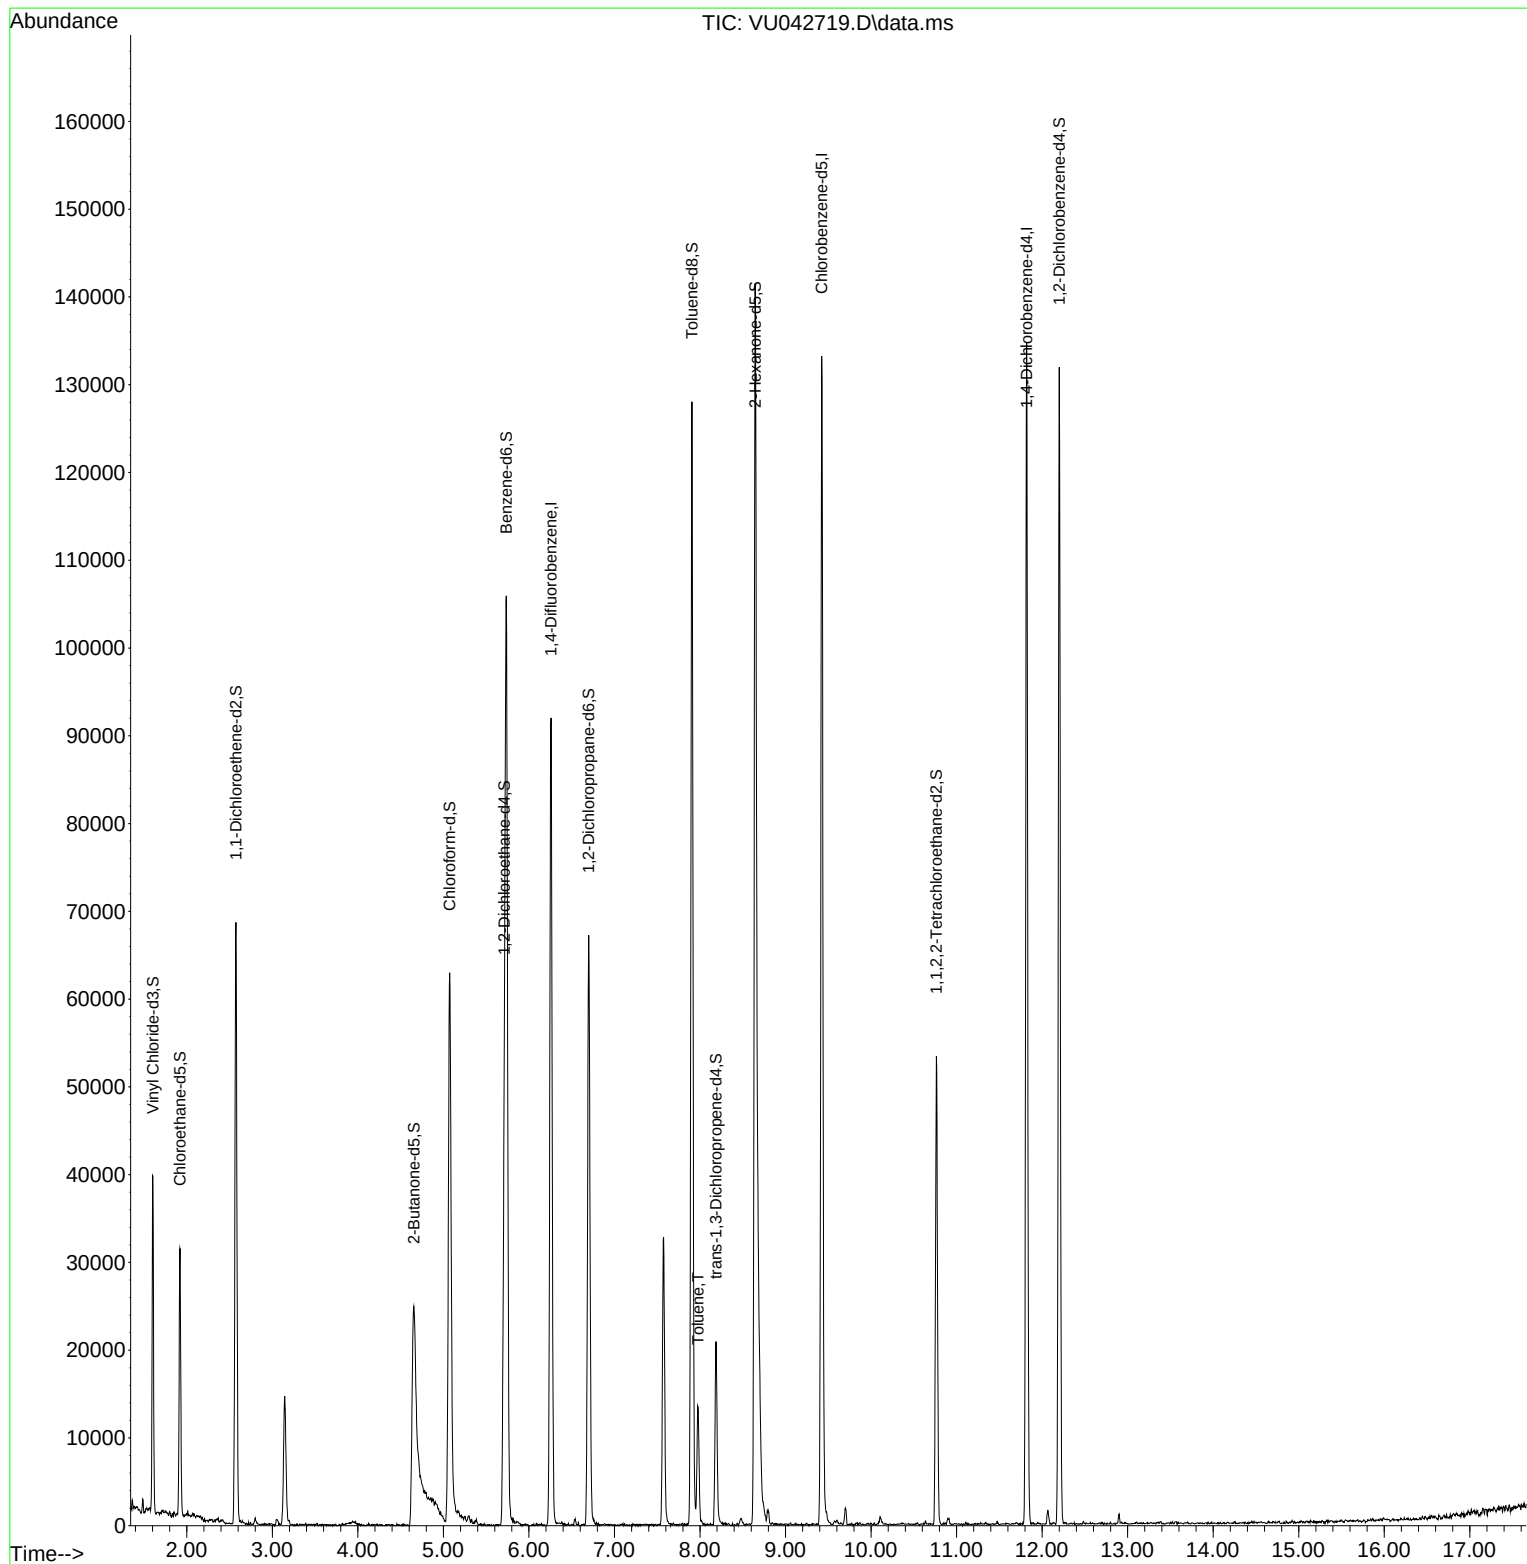

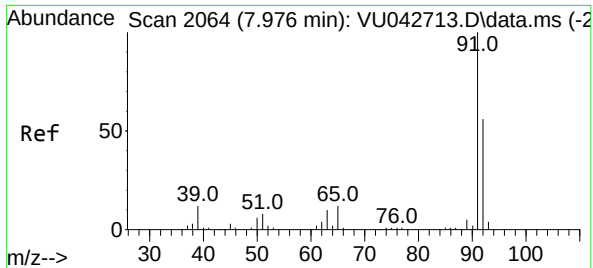

#42
Toluene
Concen: 0.38 ug/L
RT: 7.976 min Scan# 2064
Delta R.T. -0.000 min
Lab File: VU042719.D
Acq: 19 Mar 2021 14:38

Instrument :
MSVOA_U
ClientSampleId :
ETZF3

Tgt Ion: 91 Resp: 9009
Ion Ratio Lower Upper
91 100
92 56.4 41.2 76.6

