

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042722.D
 Acq On : 19 Mar 2021 15:48
 Operator : SY/MD
 Sample : M1743-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZD2

Quant Time: Mar 20 05:51:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 20 05:47:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	76830	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	78534	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	36950	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	7056	1.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	27.60%#
7) Chloroethane-d5	1.919	69	8747	2.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	45.20%#
11) 1,1-Dichloroethene-d2	2.575	63	10305	0.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	17.80%#
20) 2-Butanone-d5	4.645	46	84528	50.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.52%
24) Chloroform-d	5.073	84	29340	2.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	58.00%#
26) 1,2-Dichloroethane-d4	5.713	65	18744	3.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.20%#
32) Benzene-d6	5.735	84	36020	1.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	37.40%#
36) 1,2-Dichloropropane-d6	6.700	67	15560	2.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	50.20%#
41) Toluene-d8	7.906	98	25283	1.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	26.80%#
43) trans-1,3-Dichloroprop...	8.189	79	5772	1.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	39.80%#
46) 2-Hexanone-d5	8.645	63	52998	38.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.28%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	20989	3.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.80%
64) 1,2-Dichlorobenzene-d4	12.201	152	19311	2.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	57.60%#
Target Compounds						Qvalue
47) Tetrachloroethene	8.562	164	3782	0.68	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042722.D
Acq On : 19 Mar 2021 15:48
Operator : SY/MD
Sample : M1743-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZD2


Quant Time: Mar 20 05:51:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 20 05:47:33 2021
Response via : Initial Calibration

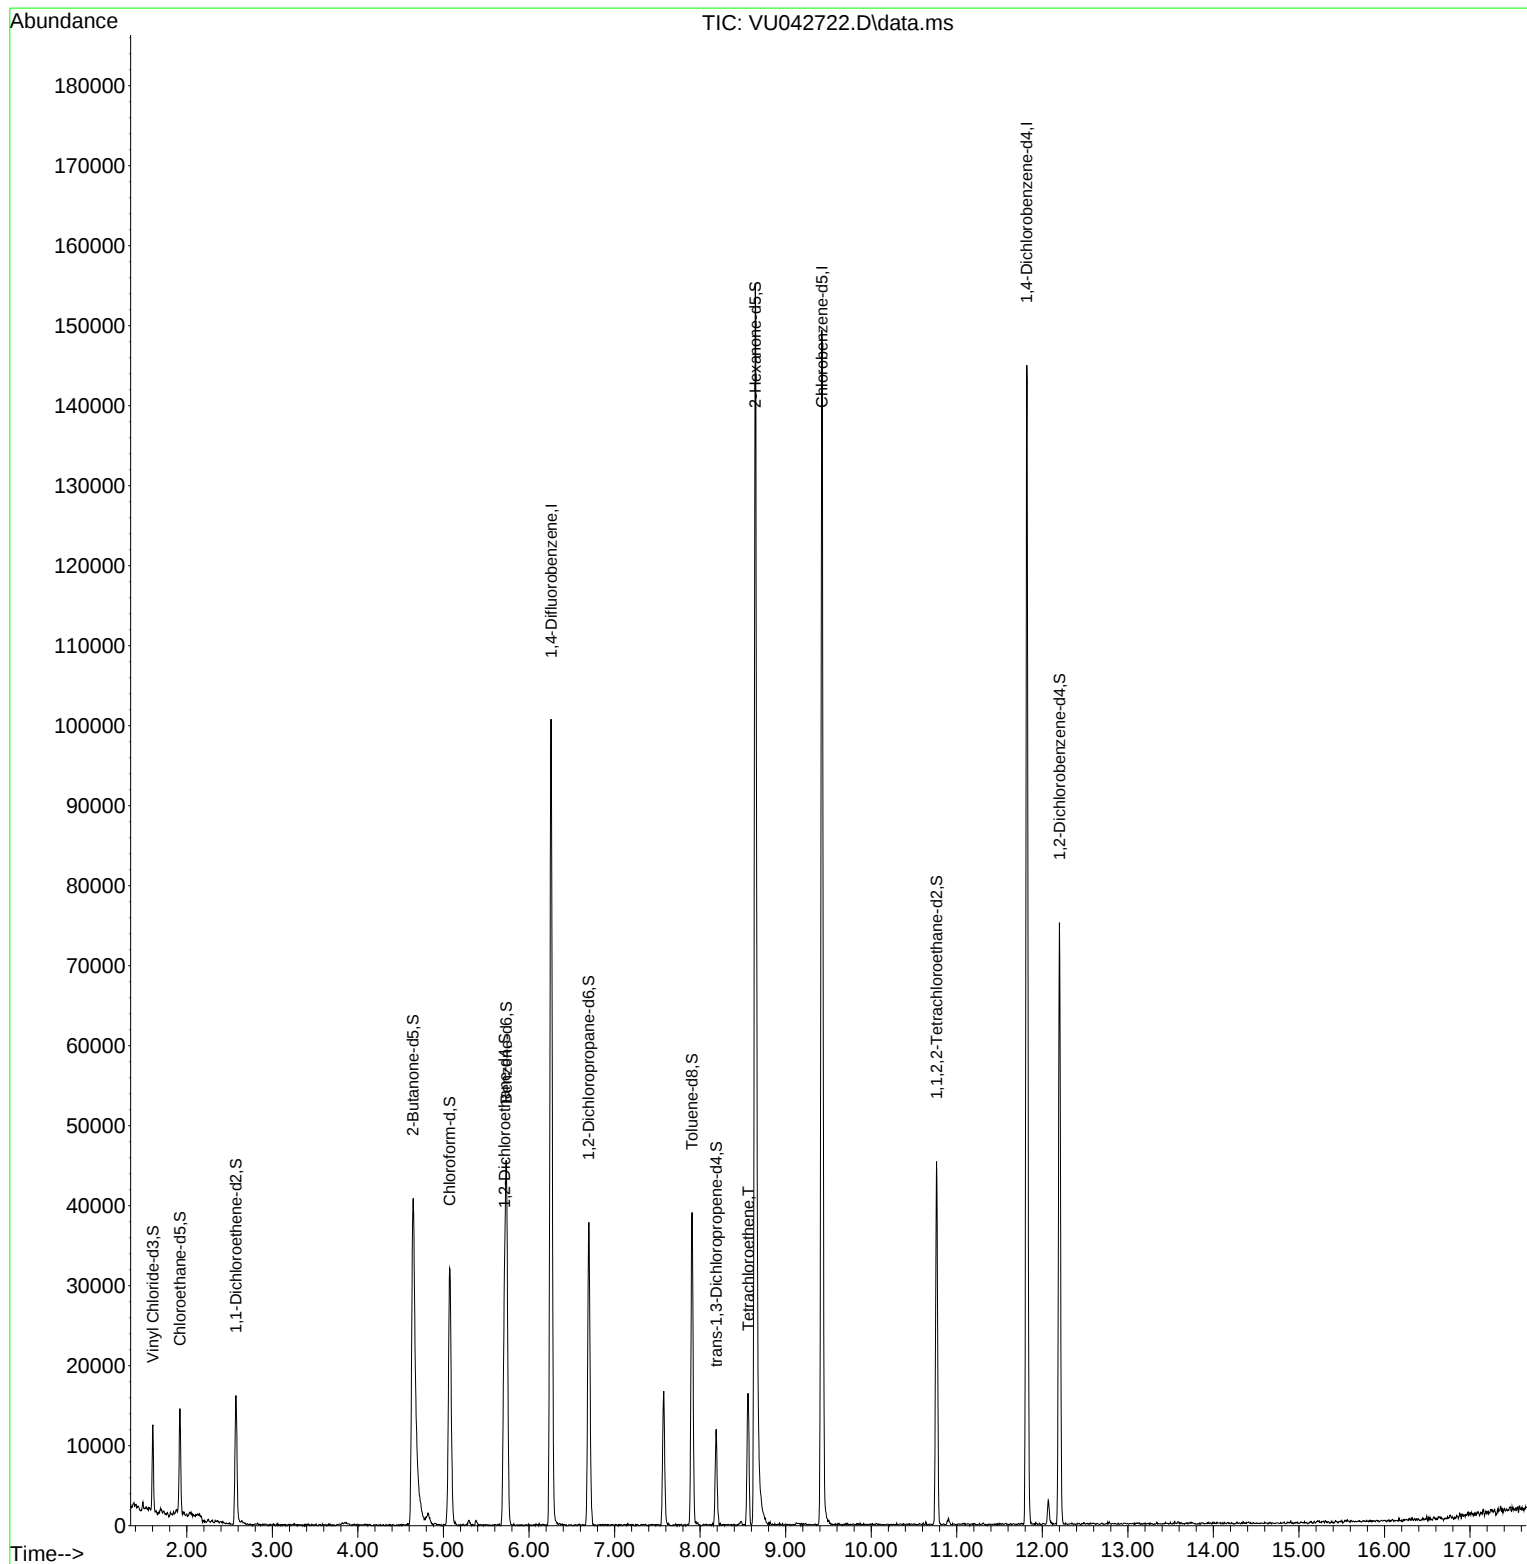

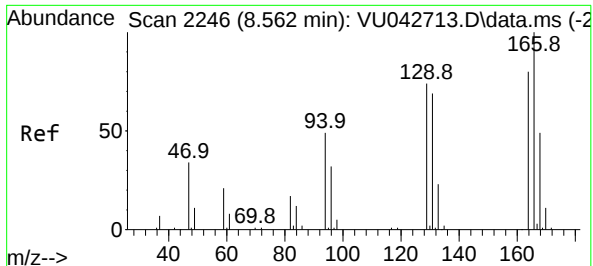

#47
 Tetrachloroethene
 Concen: 0.68 ug/L
 RT: 8.562 min Scan# 2246
 Delta R.T. 0.000 min
 Lab File: VU042722.D
 Acq: 19 Mar 2021 15:48

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZD2

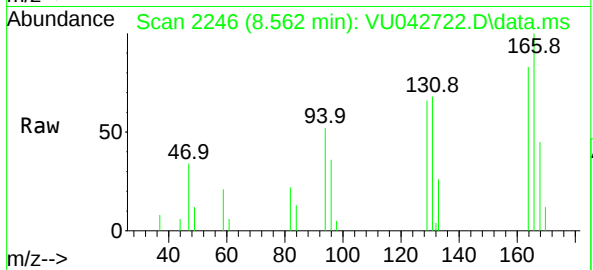

Tgt Ion:	164	Resp:	3782
Ion	Ratio	Lower	Upper
164	100		
129	79.0	64.3	119.5
131	81.3	62.2	115.6
166	119.9	88.6	164.6

