

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042736.D
 Acq On : 19 Mar 2021 22:02
 Operator : SY/MD
 Sample : M1743-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZE1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC: VU042736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	91	rVB	35280	40333	12.09%	1.485%
2	1.919	172	180	191	rVB	28496	36147	10.83%	1.331%
3	2.575	373	384	399	rBV	64347	104611	31.36%	3.851%
4	4.649	1015	1029	1051	rBV2	26753	94460	28.31%	3.478%
5	5.073	1144	1161	1180	rBV2	52082	115090	34.50%	4.237%
6	5.735	1345	1367	1380	rBV2	103271	268839	80.58%	9.898%
7	5.803	1380	1388	1405	rVB2	19801	40088	12.02%	1.476%
8	6.256	1516	1529	1545	rBV	94339	179414	53.78%	6.605%
9	6.549	1611	1620	1631	rBB4	9840	17033	5.11%	0.627%
10	6.700	1652	1667	1682	rBV2	64774	125944	37.75%	4.637%
11	7.575	1928	1939	1957	rBV	31692	55933	16.77%	2.059%
12	7.906	2030	2042	2059	rBV	121915	210149	62.99%	7.737%
13	8.189	2119	2130	2145	rBV	20673	34804	10.43%	1.281%
14	8.559	2233	2245	2259	rBV	192222	321483	96.36%	11.836%
15	8.645	2259	2272	2309	rVB	143832	333623	100.00%	12.283%
16	9.423	2502	2514	2531	rBV	138853	233708	70.05%	8.604%
17	10.764	2918	2931	2946	rBV	50090	82582	24.75%	3.040%
18	11.819	3247	3259	3275	rVB	135511	218233	65.41%	8.035%
19	12.070	3329	3337	3347	rBV5	2376	3868	1.16%	0.142%
20	12.201	3365	3378	3391	rBV	124387	199837	59.90%	7.357%




Sum of corrected areas: 2716179

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042736.D
Acq On : 19 Mar 2021 22:02
Operator : SY/MD
Sample : M1743-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

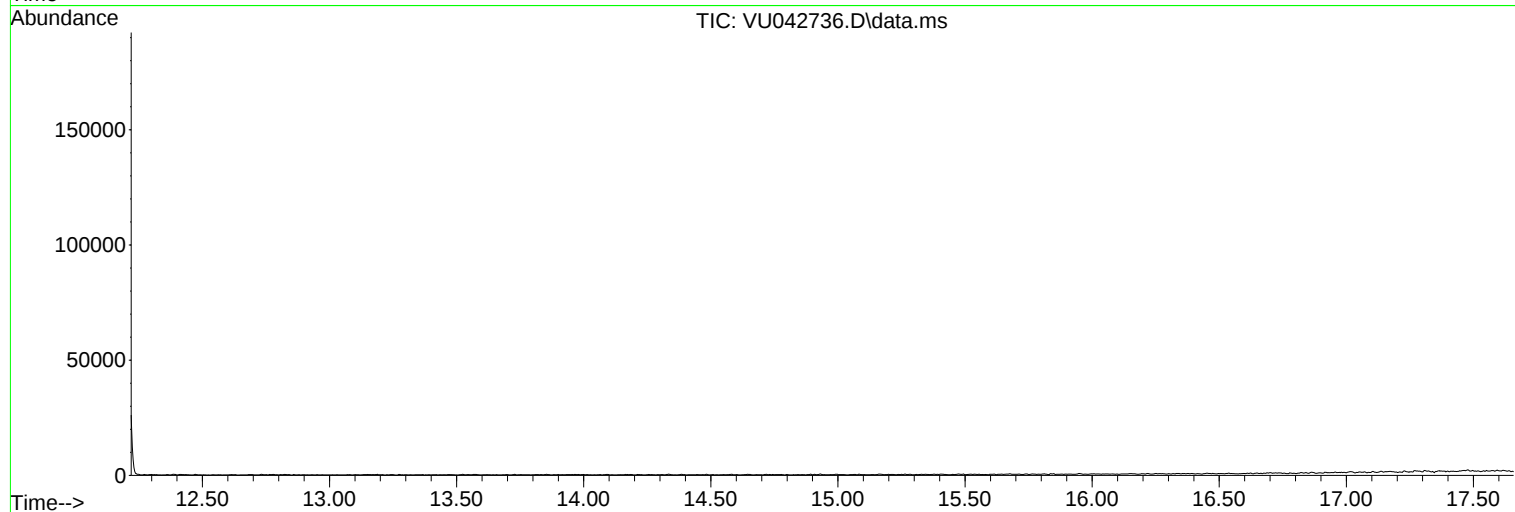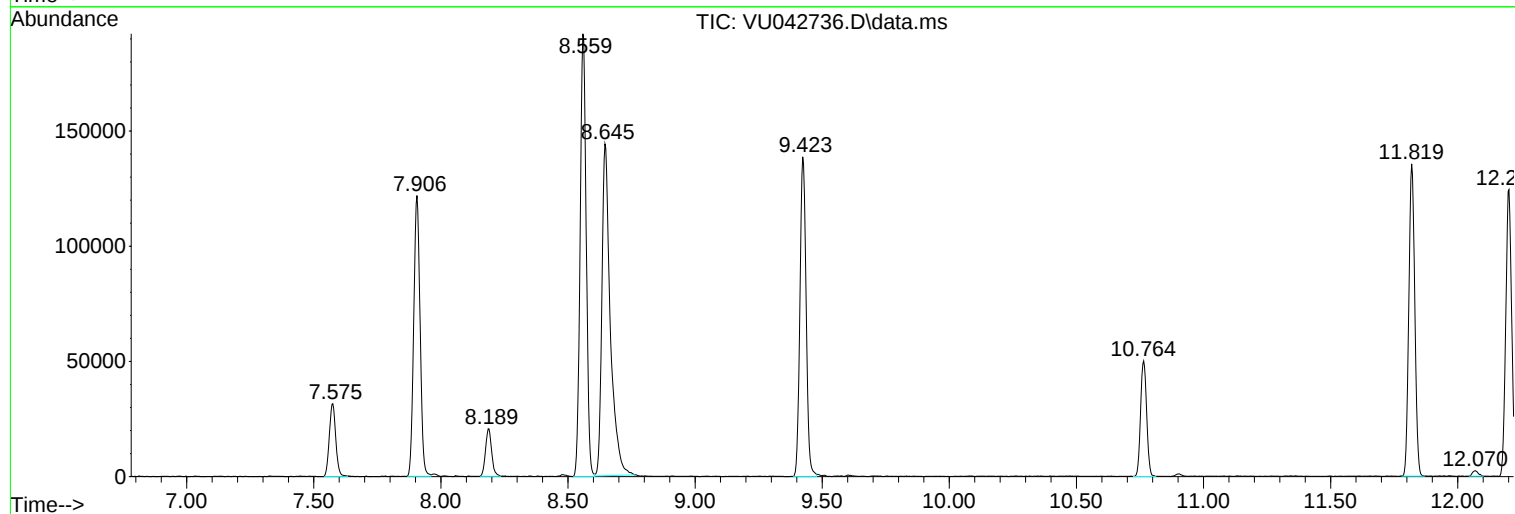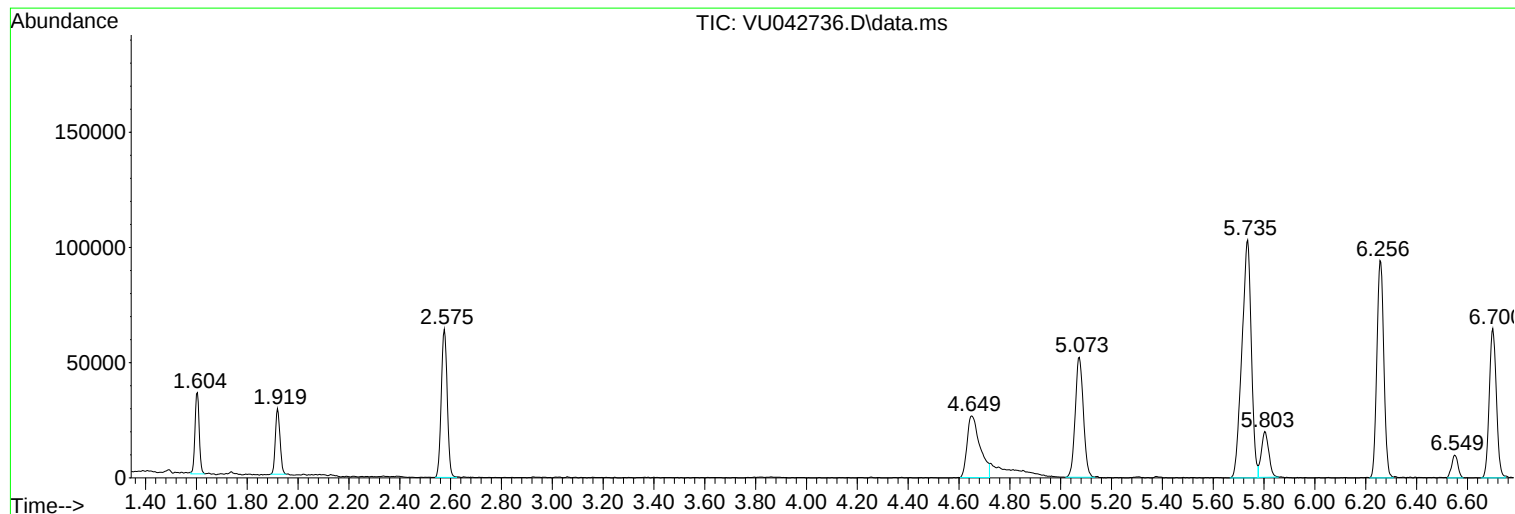

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042736.D
Acq On : 19 Mar 2021 22:02
Operator : SY/MD
Sample : M1743-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042736.D
Acq On : 19 Mar 2021 22:02
Operator : SY/MD
Sample : M1743-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
