

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042740.D
 Acq On : 19 Mar 2021 23:38
 Operator : SY/MD
 Sample : M1743-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETZE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	34826	39144	7.73%	1.357%
2	1.919	172	180	190	rVB	28093	36443	7.20%	1.263%
3	2.575	370	384	401	rBV	65054	105582	20.86%	3.659%
4	4.652	1015	1030	1053	rBV	27094	96483	19.06%	3.344%
5	5.073	1146	1161	1179	rBV2	51814	113774	22.48%	3.943%
6	5.732	1346	1366	1384	rBV4	103783	271404	53.63%	9.407%
7	6.256	1516	1529	1546	rBV	94637	178298	35.23%	6.180%
8	6.552	1610	1621	1633	rVB5	14420	27015	5.34%	0.936%
9	6.700	1654	1667	1684	rBV2	65135	126268	24.95%	4.376%
10	7.575	1928	1939	1952	rBV3	31242	55793	11.02%	1.934%
11	7.906	2029	2042	2060	rBV	122515	211884	41.87%	7.344%
12	8.186	2117	2129	2143	rBV2	19923	34428	6.80%	1.193%
13	8.478	2211	2220	2233	rBV3	2808	5400	1.07%	0.187%
14	8.559	2233	2245	2261	rBV	298714	506110	100.00%	17.542%
15	8.645	2261	2272	2303	rVB	147867	334604	66.11%	11.597%
16	9.423	2502	2514	2532	rBV	138865	233141	46.07%	8.081%
17	10.764	2920	2931	2945	rBV2	52802	86016	17.00%	2.981%
18	10.899	2964	2973	2985	rVB4	4015	6346	1.25%	0.220%
19	11.819	3247	3259	3279	rBV	137882	215625	42.60%	7.474%
20	12.201	3364	3378	3392	rBV	127993	201410	39.80%	6.981%




Sum of corrected areas: 2885168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042740.D
Acq On : 19 Mar 2021 23:38
Operator : SY/MD
Sample : M1743-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

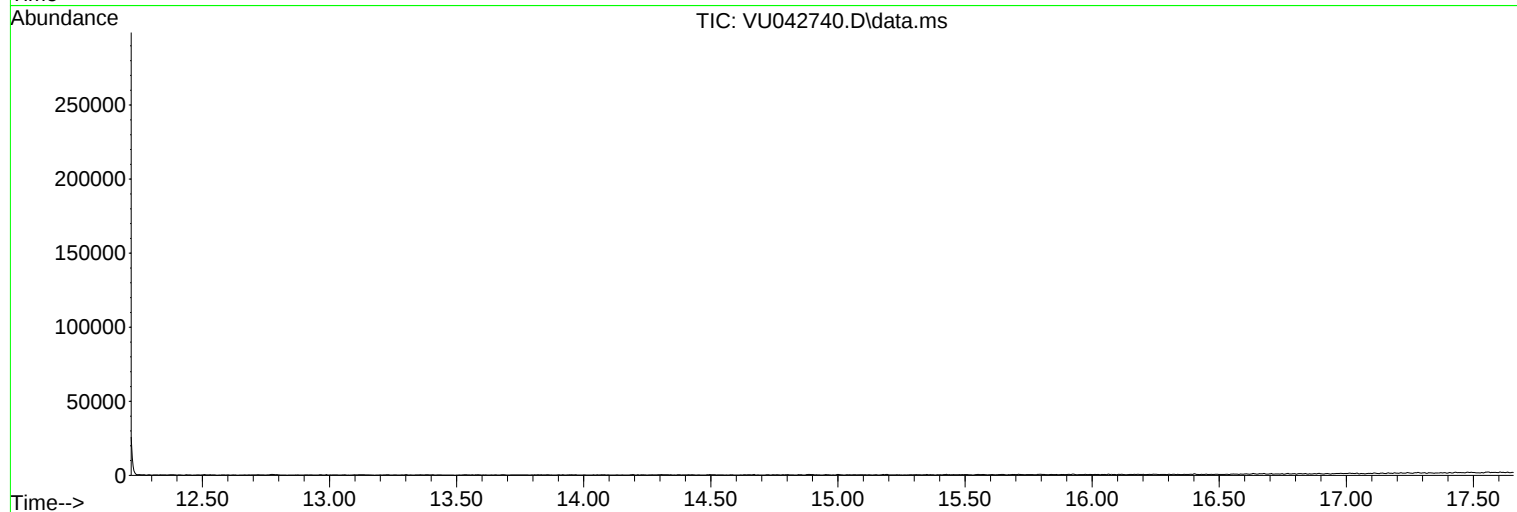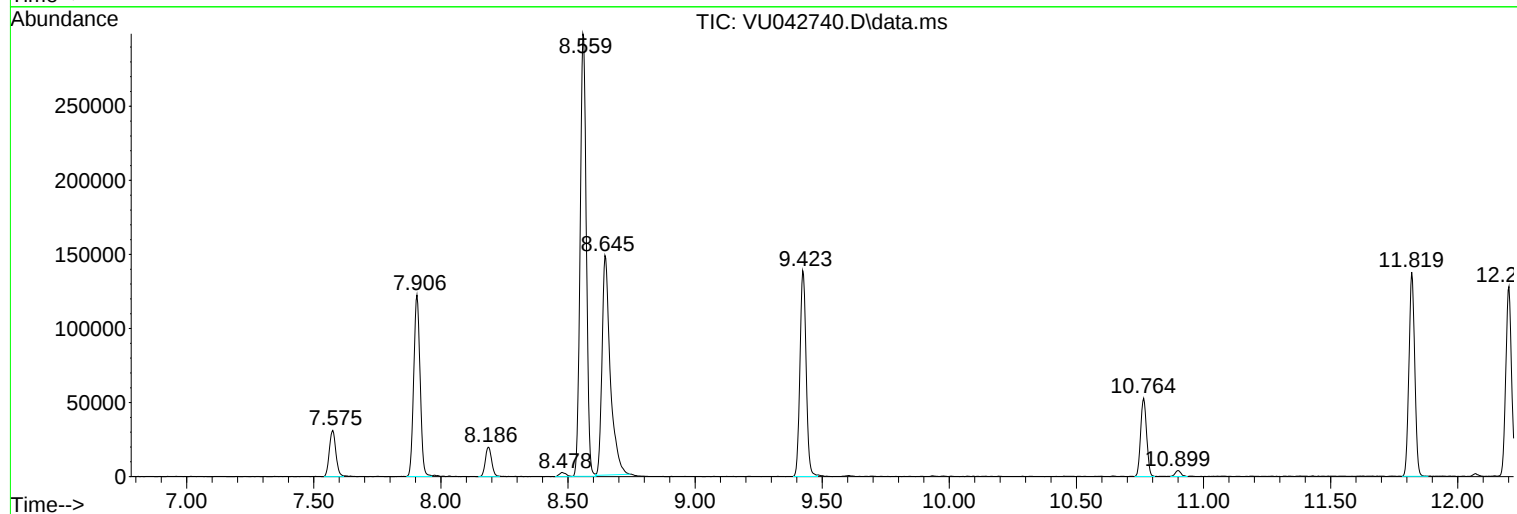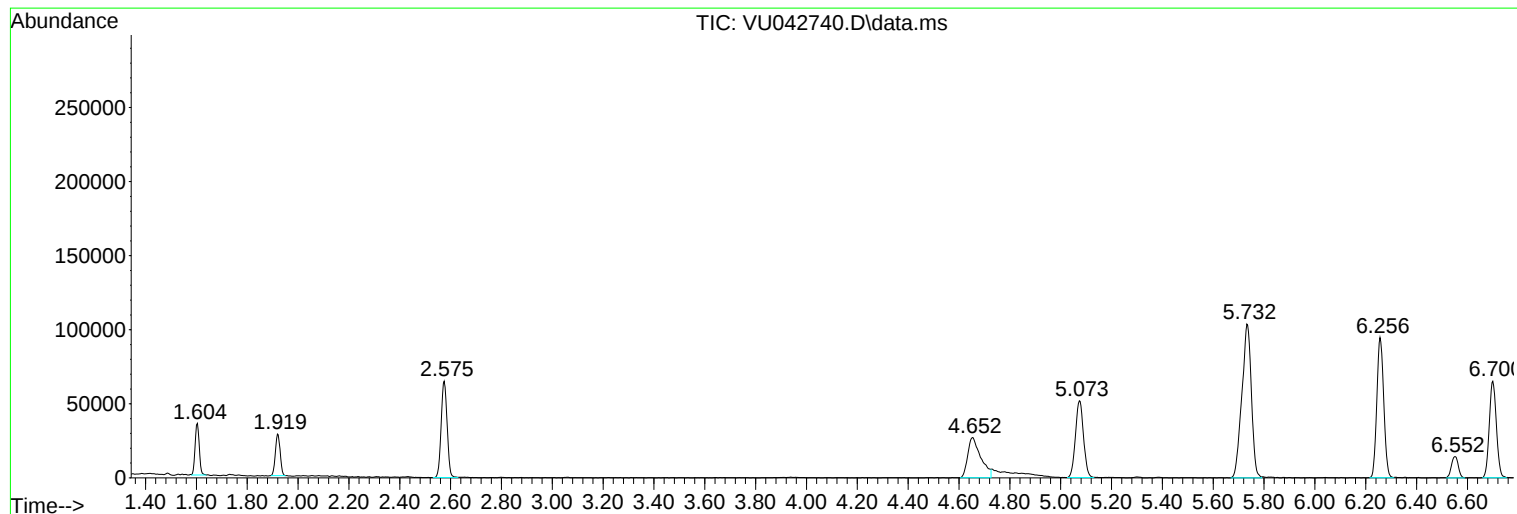

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042740.D
Acq On : 19 Mar 2021 23:38
Operator : SY/MD
Sample : M1743-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
Data File : VU042740.D
Acq On : 19 Mar 2021 23:38
Operator : SY/MD
Sample : M1743-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETZE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
