
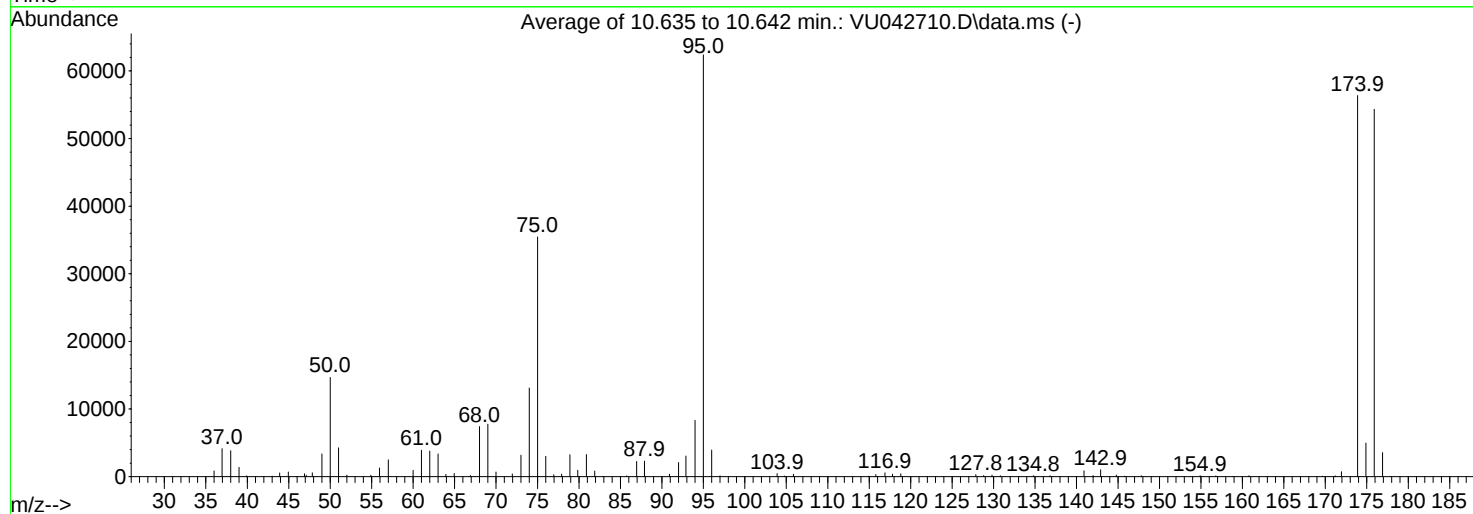


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031921\
 Data File : VU042710.D
 Acq On : 19 Mar 2021 08:47
 Operator : SY/MD
 Sample : BFB27
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 20 06:44:19 2021

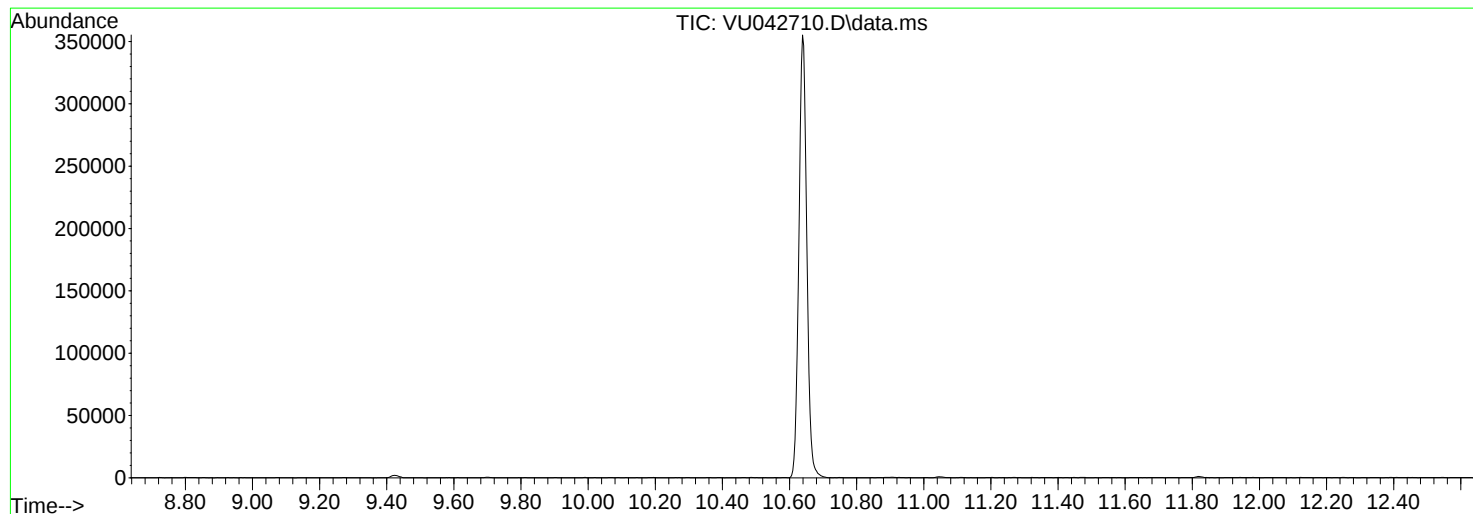

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	14673	PASS
75	95	30	80	56.8	35459	PASS
95	95	100	100	100.0	62381	PASS
96	95	5	9	6.3	3930	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.4	56368	PASS
175	174	5	9	8.8	4965	PASS
176	174	95	101	96.4	54328	PASS
177	176	5	9	6.6	3561	PASS

m/z	Abundance
36.00	787.0
37.00	4014.0
38.00	3750.0
39.00	1406.0
39.90	133.0
43.00	105.0
43.90	771.0
44.90	698.0
45.90	104.0
46.90	664.0
47.80	516.0
49.00	3392.0
50.00	14198.0
51.00	4152.0
52.00	192.0
54.90	206.0
56.00	1252.0
57.00	2454.0
60.00	892.0
61.00	3788.0
62.00	3627.0
63.00	3324.0
64.00	340.0
65.00	493.0
67.00	171.0
68.00	6844.0
69.00	7740.0
70.00	623.0
71.90	438.0
73.00	2986.0
74.00	12567.0
75.00	34352.0
76.00	2957.0
76.90	266.0
77.90	347.0
78.90	3156.0
79.90	912.0
80.90	3147.0
81.90	788.0
85.80	118.0
86.90	2186.0
87.90	2321.0
90.90	427.0
92.00	1967.0
92.90	2816.0
94.00	7956.0
95.00	60280.0
96.00	3961.0
97.00	111.0
103.90	474.0
104.80	138.0
105.80	292.0
114.90	119.0
115.80	270.0
116.90	561.0
117.80	358.0
118.80	469.0
127.90	322.0
128.90	150.0
129.80	237.0
130.80	129.0
134.80	159.0
136.80	147.0
140.90	806.0
142.00	149.0
142.90	954.0
144.80	280.0
147.80	125.0
154.90	150.0
156.80	123.0
160.80	129.0
169.60	111.0
171.90	667.0
173.90	53552.0
174.90	4782.0
175.90	51328.0
176.90	3454.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	898.0
37.00	4312.0
38.00	3953.0
39.00	1376.0
39.90	131.0
43.00	110.0
44.00	776.0
44.90	713.0
46.90	648.0
47.90	576.0
49.00	3452.0
50.00	15097.0
51.00	4328.0
52.00	250.0
54.90	229.0
56.00	1300.0
57.00	2583.0
60.00	957.0
61.00	4082.0
62.00	3886.0
63.00	3468.0
63.90	349.0
65.00	497.0
66.80	170.0
68.00	7669.0
69.00	8059.0
70.00	685.0
71.90	417.0
73.00	3239.0
74.00	13539.0
75.00	36640.0
76.00	3073.0
76.90	280.0
77.90	411.0
78.90	3291.0
79.80	982.0
80.90	3367.0
81.90	858.0
85.70	129.0
87.00	2297.0
87.90	2337.0
90.90	366.0
92.00	2151.0
92.90	3133.0
94.00	8583.0
95.00	64472.0
96.00	4030.0
97.00	135.0
103.90	458.0
104.80	128.0
105.90	370.0
114.90	121.0
115.80	323.0
116.90	601.0
117.80	383.0
118.80	430.0
127.90	317.0
128.80	167.0
129.80	245.0
130.80	151.0
134.80	133.0
136.80	153.0
140.90	918.0
142.00	175.0
142.90	1079.0
144.80	257.0
145.80	105.0
147.80	132.0
154.90	149.0
156.80	108.0
160.80	144.0
169.70	100.0
171.20	172.0
171.90	731.0
173.90	58120.0
174.90	5145.0
175.90	55888.0
176.90	3673.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	861.0
36.90	4104.0
38.00	3801.0
39.00	1319.0
39.90	125.0
44.00	723.0
45.00	672.0
47.10	617.0
47.90	582.0
49.00	3234.0
50.00	14724.0
51.00	4323.0
52.00	276.0
54.90	205.0
55.90	1272.0
57.00	2392.0
60.00	890.0
61.00	3878.0
62.00	3829.0
63.00	3297.0
63.90	315.0
64.90	466.0
66.90	156.0
68.00	7706.0
69.00	7515.0
70.00	720.0
72.00	348.0
73.00	3291.0
74.00	13219.0
75.00	35384.0
76.00	2979.0
77.00	315.0
77.90	378.0
78.90	3252.0
79.80	957.0
80.90	3323.0
81.90	809.0
82.90	118.0
85.80	104.0
87.00	2244.0
87.90	2235.0
90.90	296.0
92.00	2124.0
92.90	3181.0
94.00	8429.0
95.00	62392.0
96.00	3800.0
97.00	138.0
103.90	394.0
105.90	409.0
115.80	327.0
116.90	557.0
117.80	362.0
118.80	396.0
127.80	257.0
128.70	157.0
129.80	235.0
130.80	151.0
134.80	110.0
136.80	134.0
140.90	887.0
142.00	168.0
142.90	1021.0
144.80	206.0
145.80	100.0
147.80	138.0
154.90	141.0
156.80	110.0
158.80	106.0
160.80	125.0
171.20	188.0
172.00	794.0
173.90	57432.0
174.90	4967.0
175.90	55768.0
176.90	3555.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
43.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27