

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031924\
 Data File : VU058159.D
 Acq On : 19 Mar 2024 16:50
 Operator : MD/SY
 Sample : P1796-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCFZ6

Quant Time: Mar 20 05:21:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 20 05:19:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	118578	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	113052	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	46657	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	39323	4.609	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.200%
7) Chloroethane-d5	1.904	69	36200	5.162	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.200%
11) 1,1-Dichloroethene-d2	2.557	65	17963	4.866	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.400%
20) 2-Butanone-d5	4.615	46	78260	55.673	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.340%
24) Chloroform-d	5.052	84	80744	5.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.692	65	39535	5.407	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
32) Benzene-d6	5.717	84	162614	4.936	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
36) 1,2-Dichloropropane-d6	6.682	67	52449	5.237	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.800%
41) Toluene-d8	7.891	98	135485	4.539	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	8.177	79	14026	4.072	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.627	63	62528	54.073	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.140%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	32704	5.325	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	40352	5.251	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds					Qvalue	
13) Acetone	2.621	43	4835	4.622	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031924\
Data File : VU058159.D
Acq On : 19 Mar 2024 16:50
Operator : MD/SY
Sample : P1796-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCFZ6

Quant Time: Mar 20 05:21:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 20 05:19:57 2024
Response via : Initial Calibration

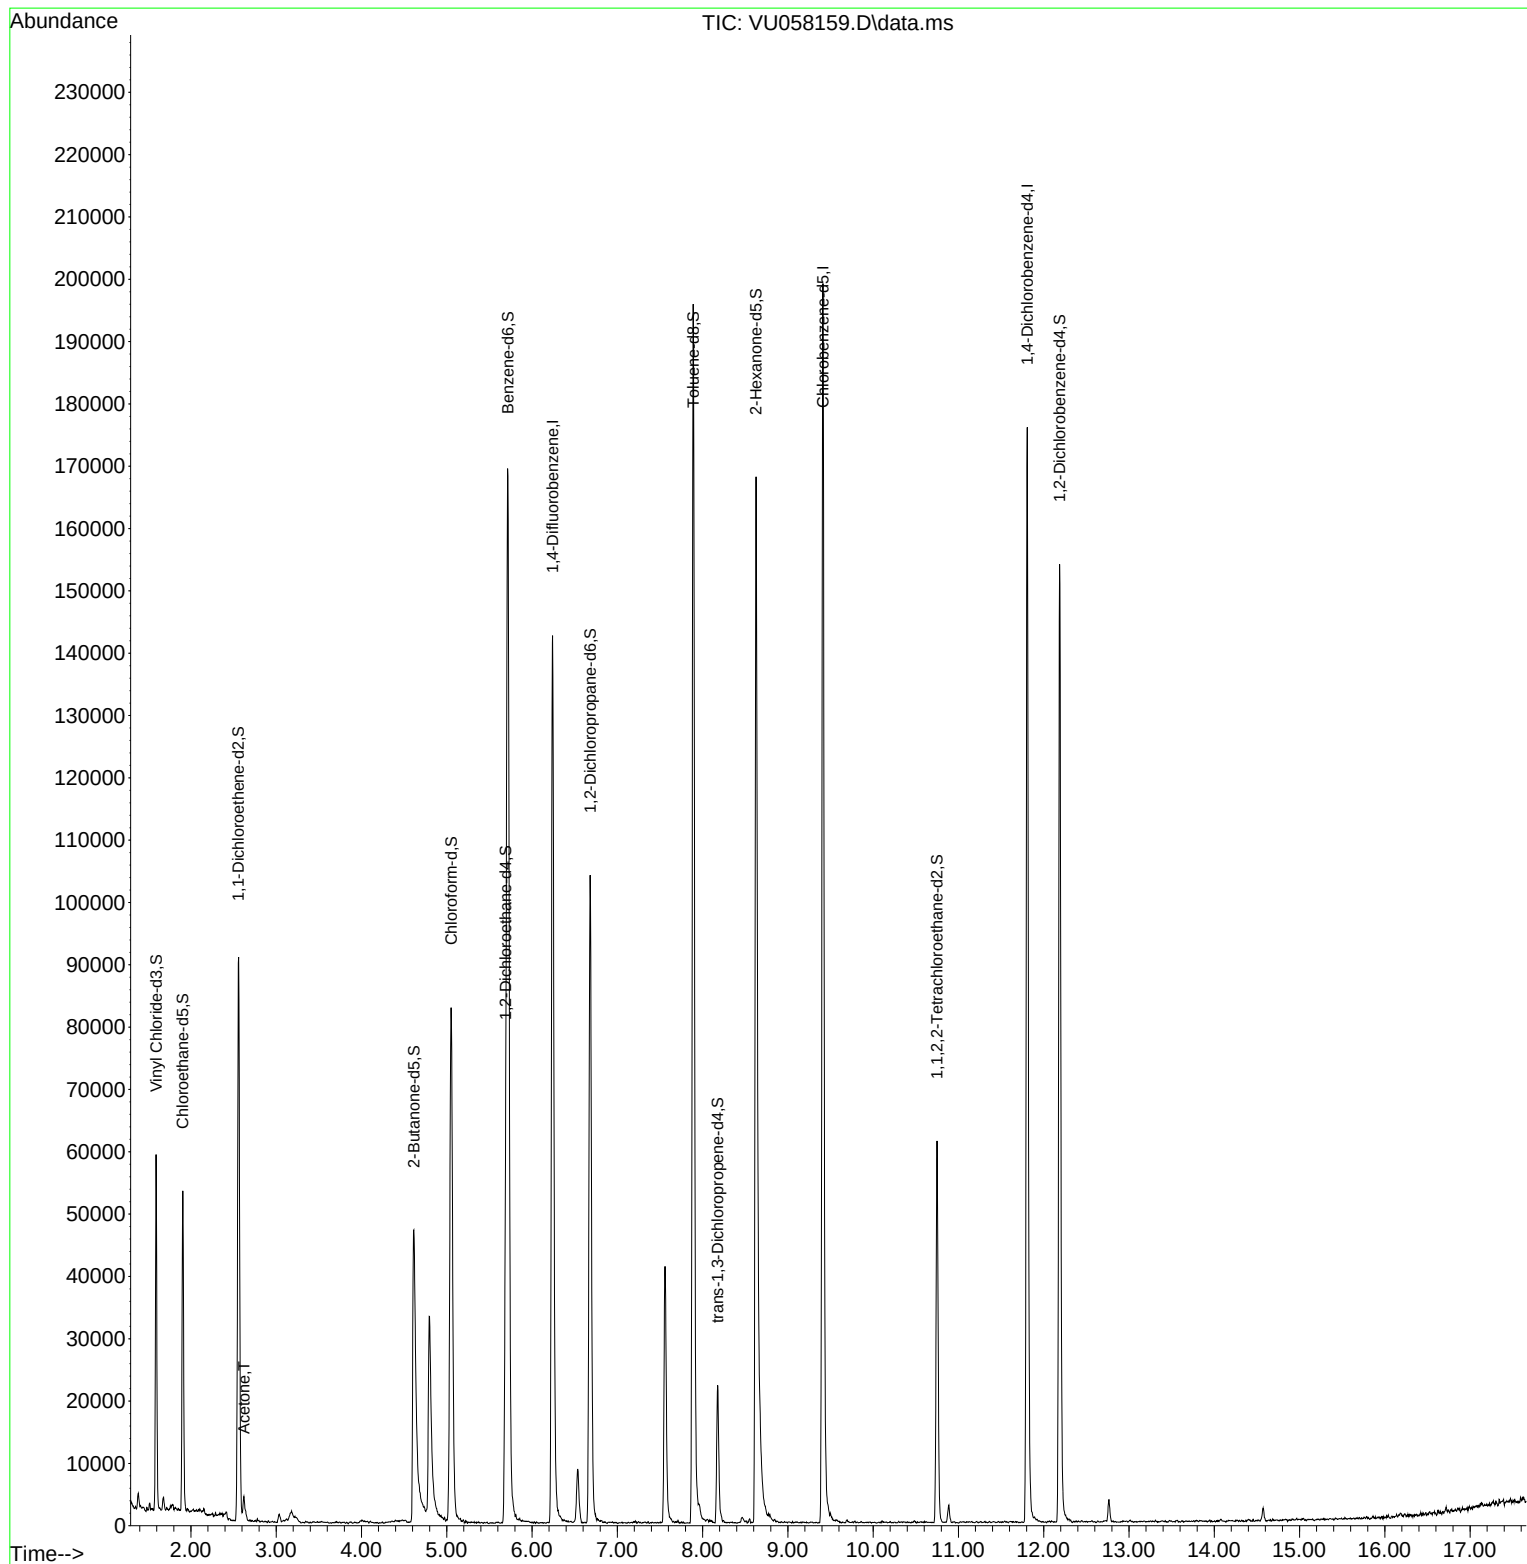

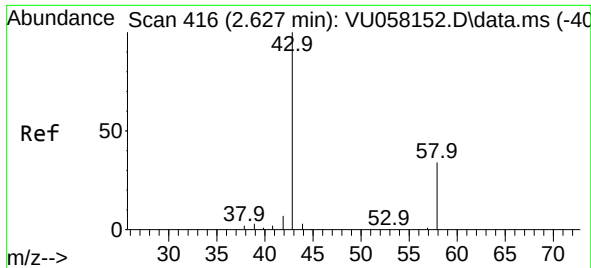

#13
 Acetone
 Concen: 4.622 ug/L
 RT: 2.621 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU058159.D
 Acq: 19 Mar 2024 16:50

Instrument :
 MSVOA_U
 ClientSampleId :
 GCFZ6

Tgt Ion: 43 Resp: 4835
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 63.6

