

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031924\
 Data File : VU058168.D
 Acq On : 19 Mar 2024 22:15
 Operator : MD/SY
 Sample : P1796-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCFZ1

Quant Time: Mar 20 05:24:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 20 05:19:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	159898	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	153416	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	67212	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	36044	3.133	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.600%
7) Chloroethane-d5	1.911	69	34078	3.604	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.000%
11) 1,1-Dichloroethene-d2	2.563	65	17098	3.434	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	4.628	46	98262	51.838	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.680%
24) Chloroform-d	5.055	84	79759	3.666	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.400%
26) 1,2-Dichloroethane-d4	5.695	65	40841	4.143	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.800%
32) Benzene-d6	5.721	84	155382	3.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.600%#
36) 1,2-Dichloropropane-d6	6.682	67	51773	3.809	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.200%
41) Toluene-d8	7.891	98	132433	3.269	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.400%#
43) trans-1,3-Dichloroprop...	8.174	79	15632	3.345	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.800%
46) 2-Hexanone-d5	8.627	63	75144	47.886	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.780%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	35237	4.228	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	43638	3.942	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	78.800%#
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.576	96	15848	1.643	ug/L #	69
22) cis-1,2-Dichloroethene	4.656	96	8895	0.769	ug/L	96
25) Chloroform	5.081	83	7579	0.354	ug/L	93
31) Carbon tetrachloride	5.518	117	22231	1.401	ug/L	97
34) Trichloroethene	6.534	95	93516	7.550	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031924\
Data File : VU058168.D
Acq On : 19 Mar 2024 22:15
Operator : MD/SY
Sample : P1796-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCFZ1

Quant Time: Mar 20 05:24:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 20 05:19:57 2024
Response via : Initial Calibration

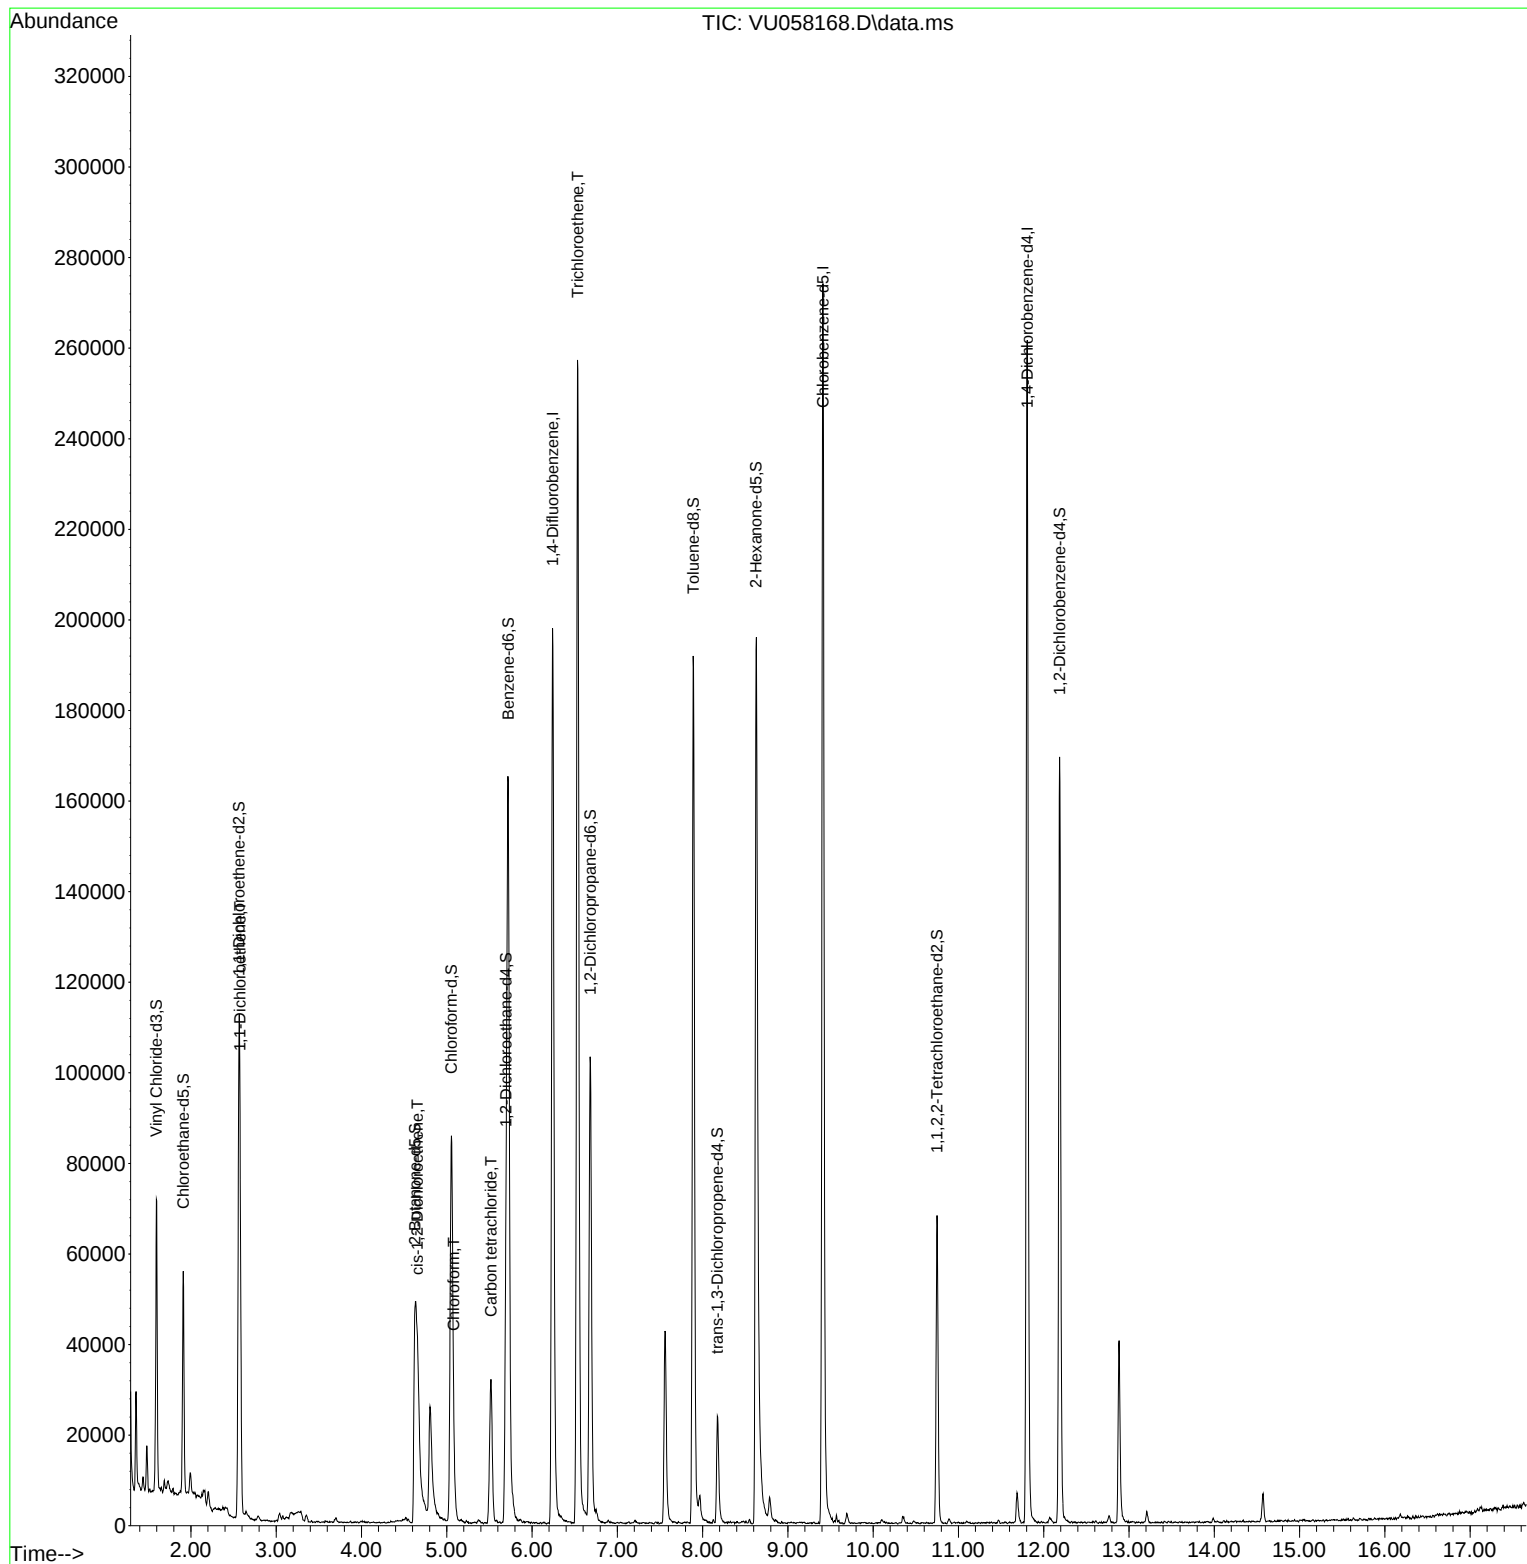

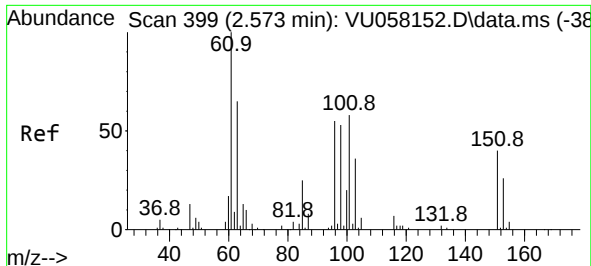

#12

1,1-Dichloroethene

Concen: 1.643 ug/L

RT: 2.576 min Scan# 400

Delta R.T. 0.003 min

Lab File: VU058168.D

Acq: 19 Mar 2024 22:15

Instrument :

MSVOA_U

ClientSampleId :

GCFZ1





Tgt Ion: 96 Resp: 15848

Ion Ratio Lower Upper

96 100

61 185.7 131.8 244.8

63 227.0 98.1 182.1#

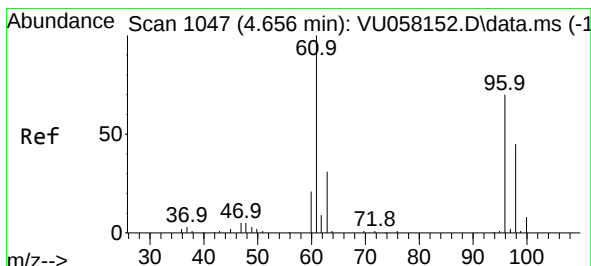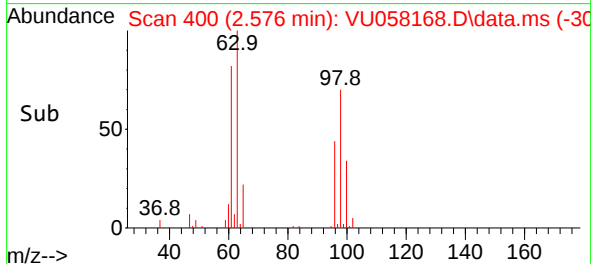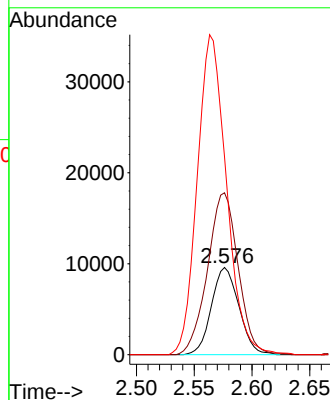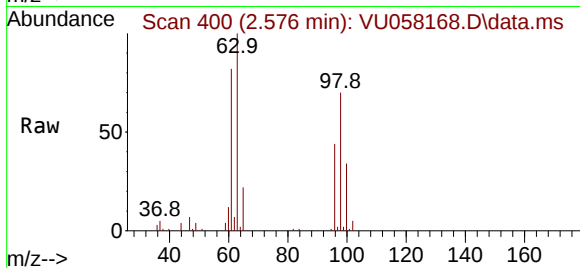

#22

cis-1,2-Dichloroethene

Concen: 0.769 ug/L

RT: 4.656 min Scan# 1047

Delta R.T. 0.000 min

Lab File: VU058168.D

Acq: 19 Mar 2024 22:15




Tgt Ion: 96 Resp: 8895


Ion Ratio Lower Upper

96 100

61 131.8 97.2 180.4

98 64.7 45.5 84.5


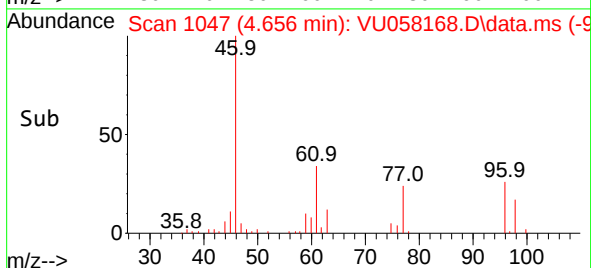
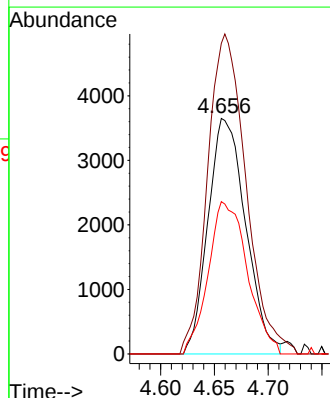
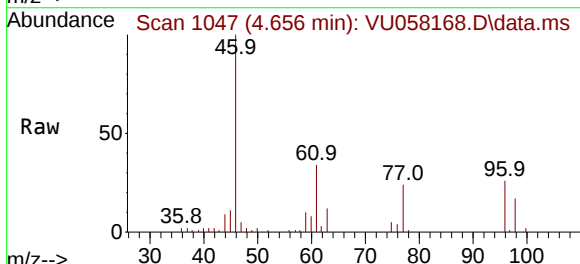


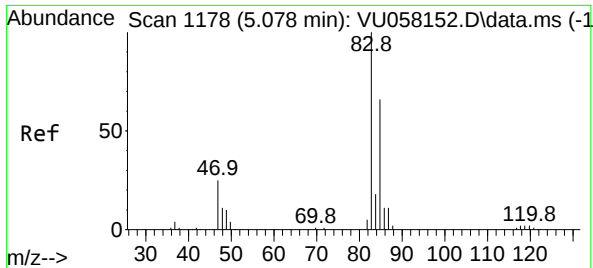

#25
Chloroform
Concen: 0.354 ug/L
RT: 5.081 min Scan# 1178
Delta R.T. 0.003 min
Lab File: VU058168.D
Acq: 19 Mar 2024 22:15




Instrument :
MSVOA_U
ClientSampleId :
GCFZ1


Tgt Ion: 83 Resp: 7579
Ion Ratio Lower Upper
83 100
85 59.4 45.4 84.4

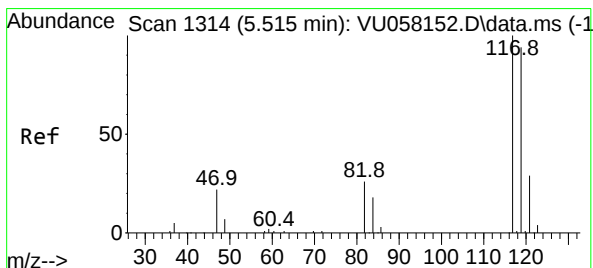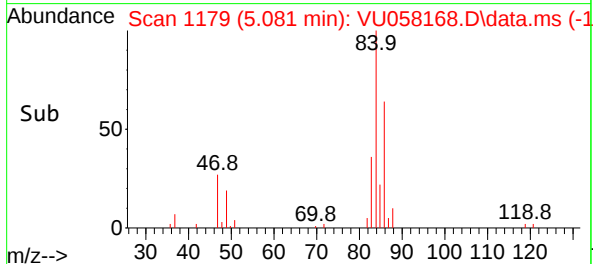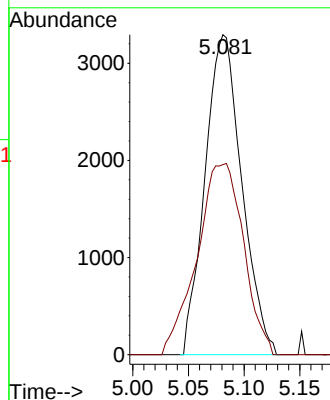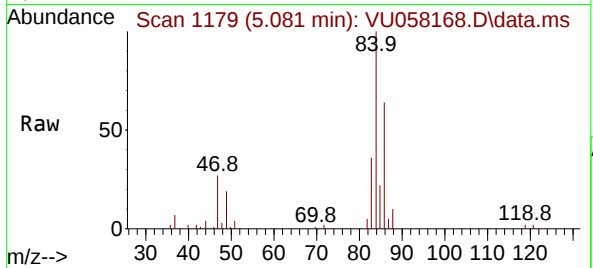

#31
Carbon tetrachloride
Concen: 1.401 ug/L
RT: 5.518 min Scan# 1315
Delta R.T. 0.003 min
Lab File: VU058168.D
Acq: 19 Mar 2024 22:15

Tgt Ion: 117 Resp: 22231
Ion Ratio Lower Upper
117 100
119 97.3 75.8 113.8

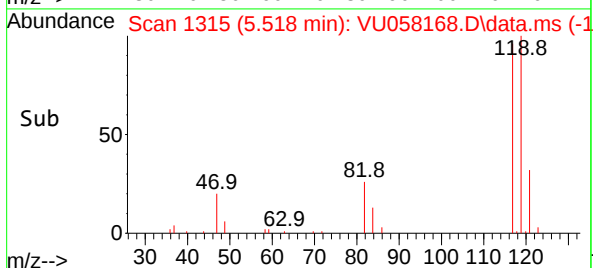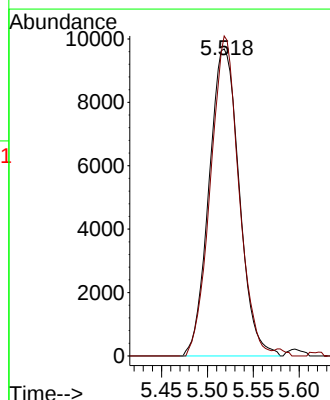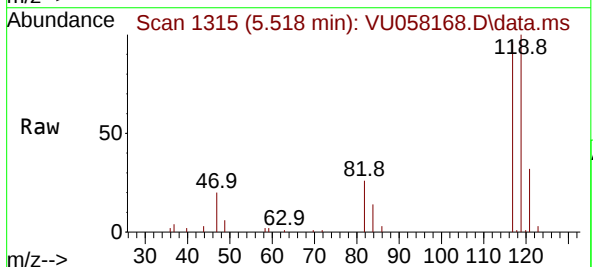

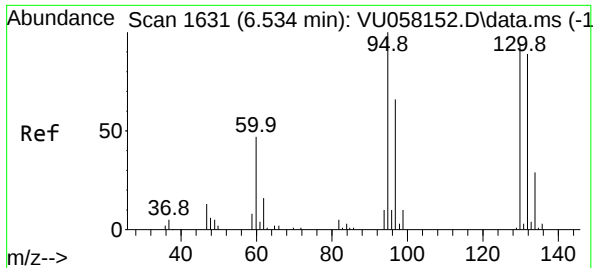

#34
 Trichloroethene
 Concen: 7.550 ug/L
 RT: 6.534 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU058168.D
 Acq: 19 Mar 2024 22:15

Instrument :
 MSVOA_U
 ClientSampleId :
 GCFZ1

Tgt Ion: 95	Resp:	93516
Ion	Ratio	Lower Upper
95	100	
97	65.7	45.3 84.1
132	88.5	63.1 117.1
130	92.3	67.6 125.6

