

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030217.D
 Acq On : 20 Mar 2019 09:20
 Operator : JC/SP
 Sample : VU0320MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rVB	12677	12510	0.68%	0.085%
2	1.399	89	96	109	rBV	261726	260999	14.22%	1.770%
3	1.678	174	183	197	rBV	194321	250805	13.66%	1.700%
4	2.270	356	367	381	rBV	422652	639997	34.86%	4.339%
5	2.479	424	432	439	rVB3	2995	4770	0.26%	0.032%
6	2.572	453	461	464	rBV5	1047	1675	0.09%	0.011%
7	2.694	496	499	503	rBV2	1296	1134	0.06%	0.008%
8	2.865	549	552	555	rBV2	1002	739	0.04%	0.005%
9	2.891	556	560	564	rVV3	813	712	0.04%	0.005%
10	3.096	617	624	626	rBV	1011	1280	0.07%	0.009%
11	3.161	641	644	648	rVB	854	626	0.03%	0.004%
12	3.199	652	656	659	rVB	946	709	0.04%	0.005%
13	3.228	659	665	668	rBV	1163	1478	0.08%	0.010%
14	3.411	719	722	726	rBV	869	669	0.04%	0.005%
15	3.566	765	770	774	rBV2	720	959	0.05%	0.007%
16	3.678	801	805	811	rVB2	1066	1073	0.06%	0.007%
17	3.730	817	821	824	rBV	928	834	0.05%	0.006%
18	3.810	840	846	847	rBV	648	677	0.04%	0.005%
19	4.045	916	919	926	rVV2	1103	980	0.05%	0.007%
20	4.173	947	959	992	rBV	168609	445674	24.28%	3.022%
21	4.643	1090	1105	1130	rBV2	294479	701712	38.22%	4.757%
22	4.974	1203	1208	1211	rBV3	1603	1737	0.09%	0.012%
23	5.337	1296	1321	1353	rBV2	623451	1835819	100.00%	12.447%
24	5.884	1477	1491	1530	rBV	577193	1182019	64.39%	8.014%
25	6.328	1615	1629	1655	rBV	393583	801970	43.68%	5.437%
26	6.646	1725	1728	1731	rBV2	1326	985	0.05%	0.007%
27	7.225	1897	1908	1930	rBV	228202	417679	22.75%	2.832%
28	7.469	1973	1984	1993	rBV5	4575	8928	0.49%	0.061%
29	7.562	2000	2013	2052	rBV	838507	1513929	82.47%	10.264%
30	7.849	2091	2102	2122	rBV	155561	280344	15.27%	1.901%
31	8.308	2234	2245	2286	rBV	572045	1046262	56.99%	7.093%
32	8.582	2327	2330	2335	rBV5	1373	1344	0.07%	0.009%
33	8.810	2396	2401	2405	rBV2	1165	1037	0.06%	0.007%
34	8.900	2421	2429	2431	rBV3	1124	1381	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030217.D
 Acq On : 20 Mar 2019 09:20
 Operator : JC/SP
 Sample : VU0320MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	8.968	2448	2450	2455	rBV2	920	731	0.04%	0.005%
36	9.086	2474	2487	2513	rBV	842735	1446528	78.79%	9.807%
37	9.360	2569	2572	2573	rBV2	1268	745	0.04%	0.005%
38	9.533	2621	2626	2627	rBV2	868	784	0.04%	0.005%
39	9.755	2692	2695	2698	rBV	1106	850	0.05%	0.006%
40	9.794	2698	2707	2710	rBV5	2667	3686	0.20%	0.025%
41	9.890	2734	2737	2740	rBV	832	667	0.04%	0.005%
42	9.955	2753	2757	2762	rBV2	892	847	0.05%	0.006%
43	10.041	2778	2784	2789	rVB2	914	1289	0.07%	0.009%
44	10.067	2789	2792	2796	rBV	1198	903	0.05%	0.006%
45	10.167	2815	2823	2831	rBV4	3092	5062	0.28%	0.034%
46	10.321	2865	2871	2874	rBV	1377	1431	0.08%	0.010%
47	10.427	2890	2904	2922	rBV	611584	989424	53.90%	6.708%
48	10.643	2968	2971	2978	rVB	945	878	0.05%	0.006%
49	10.691	2979	2986	2989	rBV2	774	983	0.05%	0.007%
50	10.797	3013	3019	3021	rBV	788	772	0.04%	0.005%
51	10.855	3033	3037	3044	rVB3	972	1165	0.06%	0.008%
52	10.900	3048	3051	3054	rVB	1187	761	0.04%	0.005%
53	11.061	3097	3101	3104	rBV2	751	713	0.04%	0.005%
54	11.083	3104	3108	3114	rVV4	1146	1014	0.06%	0.007%
55	11.138	3121	3125	3128	rBV	959	806	0.04%	0.005%
56	11.189	3136	3141	3144	rBV2	809	745	0.04%	0.005%
57	11.286	3168	3171	3173	rBV2	920	653	0.04%	0.004%
58	11.353	3189	3192	3195	rVV2	686	610	0.03%	0.004%
59	11.418	3201	3212	3220	rBV6	5657	10443	0.57%	0.071%
60	11.479	3220	3231	3257	rVV	836840	1366043	74.41%	9.262%
61	11.858	3336	3349	3383	rBV	830497	1374058	74.85%	9.316%
62	12.305	3481	3488	3496	rBV4	823	1368	0.07%	0.009%
63	12.389	3511	3514	3517	rBV3	742	656	0.04%	0.004%
64	12.453	3527	3534	3536	rBV	842	942	0.05%	0.006%
65	12.649	3590	3595	3596	rVV3	726	631	0.03%	0.004%
66	12.707	3610	3613	3619	rVB2	895	712	0.04%	0.005%
67	12.781	3633	3636	3640	rVV	791	786	0.04%	0.005%
68	12.852	3651	3658	3662	rBV3	793	815	0.04%	0.006%
69	12.893	3662	3671	3683	rBV8	7035	13965	0.76%	0.095%
70	12.977	3694	3697	3700	rVB2	1010	609	0.03%	0.004%
71	13.003	3700	3705	3707	rBV2	569	649	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030217.D
 Acq On : 20 Mar 2019 09:20
 Operator : JC/SP
 Sample : VU0320MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	13.048	3716	3719	3725	rVB2	1227	1093	0.06%	0.007%
73	13.080	3725	3729	3733	rBV2	1131	941	0.05%	0.006%
74	13.109	3733	3738	3743	rBV3	478	610	0.03%	0.004%
75	13.176	3753	3759	3762	rBV2	845	858	0.05%	0.006%
76	13.196	3762	3765	3771	rVB	776	848	0.05%	0.006%
77	13.247	3771	3781	3792	rVB3	1364	2615	0.14%	0.018%
78	13.302	3792	3798	3804	rBV2	856	1039	0.06%	0.007%
79	13.398	3824	3828	3831	rVB2	921	653	0.04%	0.004%
80	13.514	3854	3864	3874	rBV6	7154	15239	0.83%	0.103%
81	13.688	3908	3918	3925	rVB	1178	1751	0.10%	0.012%
82	13.755	3925	3939	3950	rBV2	12432	32659	1.78%	0.221%
83	13.881	3975	3978	3983	rVB2	1048	765	0.04%	0.005%
84	13.909	3983	3987	3991	rBV2	1042	851	0.05%	0.006%
85	13.996	4004	4014	4020	rBV6	9863	17450	0.95%	0.118%
86	14.131	4052	4056	4063	rBV5	1197	1357	0.07%	0.009%
87	14.273	4095	4100	4102	rBV4	877	763	0.04%	0.005%
88	14.356	4123	4126	4130	rVB2	1060	773	0.04%	0.005%
89	14.389	4130	4136	4139	rBV	835	679	0.04%	0.005%
90	14.437	4146	4151	4156	rBV3	925	798	0.04%	0.005%
91	14.475	4160	4163	4166	rBV2	930	712	0.04%	0.005%
92	14.543	4181	4184	4189	rBV2	1038	915	0.05%	0.006%
93	14.643	4210	4215	4218	rVB2	1284	1168	0.06%	0.008%
94	14.794	4259	4262	4271	rVB4	763	833	0.05%	0.006%
95	14.951	4308	4311	4315	rVV3	1074	712	0.04%	0.005%
96	15.028	4331	4335	4339	rBV5	1100	1103	0.06%	0.007%
97	15.131	4364	4367	4371	rBV3	1171	935	0.05%	0.006%
98	15.305	4418	4421	4426	rVB4	1346	937	0.05%	0.006%
99	15.488	4473	4478	4482	rBV5	1212	1573	0.09%	0.011%
100	15.633	4518	4523	4526	rBV6	1650	1834	0.10%	0.012%


Sum of corrected areas: 14749634

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU032017.D
Acq On : 20 Mar 2019 09:20
Operator : JC/SP
Sample : VU0320MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

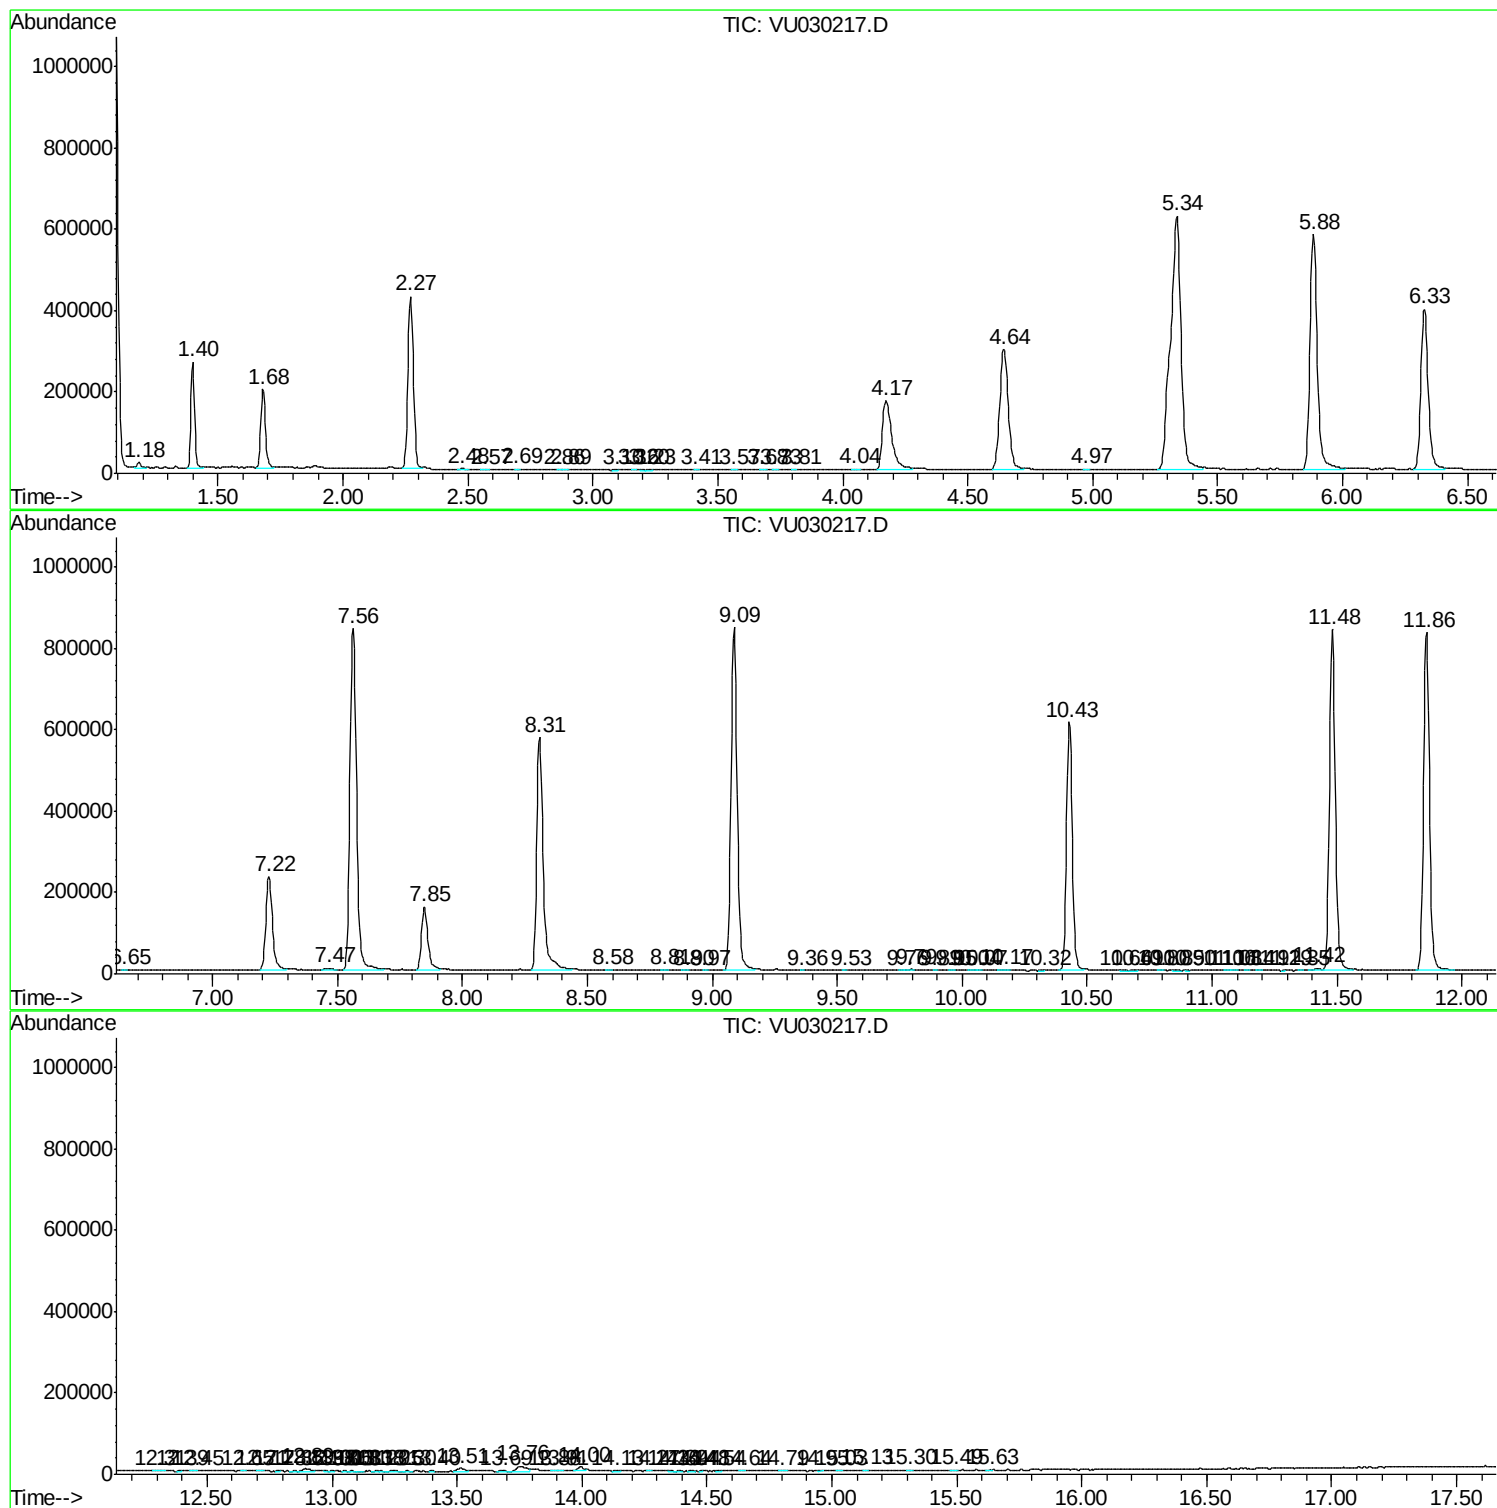

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030217.D
Acq On : 20 Mar 2019 09:20
Operator : JC/SP
Sample : VU0320MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030217.D
Acq On : 20 Mar 2019 09:20
Operator : JC/SP
Sample : VU0320MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc