

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030218.D
 Acq On : 20 Mar 2019 09:44
 Operator : JC/SP
 Sample : VU0320WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	10876	9987	0.57%	0.070%
2	1.399	89	96	113	rBV	249100	252231	14.28%	1.769%
3	1.679	175	183	201	rVB	180438	235575	13.34%	1.652%
4	2.270	357	367	382	rBV	408313	616766	34.92%	4.325%
5	4.174	947	959	987	rBV	171262	449306	25.44%	3.151%
6	4.646	1091	1106	1126	rBV	285765	682467	38.64%	4.786%
7	5.338	1298	1321	1351	rBV2	602366	1766361	100.00%	12.387%
8	5.884	1477	1491	1523	rBV	554940	1138386	64.45%	7.983%
9	6.328	1615	1629	1652	rBV	383791	786305	44.52%	5.514%
10	6.530	1689	1692	1693	rBV2	1221	727	0.04%	0.005%
11	7.055	1852	1855	1857	rBV2	1174	749	0.04%	0.005%
12	7.112	1870	1873	1874	rBV2	1011	620	0.04%	0.004%
13	7.180	1891	1894	1896	rBV	1268	877	0.05%	0.006%
14	7.225	1897	1908	1940	rVB	219697	413397	23.40%	2.899%
15	7.563	2000	2013	2048	rBV	823284	1474203	83.46%	10.338%
16	7.849	2092	2102	2122	rBV	149041	265486	15.03%	1.862%
17	8.177	2198	2204	2212	rBV5	3277	5026	0.28%	0.035%
18	8.309	2234	2245	2281	rBV	571827	1045578	59.19%	7.332%
19	8.720	2371	2373	2380	rVB	1390	1202	0.07%	0.008%
20	8.807	2397	2400	2402	rBV	823	635	0.04%	0.004%
21	8.929	2435	2438	2444	rVV	1035	849	0.05%	0.006%
22	8.958	2444	2447	2450	rVB2	723	529	0.03%	0.004%
23	9.000	2456	2460	2464	rBV	1030	893	0.05%	0.006%
24	9.022	2464	2467	2469	rBV	521	391	0.02%	0.003%
25	9.087	2474	2487	2509	rBV	837919	1406478	79.63%	9.863%
26	9.363	2570	2573	2575	rVB	746	443	0.03%	0.003%
27	9.382	2576	2579	2582	rBV2	1436	1118	0.06%	0.008%
28	9.447	2597	2599	2605	rVB2	705	596	0.03%	0.004%
29	9.476	2605	2608	2612	rBV2	887	617	0.03%	0.004%
30	9.505	2612	2617	2622	rVB2	899	1019	0.06%	0.007%
31	9.534	2623	2626	2628	rBV	760	424	0.02%	0.003%
32	9.550	2628	2631	2634	rVV3	403	223	0.01%	0.002%
33	9.611	2644	2650	2651	rBV	817	809	0.05%	0.006%
34	9.730	2684	2687	2689	rBV	796	527	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030218.D
 Acq On : 20 Mar 2019 09:44
 Operator : JC/SP
 Sample : VU0320WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	9.746	2689	2692	2697	rVB	999	664	0.04%	0.005%
36	9.778	2697	2702	2704	rVB2	696	550	0.03%	0.004%
37	9.794	2704	2707	2710	rBV2	586	441	0.02%	0.003%
38	9.839	2719	2721	2724	rVB2	543	282	0.02%	0.002%
39	10.009	2769	2774	2777	rBV2	1356	1225	0.07%	0.009%
40	10.090	2795	2799	2804	rBV2	937	1279	0.07%	0.009%
41	10.209	2832	2836	2841	rBV3	1256	1321	0.07%	0.009%
42	10.238	2842	2845	2848	rVB	739	552	0.03%	0.004%
43	10.325	2869	2872	2875	rBV3	790	469	0.03%	0.003%
44	10.427	2891	2904	2921	rBV	606301	980127	55.49%	6.873%
45	10.559	2942	2945	2947	rBV	506	274	0.02%	0.002%
46	10.582	2947	2952	2955	rVV3	766	810	0.05%	0.006%
47	10.604	2955	2959	2972	rVB6	2695	4479	0.25%	0.031%
48	10.656	2972	2975	2977	rBV2	326	222	0.01%	0.002%
49	10.672	2977	2980	2982	rBV2	670	376	0.02%	0.003%
50	10.704	2987	2990	2993	rVB	883	553	0.03%	0.004%
51	10.723	2993	2996	2998	rBV2	628	359	0.02%	0.003%
52	10.752	3002	3005	3009	rVB	713	502	0.03%	0.004%
53	10.778	3009	3013	3021	rVB2	982	1296	0.07%	0.009%
54	10.813	3021	3024	3028	rBV2	853	673	0.04%	0.005%
55	10.839	3028	3032	3034	rBV2	763	573	0.03%	0.004%
56	10.887	3043	3047	3049	rBV2	524	468	0.03%	0.003%
57	10.903	3049	3052	3055	rBV	522	312	0.02%	0.002%
58	10.939	3060	3063	3066	rBV2	875	687	0.04%	0.005%
59	11.032	3089	3092	3094	rVV	446	272	0.02%	0.002%
60	11.048	3094	3097	3102	rVV3	653	602	0.03%	0.004%
61	11.083	3106	3108	3116	rVB2	1019	930	0.05%	0.007%
62	11.119	3116	3119	3124	rVB	699	593	0.03%	0.004%
63	11.161	3129	3132	3135	rVB	893	506	0.03%	0.004%
64	11.177	3135	3137	3142	rVB	835	677	0.04%	0.005%
65	11.206	3142	3146	3151	rBV	896	846	0.05%	0.006%
66	11.234	3151	3155	3160	rBV3	681	739	0.04%	0.005%
67	11.263	3160	3164	3171	rVB3	842	1214	0.07%	0.009%
68	11.296	3171	3174	3175	rBV	395	251	0.01%	0.002%
69	11.331	3181	3185	3186	rBV2	586	434	0.02%	0.003%
70	11.421	3205	3213	3219	rBV7	2837	4103	0.23%	0.029%
71	11.479	3219	3231	3255	rBV	809933	1332184	75.42%	9.342%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030218.D
 Acq On : 20 Mar 2019 09:44
 Operator : JC/SP
 Sample : VU0320WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.807	3330	3333	3335	rBV3	1291	889	0.05%	0.006%
73	11.855	3336	3348	3373	rVV	794188	1333068	75.47%	9.348%
74	12.086	3417	3420	3428	rVB3	1158	1404	0.08%	0.010%
75	12.125	3428	3432	3437	rBV2	1417	1218	0.07%	0.009%
76	12.296	3482	3485	3487	rBV	902	580	0.03%	0.004%
77	12.341	3495	3499	3505	rBV2	1220	1587	0.09%	0.011%
78	12.392	3511	3515	3521	rBV4	923	1295	0.07%	0.009%
79	12.479	3538	3542	3545	rVB2	1271	883	0.05%	0.006%
80	12.627	3582	3588	3594	rBV2	1383	1768	0.10%	0.012%
81	12.810	3642	3645	3646	rBV	637	386	0.02%	0.003%
82	12.868	3661	3663	3665	rBV	762	397	0.02%	0.003%
83	12.884	3665	3668	3669	rBV3	961	567	0.03%	0.004%
84	12.958	3688	3691	3693	rBV	781	500	0.03%	0.004%
85	12.974	3694	3696	3699	rBV2	768	446	0.03%	0.003%
86	13.035	3712	3715	3716	rBV	707	393	0.02%	0.003%
87	13.167	3754	3756	3758	rBV2	564	319	0.02%	0.002%
88	13.202	3765	3767	3770	rBV	613	412	0.02%	0.003%
89	13.241	3775	3779	3785	rVB2	1112	1052	0.06%	0.007%
90	13.308	3797	3800	3803	rBV	782	541	0.03%	0.004%
91	13.363	3813	3817	3818	rBV2	666	480	0.03%	0.003%
92	13.395	3825	3827	3832	rVB	1021	620	0.04%	0.004%
93	13.517	3861	3865	3866	rBV3	1502	1015	0.06%	0.007%
94	13.588	3884	3887	3891	rBV3	1404	1143	0.06%	0.008%
95	13.694	3917	3920	3922	rBV2	885	568	0.03%	0.004%
96	13.768	3937	3943	3945	rBV3	2351	2483	0.14%	0.017%
97	14.090	4040	4043	4046	rBV2	891	814	0.05%	0.006%
98	14.800	4261	4264	4267	rBV2	1060	859	0.05%	0.006%
99	14.910	4295	4298	4300	rBV2	1128	785	0.04%	0.006%
100	15.479	4472	4475	4477	rBV2	1190	921	0.05%	0.006%


Sum of corrected areas: 14260038

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030218.D
Acq On : 20 Mar 2019 09:44
Operator : JC/SP
Sample : VU0320WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

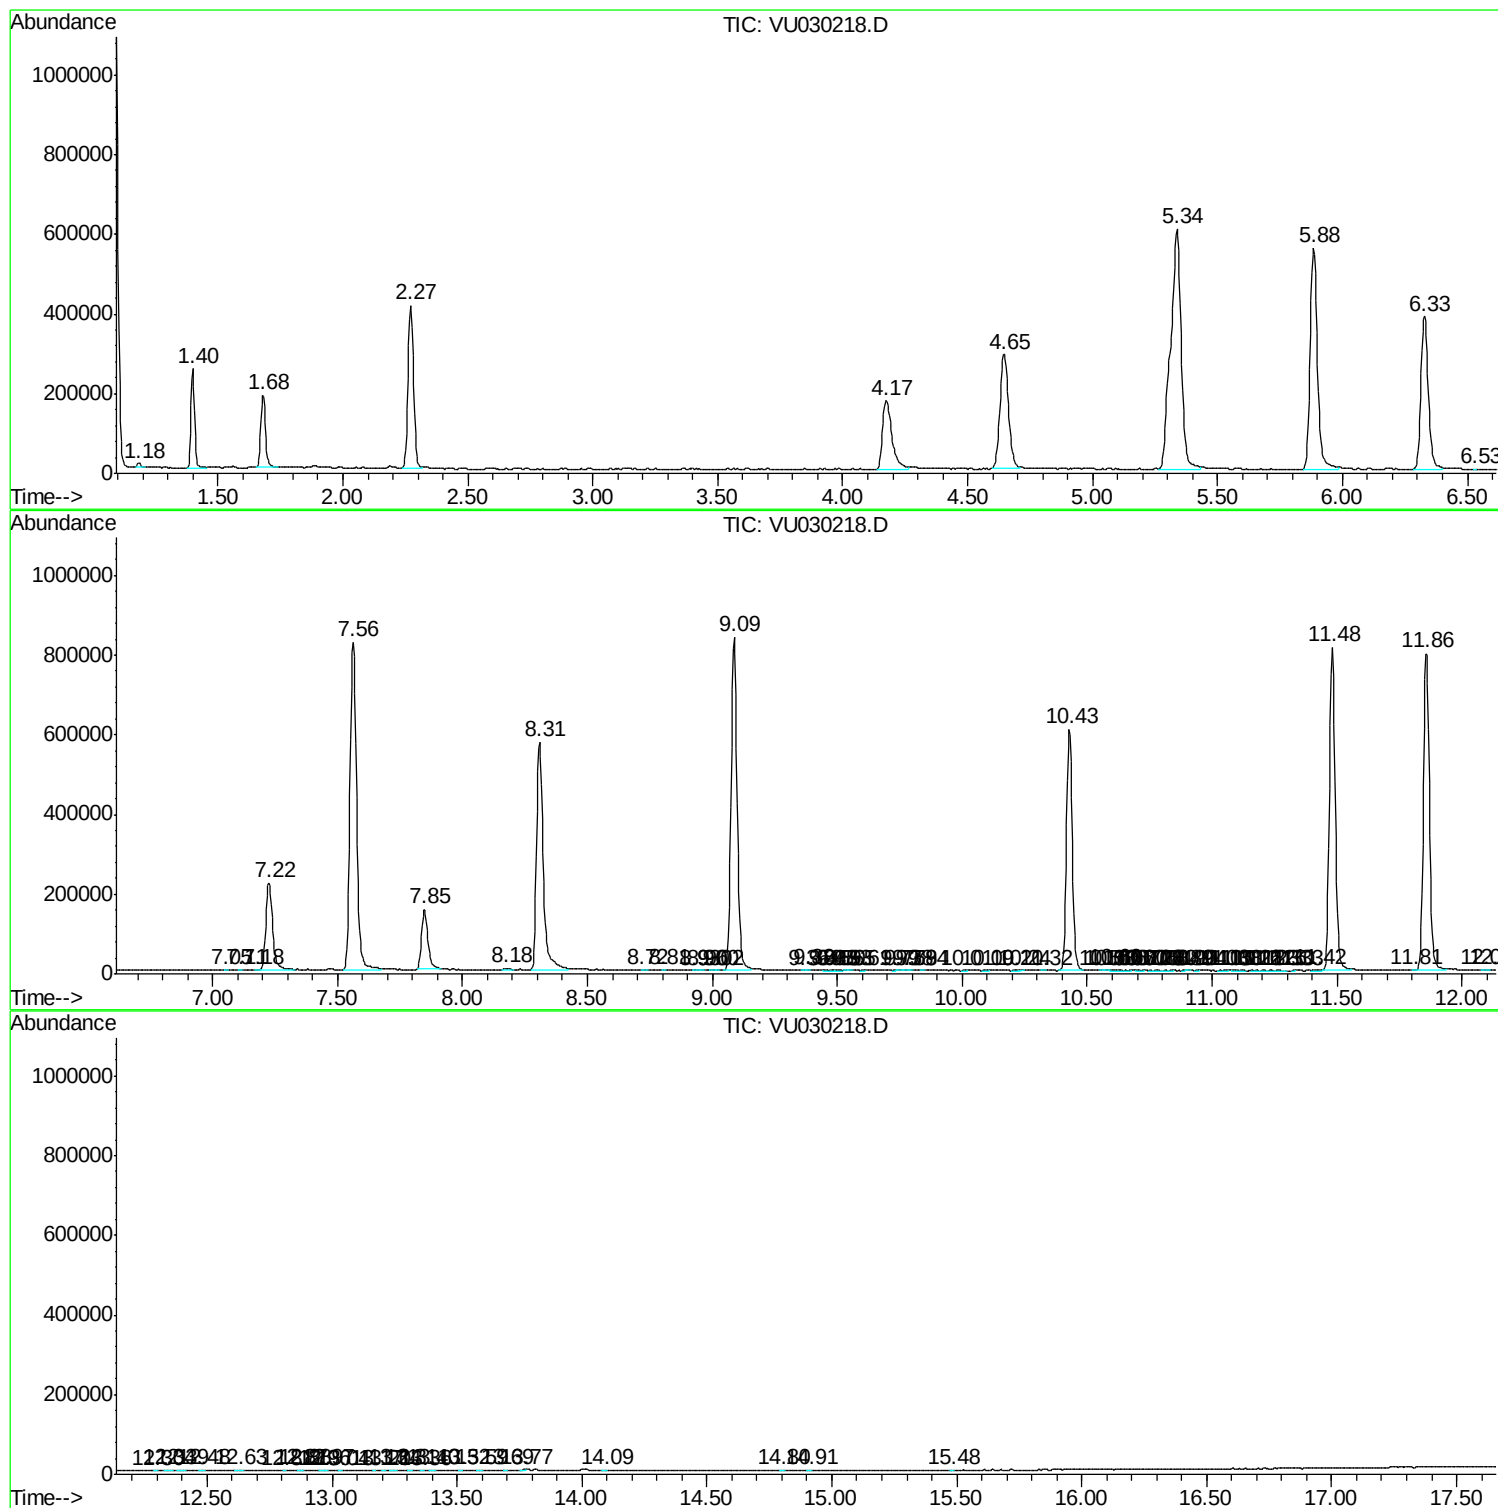

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030218.D
Acq On : 20 Mar 2019 09:44
Operator : JC/SP
Sample : VU0320WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030218.D
Acq On : 20 Mar 2019 09:44
Operator : JC/SP
Sample : VU0320WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc