

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030221.D
 Acq On : 20 Mar 2019 11:01
 Operator : JC/SP
 Sample : K1967-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB2	11454	10884	0.59%	0.075%
2	1.399	89	96	112	rBV	268549	269929	14.54%	1.851%
3	1.678	175	183	203	rVB	193667	247356	13.33%	1.696%
4	2.270	356	367	381	rBV	432762	656382	35.37%	4.500%
5	2.849	545	547	553	rVB	1545	1024	0.06%	0.007%
6	2.891	553	560	563	rBV3	1505	1975	0.11%	0.014%
7	2.990	588	591	594	rBV	1122	753	0.04%	0.005%
8	3.032	601	604	607	rBV	973	742	0.04%	0.005%
9	3.190	650	653	660	rBV4	1014	915	0.05%	0.006%
10	3.350	699	703	705	rBV	1076	878	0.05%	0.006%
11	3.473	739	741	745	rVB	1884	1276	0.07%	0.009%
12	3.508	745	752	759	rBV	1270	1893	0.10%	0.013%
13	3.540	759	762	767	rBV2	695	769	0.04%	0.005%
14	3.682	802	806	809	rBV	1328	1200	0.06%	0.008%
15	3.778	834	836	840	rBV	902	899	0.05%	0.006%
16	3.948	886	889	893	rVB	1171	839	0.05%	0.006%
17	4.000	902	905	912	rVB	1511	1165	0.06%	0.008%
18	4.039	912	917	920	rBV	901	826	0.04%	0.006%
19	4.174	947	959	989	rBV	159058	421261	22.70%	2.888%
20	4.514	1062	1065	1070	rBV2	749	699	0.04%	0.005%
21	4.643	1088	1105	1135	rVV	301272	722591	38.93%	4.954%
22	4.846	1163	1168	1173	rBV3	1075	1248	0.07%	0.009%
23	4.874	1173	1177	1184	rVV4	1638	2255	0.12%	0.015%
24	4.920	1188	1191	1197	rVB	1381	1121	0.06%	0.008%
25	4.961	1197	1204	1208	rBV	1625	1965	0.11%	0.013%
26	5.074	1236	1239	1244	rBV3	848	901	0.05%	0.006%
27	5.337	1297	1321	1359	rVV2	633503	1855964	100.00%	12.724%
28	5.511	1373	1375	1378	rVB2	1398	684	0.04%	0.005%
29	5.534	1379	1382	1387	rVB	1739	1327	0.07%	0.009%
30	5.559	1387	1390	1397	rBV2	917	1001	0.05%	0.007%
31	5.643	1412	1416	1421	rBV2	1033	940	0.05%	0.006%
32	5.717	1434	1439	1441	rBV3	769	778	0.04%	0.005%
33	5.884	1476	1491	1522	rBV	576764	1172494	63.17%	8.039%
34	6.180	1575	1583	1592	rBV6	1817	3469	0.19%	0.024%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030221.D
 Acq On : 20 Mar 2019 11:01
 Operator : JC/SP
 Sample : K1967-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.228	1596	1598	1608	rVB	1509	1564	0.08%	0.011%
36	6.328	1612	1629	1650	rBV	396953	812041	43.75%	5.567%
37	6.572	1699	1705	1707	rBV4	820	760	0.04%	0.005%
38	6.665	1731	1734	1737	rVV2	1115	781	0.04%	0.005%
39	6.704	1743	1746	1751	rVB	872	744	0.04%	0.005%
40	6.739	1753	1757	1763	rBV	588	712	0.04%	0.005%
41	6.897	1802	1806	1809	rBV2	1191	1250	0.07%	0.009%
42	7.003	1836	1839	1842	rVB	1073	736	0.04%	0.005%
43	7.048	1847	1853	1857	rVV2	812	1056	0.06%	0.007%
44	7.161	1884	1888	1891	rBV	1090	942	0.05%	0.006%
45	7.225	1897	1908	1936	rBV	216636	401742	21.65%	2.754%
46	7.469	1981	1984	1990	rVV2	1270	1322	0.07%	0.009%
47	7.562	1999	2013	2047	rBV	867121	1524842	82.16%	10.454%
48	7.849	2090	2102	2123	rBV	148839	265765	14.32%	1.822%
49	7.974	2136	2141	2147	rVB2	1501	1876	0.10%	0.013%
50	8.064	2164	2169	2174	rVB3	1657	1659	0.09%	0.011%
51	8.148	2192	2195	2198	rBV2	875	701	0.04%	0.005%
52	8.180	2198	2205	2213	rVV3	4040	7162	0.39%	0.049%
53	8.228	2217	2220	2223	rBV	1897	1627	0.09%	0.011%
54	8.308	2233	2245	2284	rBV	542330	1003379	54.06%	6.879%
55	8.556	2319	2322	2330	rVB	1833	1906	0.10%	0.013%
56	8.688	2360	2363	2366	rBV2	1221	1021	0.06%	0.007%
57	8.749	2379	2382	2386	rVB2	1283	877	0.05%	0.006%
58	8.794	2393	2396	2403	rVB4	1098	1204	0.06%	0.008%
59	8.890	2422	2426	2431	rVB3	1451	1115	0.06%	0.008%
60	8.916	2431	2434	2440	rBV2	1418	1770	0.10%	0.012%
61	9.087	2474	2487	2520	rBV	860633	1446530	77.94%	9.917%
62	9.337	2561	2565	2570	rBV3	980	975	0.05%	0.007%
63	9.373	2574	2576	2579	rVV2	1301	723	0.04%	0.005%
64	9.569	2633	2637	2641	rBV3	1385	1393	0.08%	0.010%
65	9.617	2649	2652	2655	rBV	1323	993	0.05%	0.007%
66	9.784	2699	2704	2705	rBV	1009	879	0.05%	0.006%
67	9.890	2732	2737	2739	rBV2	1185	943	0.05%	0.006%
68	10.115	2803	2807	2814	rVB4	1154	1455	0.08%	0.010%
69	10.350	2878	2880	2885	rVB	1282	783	0.04%	0.005%
70	10.427	2892	2904	2931	rBV	606107	969082	52.21%	6.644%
71	10.601	2953	2958	2962	rBV5	2554	3377	0.18%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030221.D
 Acq On : 20 Mar 2019 11:01
 Operator : JC/SP
 Sample : K1967-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.746	2998	3003	3009	rVB2	794	805	0.04%	0.006%
73	10.820	3023	3026	3035	rBV3	864	1303	0.07%	0.009%
74	10.874	3040	3043	3049	rVB2	1025	809	0.04%	0.006%
75	11.157	3125	3131	3133	rBV2	1009	977	0.05%	0.007%
76	11.173	3133	3136	3140	rVB	1369	892	0.05%	0.006%
77	11.321	3177	3182	3187	rBV	833	816	0.04%	0.006%
78	11.414	3207	3211	3213	rBV2	1369	1138	0.06%	0.008%
79	11.482	3219	3232	3257	rBV	825843	1344369	72.44%	9.217%
80	11.858	3336	3349	3374	rBV	819028	1356745	73.10%	9.302%
81	12.353	3499	3503	3506	rBV3	1277	1125	0.06%	0.008%
82	12.450	3527	3533	3536	rBV3	1141	1355	0.07%	0.009%
83	12.537	3555	3560	3562	rBV3	1000	866	0.05%	0.006%
84	12.707	3607	3613	3616	rBV	1000	1290	0.07%	0.009%
85	12.803	3639	3643	3649	rBV	1364	1464	0.08%	0.010%
86	12.922	3674	3680	3682	rBV2	1515	1480	0.08%	0.010%
87	13.028	3708	3713	3715	rBV2	856	1016	0.05%	0.007%
88	13.125	3741	3743	3747	rVB3	1234	734	0.04%	0.005%
89	13.466	3846	3849	3853	rBV	1263	1011	0.05%	0.007%
90	13.508	3859	3862	3866	rBV	1019	831	0.04%	0.006%
91	13.649	3903	3906	3911	rVB	1364	967	0.05%	0.007%
92	13.746	3933	3936	3938	rBV	1054	679	0.04%	0.005%
93	14.061	4031	4034	4037	rBV2	1489	981	0.05%	0.007%
94	14.372	4127	4131	4134	rBV	1295	1124	0.06%	0.008%
95	14.401	4137	4140	4144	rVV2	872	698	0.04%	0.005%
96	15.070	4345	4348	4355	rVB3	1474	1581	0.09%	0.011%
97	15.102	4355	4358	4362	rBV2	1195	902	0.05%	0.006%
98	15.344	4429	4433	4437	rBV2	1899	1853	0.10%	0.013%
99	15.424	4453	4458	4464	rBV2	1937	2331	0.13%	0.016%
100	15.585	4505	4508	4515	rVB4	1321	1663	0.09%	0.011%


Sum of corrected areas: 14585895

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030221.D
Acq On : 20 Mar 2019 11:01
Operator : JC/SP
Sample : K1967-16
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

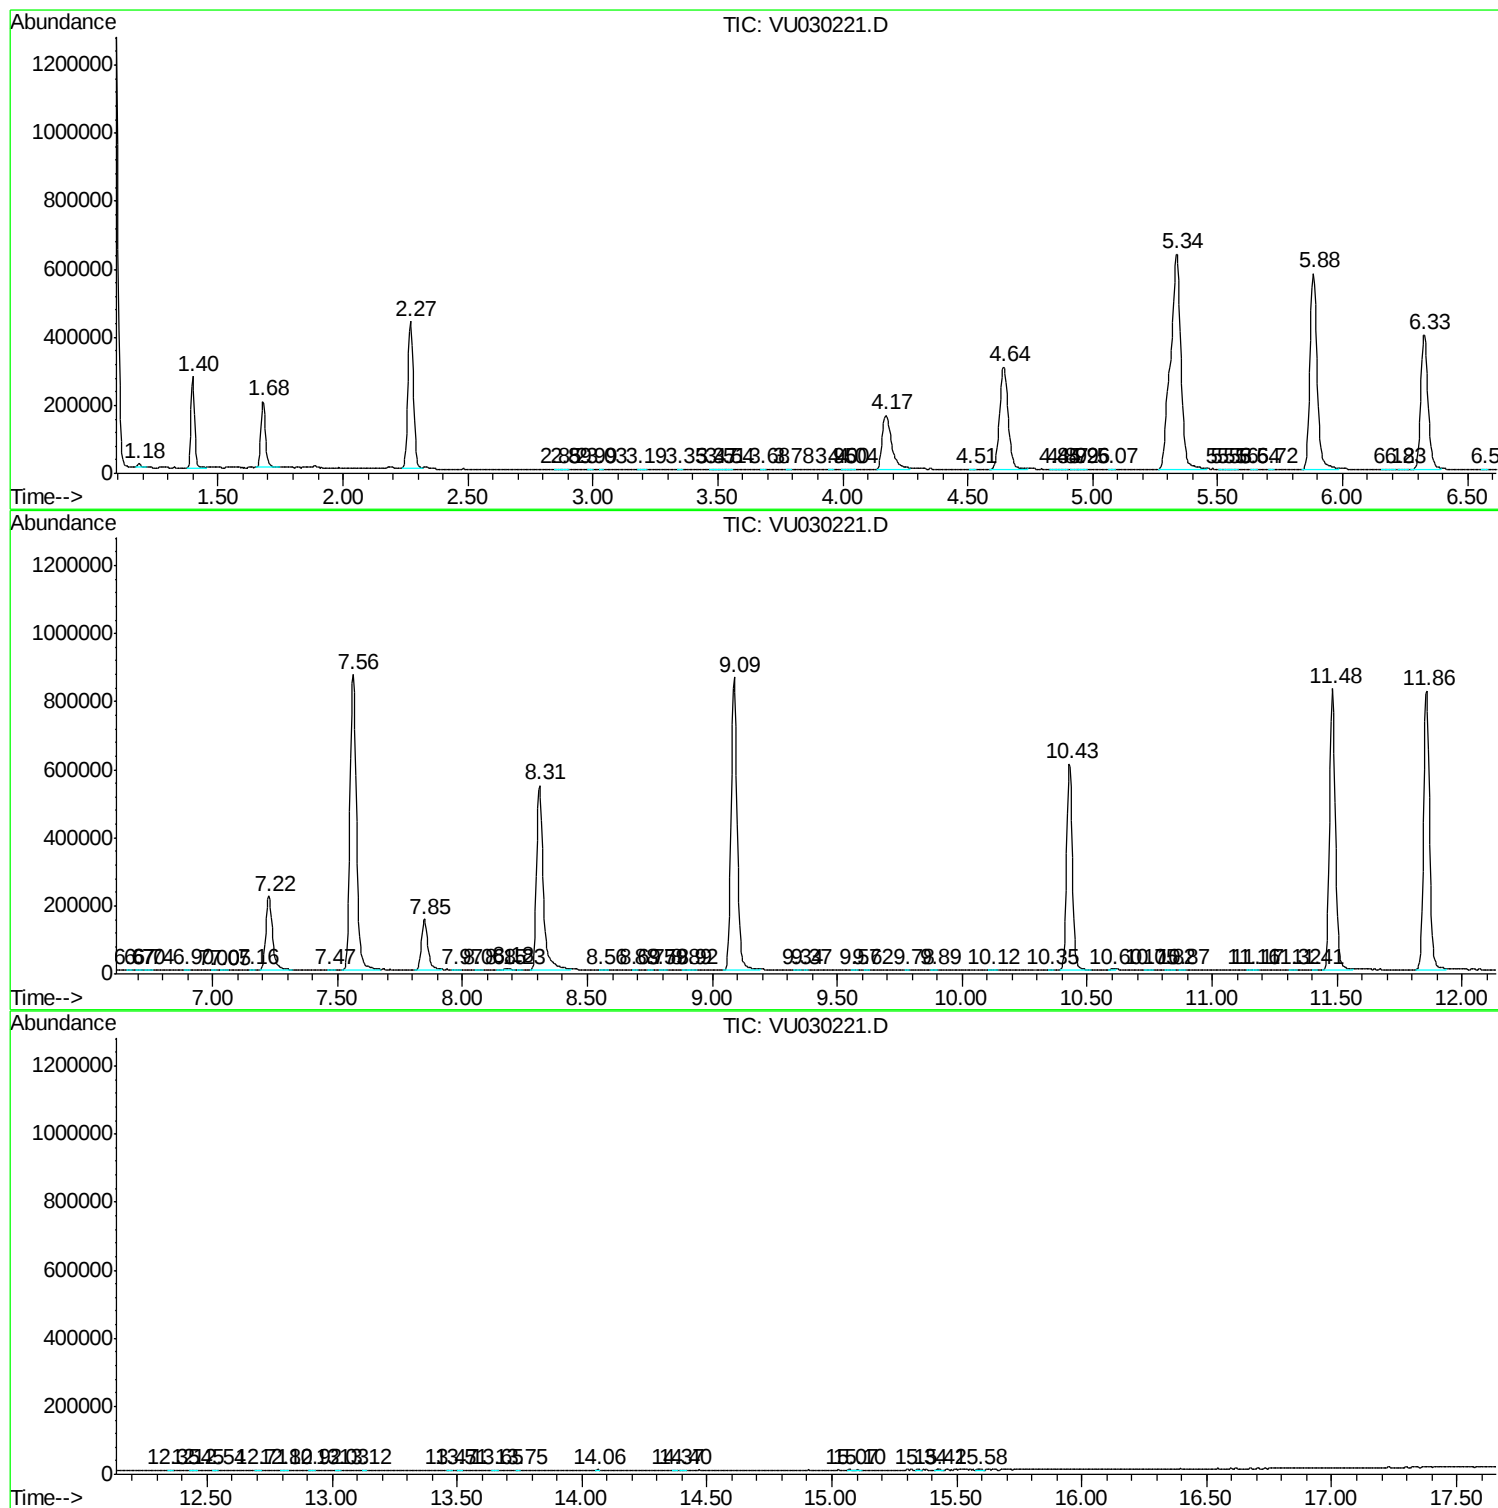

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030221.D
Acq On : 20 Mar 2019 11:01
Operator : JC/SP
Sample : K1967-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030221.D
Acq On : 20 Mar 2019 11:01
Operator : JC/SP
Sample : K1967-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc