

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030223.D
 Acq On : 20 Mar 2019 15:31
 Operator : JC/SP
 Sample : K2017-05 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB2	11183	11041	0.68%	0.084%
2	1.399	89	96	110	rBV	221952	224654	13.94%	1.717%
3	1.682	176	184	198	rVB	160236	200369	12.43%	1.531%
4	2.273	357	368	381	rBV	356268	540504	33.53%	4.130%
5	2.540	445	451	452	rBV	992	907	0.06%	0.007%
6	2.653	483	486	490	rVB	862	615	0.04%	0.005%
7	2.688	494	497	498	rBV	1407	758	0.05%	0.006%
8	2.756	513	518	520	rBV	791	797	0.05%	0.006%
9	2.804	530	533	538	rBV	1428	1436	0.09%	0.011%
10	2.842	542	545	548	rBV	1232	782	0.05%	0.006%
11	2.881	554	557	560	rBV	1055	694	0.04%	0.005%
12	2.997	586	593	596	rBV	1832	1743	0.11%	0.013%
13	3.023	596	601	609	rVB	1272	1955	0.12%	0.015%
14	3.058	609	612	613	rBV	996	592	0.04%	0.005%
15	3.074	614	617	621	rVB	838	608	0.04%	0.005%
16	3.125	629	633	636	rVB	1341	1046	0.06%	0.008%
17	3.151	636	641	644	rBV	1780	1691	0.10%	0.013%
18	3.199	652	656	659	rVB	1113	878	0.05%	0.007%
19	3.232	663	666	670	rBV	692	666	0.04%	0.005%
20	3.331	692	697	702	rBV2	1791	2398	0.15%	0.018%
21	3.357	702	705	708	rBV	1177	826	0.05%	0.006%
22	3.444	729	732	735	rBV	785	590	0.04%	0.005%
23	3.498	746	749	752	rVB	1242	869	0.05%	0.007%
24	3.556	764	767	771	rVB	1375	946	0.06%	0.007%
25	3.582	771	775	779	rVB	1501	1298	0.08%	0.010%
26	3.624	779	788	791	rBV	2058	2682	0.17%	0.020%
27	3.669	799	802	807	rBV	1600	1116	0.07%	0.009%
28	3.743	823	825	829	rVB2	1315	810	0.05%	0.006%
29	3.788	831	839	841	rBV	1373	1756	0.11%	0.013%
30	3.852	856	859	863	rVB	1763	1271	0.08%	0.010%
31	3.884	863	869	871	rBV	1162	978	0.06%	0.007%
32	3.965	888	894	897	rBV	926	1272	0.08%	0.010%
33	4.090	927	933	936	rBV	1775	1725	0.11%	0.013%
34	4.177	946	960	988	rBV	132272	346212	21.48%	2.646%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030223.D
 Acq On : 20 Mar 2019 15:31
 Operator : JC/SP
 Sample : K2017-05 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	4.460	1044	1048	1051	rBV	1404	1275	0.08%	0.010%
36	4.550	1073	1076	1078	rBV	1328	774	0.05%	0.006%
37	4.646	1089	1106	1128	rBV	245044	577855	35.85%	4.416%
38	5.035	1224	1227	1228	rBV	1237	710	0.04%	0.005%
39	5.103	1244	1248	1250	rBV	1241	971	0.06%	0.007%
40	5.148	1260	1262	1265	rBV	1101	709	0.04%	0.005%
41	5.193	1273	1276	1278	rBV	1165	634	0.04%	0.005%
42	5.338	1298	1321	1357	rBV2	505043	1483408	92.03%	11.336%
43	5.514	1373	1376	1380	rBV3	1137	773	0.05%	0.006%
44	5.540	1381	1384	1389	rVB	1577	1196	0.07%	0.009%
45	5.682	1423	1428	1434	rBV3	1182	1370	0.08%	0.010%
46	5.804	1462	1466	1468	rBV2	1225	962	0.06%	0.007%
47	5.884	1477	1491	1527	rBV	649257	1312202	81.41%	10.027%
48	6.074	1547	1550	1552	rBV	1078	756	0.05%	0.006%
49	6.193	1584	1587	1589	rBV	1173	900	0.06%	0.007%
50	6.328	1615	1629	1655	rBV	313505	647968	40.20%	4.952%
51	6.659	1727	1732	1735	rBV	1103	1096	0.07%	0.008%
52	6.698	1741	1744	1746	rBV2	1396	879	0.05%	0.007%
53	6.739	1754	1757	1760	rBV	1398	823	0.05%	0.006%
54	6.791	1766	1773	1776	rBV	1683	2042	0.13%	0.016%
55	6.852	1786	1792	1795	rBV3	1233	1320	0.08%	0.010%
56	6.926	1809	1815	1818	rBV	1401	1327	0.08%	0.010%
57	7.119	1872	1875	1881	rVB	1622	1441	0.09%	0.011%
58	7.145	1881	1883	1886	rBV	1038	676	0.04%	0.005%
59	7.225	1897	1908	1933	rBV	183889	337631	20.95%	2.580%
60	7.328	1938	1940	1944	rVB	1734	1176	0.07%	0.009%
61	7.354	1944	1948	1950	rBV2	1098	866	0.05%	0.007%
62	7.450	1975	1978	1980	rBV	965	666	0.04%	0.005%
63	7.563	2001	2013	2032	rBV	691486	1215790	75.43%	9.291%
64	7.849	2091	2102	2120	rBV	124697	228348	14.17%	1.745%
65	8.170	2197	2202	2205	rBV3	2580	2755	0.17%	0.021%
66	8.228	2214	2220	2232	rVB5	10937	16515	1.02%	0.126%
67	8.308	2234	2245	2277	rBV	442281	809287	50.21%	6.184%
68	8.588	2328	2332	2336	rBV	2060	1564	0.10%	0.012%
69	9.087	2474	2487	2512	rBV	961708	1611885	100.00%	12.318%
70	9.498	2610	2615	2621	rBV	2528	2993	0.19%	0.023%
71	9.598	2643	2646	2648	rBV	1104	752	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030223.D
 Acq On : 20 Mar 2019 15:31
 Operator : JC/SP
 Sample : K2017-05 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	9.762	2694	2697	2700	rVV	1345	989	0.06%	0.008%
73	9.855	2724	2726	2729	rVB	1256	704	0.04%	0.005%
74	9.984	2762	2766	2769	rBV	2042	1687	0.10%	0.013%
75	10.205	2832	2835	2838	rBV	1400	1260	0.08%	0.010%
76	10.427	2892	2904	2923	rBV	491549	791370	49.10%	6.047%
77	10.604	2953	2959	2964	rBV3	2770	4242	0.26%	0.032%
78	10.730	2996	2998	3003	rBV	854	785	0.05%	0.006%
79	10.932	3058	3061	3063	rBV	1448	845	0.05%	0.006%
80	11.193	3138	3142	3146	rBV3	1716	2157	0.13%	0.016%
81	11.244	3155	3158	3160	rBV2	1499	1084	0.07%	0.008%
82	11.418	3208	3212	3217	rBV5	1641	2232	0.14%	0.017%
83	11.479	3220	3231	3254	rBV	942378	1523544	94.52%	11.642%
84	11.855	3336	3348	3374	rBV	673114	1105627	68.59%	8.449%
85	12.418	3518	3523	3525	rBV	2112	1896	0.12%	0.014%
86	12.807	3641	3644	3648	rVB	1464	1136	0.07%	0.009%
87	13.713	3917	3926	3929	rBV	2402	3231	0.20%	0.025%
88	13.762	3937	3941	3944	rBV	1804	1513	0.09%	0.012%
89	13.807	3952	3955	3958	rBV	1273	1150	0.07%	0.009%
90	13.861	3969	3972	3974	rBV	1010	693	0.04%	0.005%
91	13.990	4009	4012	4014	rBV2	1155	709	0.04%	0.005%
92	14.305	4106	4110	4112	rBV	1192	1041	0.06%	0.008%
93	14.926	4300	4303	4306	rBV	1238	764	0.05%	0.006%
94	14.945	4306	4309	4312	rBV	1047	596	0.04%	0.005%
95	15.048	4337	4341	4345	rBV	1497	1290	0.08%	0.010%
96	15.443	4461	4464	4467	rBV	1174	1174	0.07%	0.009%
97	15.485	4475	4477	4484	rVB3	1996	1986	0.12%	0.015%
98	15.520	4484	4488	4491	rBV2	1970	2062	0.13%	0.016%
99	15.591	4507	4510	4512	rBV	1396	927	0.06%	0.007%
100	16.048	4650	4652	4655	rVB4	1310	629	0.04%	0.005%


Sum of corrected areas: 13086103

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030223.D
Acq On : 20 Mar 2019 15:31
Operator : JC/SP
Sample : K2017-05 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

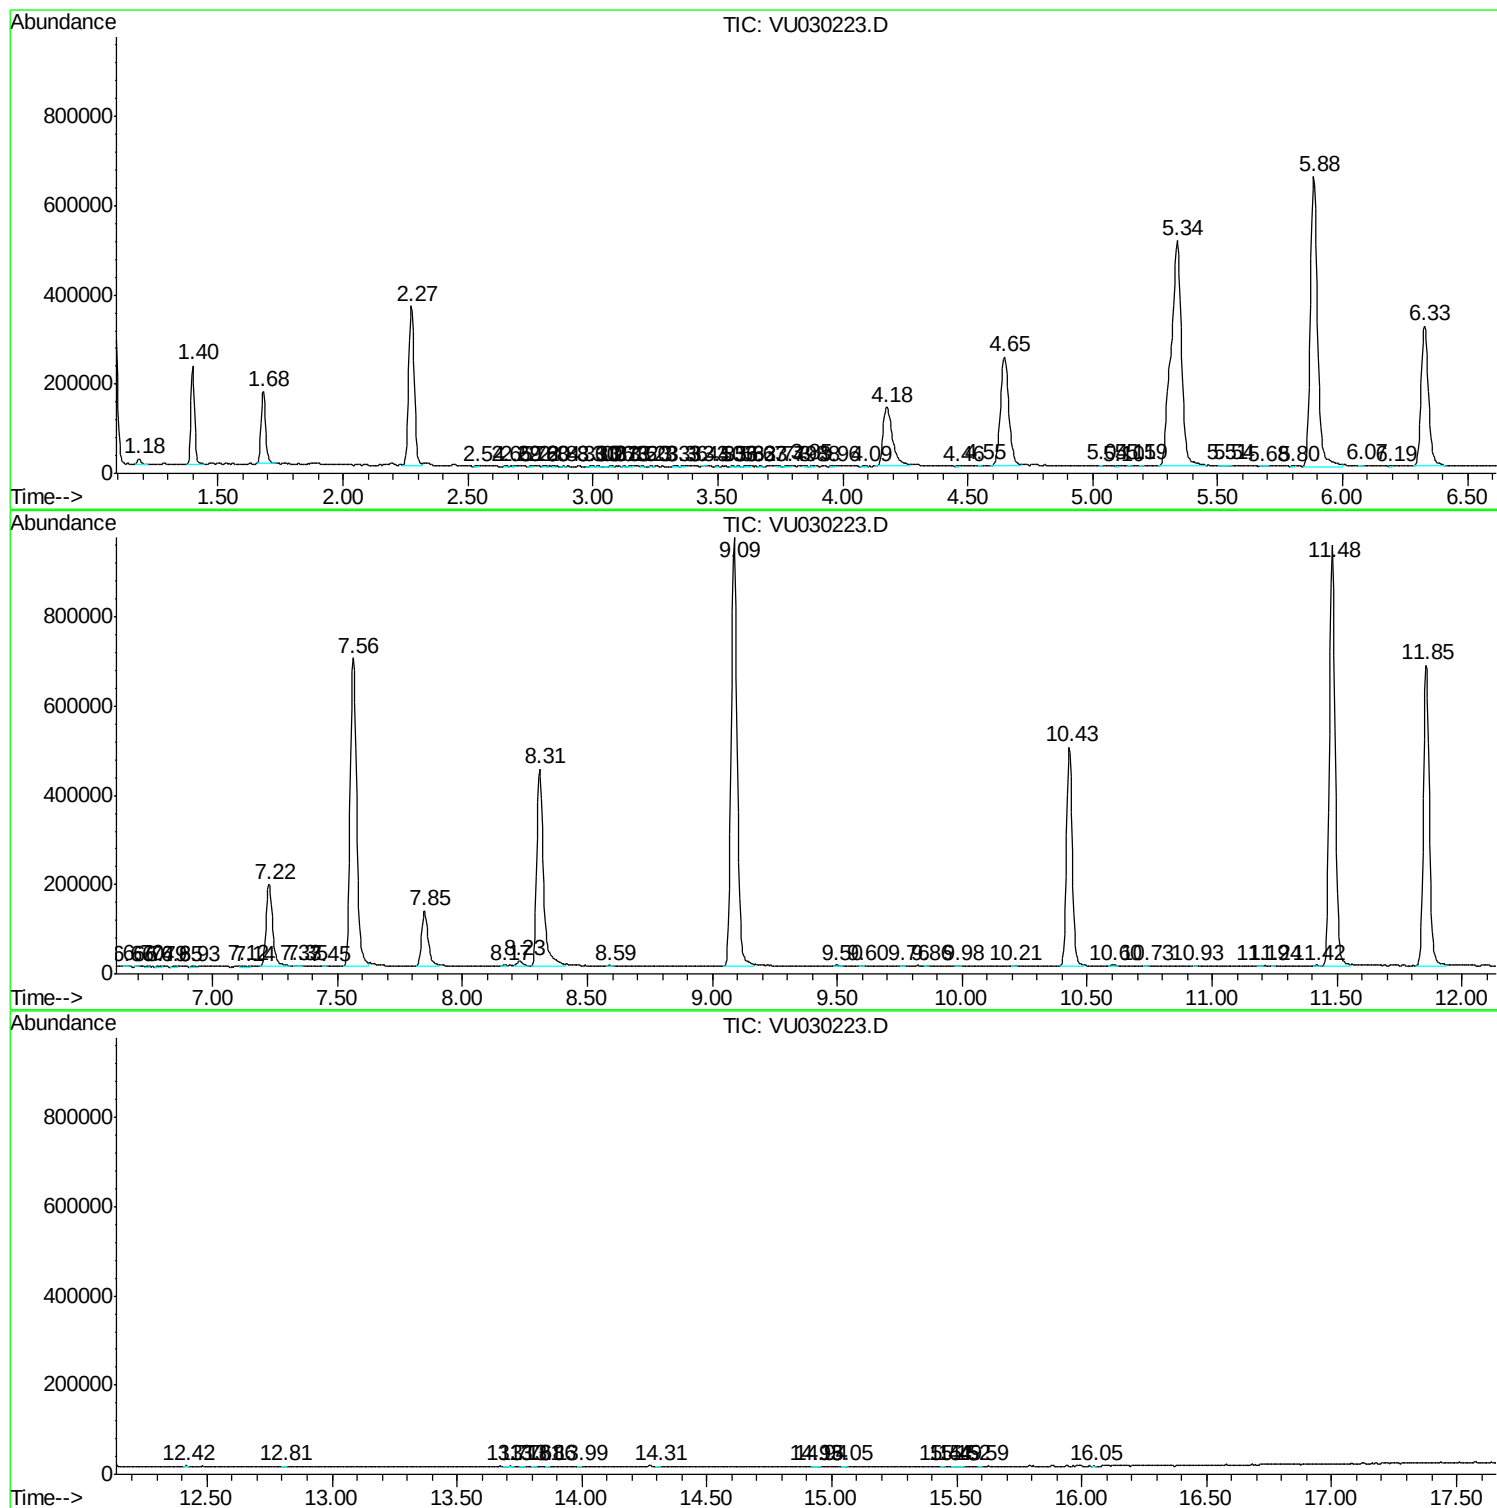

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030223.D
Acq On : 20 Mar 2019 15:31
Operator : JC/SP
Sample : K2017-05 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030223.D
Acq On : 20 Mar 2019 15:31
Operator : JC/SP
Sample : K2017-05 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc