

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030225.D
 Acq On : 20 Mar 2019 16:21
 Operator : JC/SP
 Sample : VU0320WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rBV	12388	12086	0.67%	0.085%
2	1.399	89	96	105	rBV	263397	262685	14.55%	1.850%
3	1.678	175	183	205	rVB	190639	242236	13.41%	1.706%
4	2.270	356	367	381	rBV	424175	642160	35.56%	4.522%
5	2.534	446	449	452	rVB2	1643	1055	0.06%	0.007%
6	2.608	468	472	477	rBV	1681	1680	0.09%	0.012%
7	2.923	567	570	572	rBV	1434	1012	0.06%	0.007%
8	3.061	610	613	623	rVB	1773	1822	0.10%	0.013%
9	3.604	778	782	785	rBV	1542	1271	0.07%	0.009%
10	3.659	796	799	805	rBV	1304	1122	0.06%	0.008%
11	3.717	814	817	821	rBV	1339	996	0.06%	0.007%
12	3.823	846	850	854	rVV	1634	1279	0.07%	0.009%
13	4.035	912	916	920	rVB	1527	1200	0.07%	0.008%
14	4.096	932	935	939	rBV	1427	1073	0.06%	0.008%
15	4.174	947	959	985	rBV	159473	415235	22.99%	2.924%
16	4.643	1087	1105	1129	rBV	296400	707403	39.17%	4.981%
17	4.804	1153	1155	1163	rVB3	928	1160	0.06%	0.008%
18	4.913	1187	1189	1199	rVB	1449	1910	0.11%	0.013%
19	4.981	1205	1210	1213	rBV	1290	1330	0.07%	0.009%
20	5.338	1296	1321	1341	rBV2	619881	1805825	100.00%	12.715%
21	5.630	1409	1412	1417	rBV	1221	1059	0.06%	0.007%
22	5.682	1424	1428	1432	rVB	1584	1155	0.06%	0.008%
23	5.884	1477	1491	1511	rBV	528015	1058556	58.62%	7.453%
24	6.180	1579	1583	1585	rBV2	1472	1348	0.07%	0.009%
25	6.276	1610	1613	1615	rBV	1500	1068	0.06%	0.008%
26	6.328	1615	1629	1658	rVV	390876	798558	44.22%	5.623%
27	6.582	1702	1708	1710	rBV2	1375	1229	0.07%	0.009%
28	6.662	1731	1733	1739	rVB	1765	1257	0.07%	0.009%
29	6.784	1768	1771	1777	rBV2	1184	1219	0.07%	0.009%
30	6.897	1800	1806	1810	rBV2	843	1211	0.07%	0.009%
31	6.923	1811	1814	1822	rVV2	1244	1780	0.10%	0.013%
32	7.048	1850	1853	1861	rBV3	1321	1798	0.10%	0.013%
33	7.225	1894	1908	1927	rBV	211506	387939	21.48%	2.732%
34	7.415	1963	1967	1970	rVB	1389	993	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030225.D
 Acq On : 20 Mar 2019 16:21
 Operator : JC/SP
 Sample : VU0320WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.466	1976	1983	1992	rBV3	4494	7457	0.41%	0.053%
36	7.562	1999	2013	2046	rBV	830891	1504318	83.30%	10.592%
37	7.775	2074	2079	2085	rVB3	1286	1393	0.08%	0.010%
38	7.849	2090	2102	2121	rBV	143013	260019	14.40%	1.831%
39	8.045	2160	2163	2167	rVB	1915	1686	0.09%	0.012%
40	8.070	2167	2171	2174	rBV	2002	1395	0.08%	0.010%
41	8.099	2174	2180	2185	rVV2	1337	1850	0.10%	0.013%
42	8.164	2197	2200	2210	rBV3	2606	4025	0.22%	0.028%
43	8.231	2217	2221	2227	rBV2	1968	1955	0.11%	0.014%
44	8.308	2232	2245	2272	rBV	535686	992034	54.94%	6.985%
45	8.736	2373	2378	2382	rVB2	1191	1138	0.06%	0.008%
46	8.916	2429	2434	2436	rBV	1189	999	0.06%	0.007%
47	9.087	2472	2487	2509	rBV	789450	1326069	73.43%	9.337%
48	9.247	2531	2537	2541	rBV4	2144	2893	0.16%	0.020%
49	9.350	2566	2569	2572	rBV	1425	1065	0.06%	0.007%
50	9.379	2572	2578	2584	rVV5	2292	3694	0.20%	0.026%
51	9.408	2585	2587	2592	rVV	1513	1112	0.06%	0.008%
52	9.476	2603	2608	2611	rVB	1230	1113	0.06%	0.008%
53	9.501	2611	2616	2619	rVB	1667	1434	0.08%	0.010%
54	9.524	2619	2623	2625	rBV	1295	1044	0.06%	0.007%
55	9.575	2633	2639	2643	rVB	1465	1492	0.08%	0.011%
56	9.685	2668	2673	2677	rBV	1089	1318	0.07%	0.009%
57	9.778	2698	2702	2704	rBV2	2106	1717	0.10%	0.012%
58	9.996	2763	2770	2773	rBV2	1504	1644	0.09%	0.012%
59	10.029	2774	2780	2783	rVV	899	1143	0.06%	0.008%
60	10.090	2794	2799	2801	rBV	1476	1191	0.07%	0.008%
61	10.164	2818	2822	2823	rBV	2007	1427	0.08%	0.010%
62	10.244	2843	2847	2853	rBV2	1576	1480	0.08%	0.010%
63	10.347	2876	2879	2884	rVB2	1510	1012	0.06%	0.007%
64	10.427	2890	2904	2923	rBV	593185	962788	53.32%	6.779%
65	10.559	2940	2945	2950	rVB	1335	1463	0.08%	0.010%
66	10.607	2953	2960	2965	rBV2	2419	2839	0.16%	0.020%
67	10.688	2981	2985	2991	rBV	1807	1839	0.10%	0.013%
68	10.826	3023	3028	3033	rBV2	1344	1882	0.10%	0.013%
69	10.903	3049	3052	3062	rVB2	1210	1792	0.10%	0.013%
70	11.244	3155	3158	3164	rBV	1308	1161	0.06%	0.008%
71	11.308	3175	3178	3182	rBV	1650	1141	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030225.D
 Acq On : 20 Mar 2019 16:21
 Operator : JC/SP
 Sample : VU0320WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.424	3205	3214	3221	rBV5	5223	9415	0.52%	0.066%
73	11.482	3221	3232	3252	rBV	770979	1256124	69.56%	8.845%
74	11.633	3276	3279	3287	rVB	1886	1596	0.09%	0.011%
75	11.858	3336	3349	3369	rBV	815962	1351042	74.82%	9.513%
76	12.086	3417	3420	3421	rBV2	1732	1051	0.06%	0.007%
77	12.196	3451	3454	3461	rVB3	1712	1714	0.09%	0.012%
78	12.308	3486	3489	3495	rVB	1427	1062	0.06%	0.007%
79	12.340	3495	3499	3503	rBV	1611	1726	0.10%	0.012%
80	12.402	3515	3518	3523	rBV	1376	1085	0.06%	0.008%
81	12.594	3573	3578	3584	rBV2	1283	1824	0.10%	0.013%
82	12.662	3595	3599	3606	rBV3	1873	2614	0.14%	0.018%
83	12.787	3632	3638	3641	rVB	1165	1205	0.07%	0.008%
84	12.836	3650	3653	3659	rBV	1306	1296	0.07%	0.009%
85	12.893	3659	3671	3682	rBV5	8291	14799	0.82%	0.104%
86	12.967	3692	3694	3701	rVB	1646	1804	0.10%	0.013%
87	13.048	3714	3719	3721	rBV	2028	1952	0.11%	0.014%
88	13.344	3806	3811	3816	rBV2	792	1247	0.07%	0.009%
89	13.453	3839	3845	3851	rBV	1188	1514	0.08%	0.011%
90	13.514	3855	3864	3879	rBV5	7526	15885	0.88%	0.112%
91	13.620	3894	3897	3899	rBV	1730	1244	0.07%	0.009%
92	13.755	3929	3939	3954	rBV2	15635	43165	2.39%	0.304%
93	13.990	4003	4012	4013	rBV4	9227	10238	0.57%	0.072%
94	14.257	4092	4095	4101	rVB2	1704	1798	0.10%	0.013%
95	14.289	4101	4105	4109	rBV	1595	1828	0.10%	0.013%
96	14.633	4209	4212	4216	rVV	2050	1356	0.08%	0.010%
97	15.032	4329	4336	4339	rBV3	1588	2102	0.12%	0.015%
98	15.157	4371	4375	4378	rBV	1463	1482	0.08%	0.010%
99	15.321	4423	4426	4429	rBV2	1676	1047	0.06%	0.007%
100	15.491	4476	4479	4483	rBV	1486	1230	0.07%	0.009%


Sum of corrected areas: 14202177

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030225.D
Acq On : 20 Mar 2019 16:21
Operator : JC/SP
Sample : VU0320WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VBLK42

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

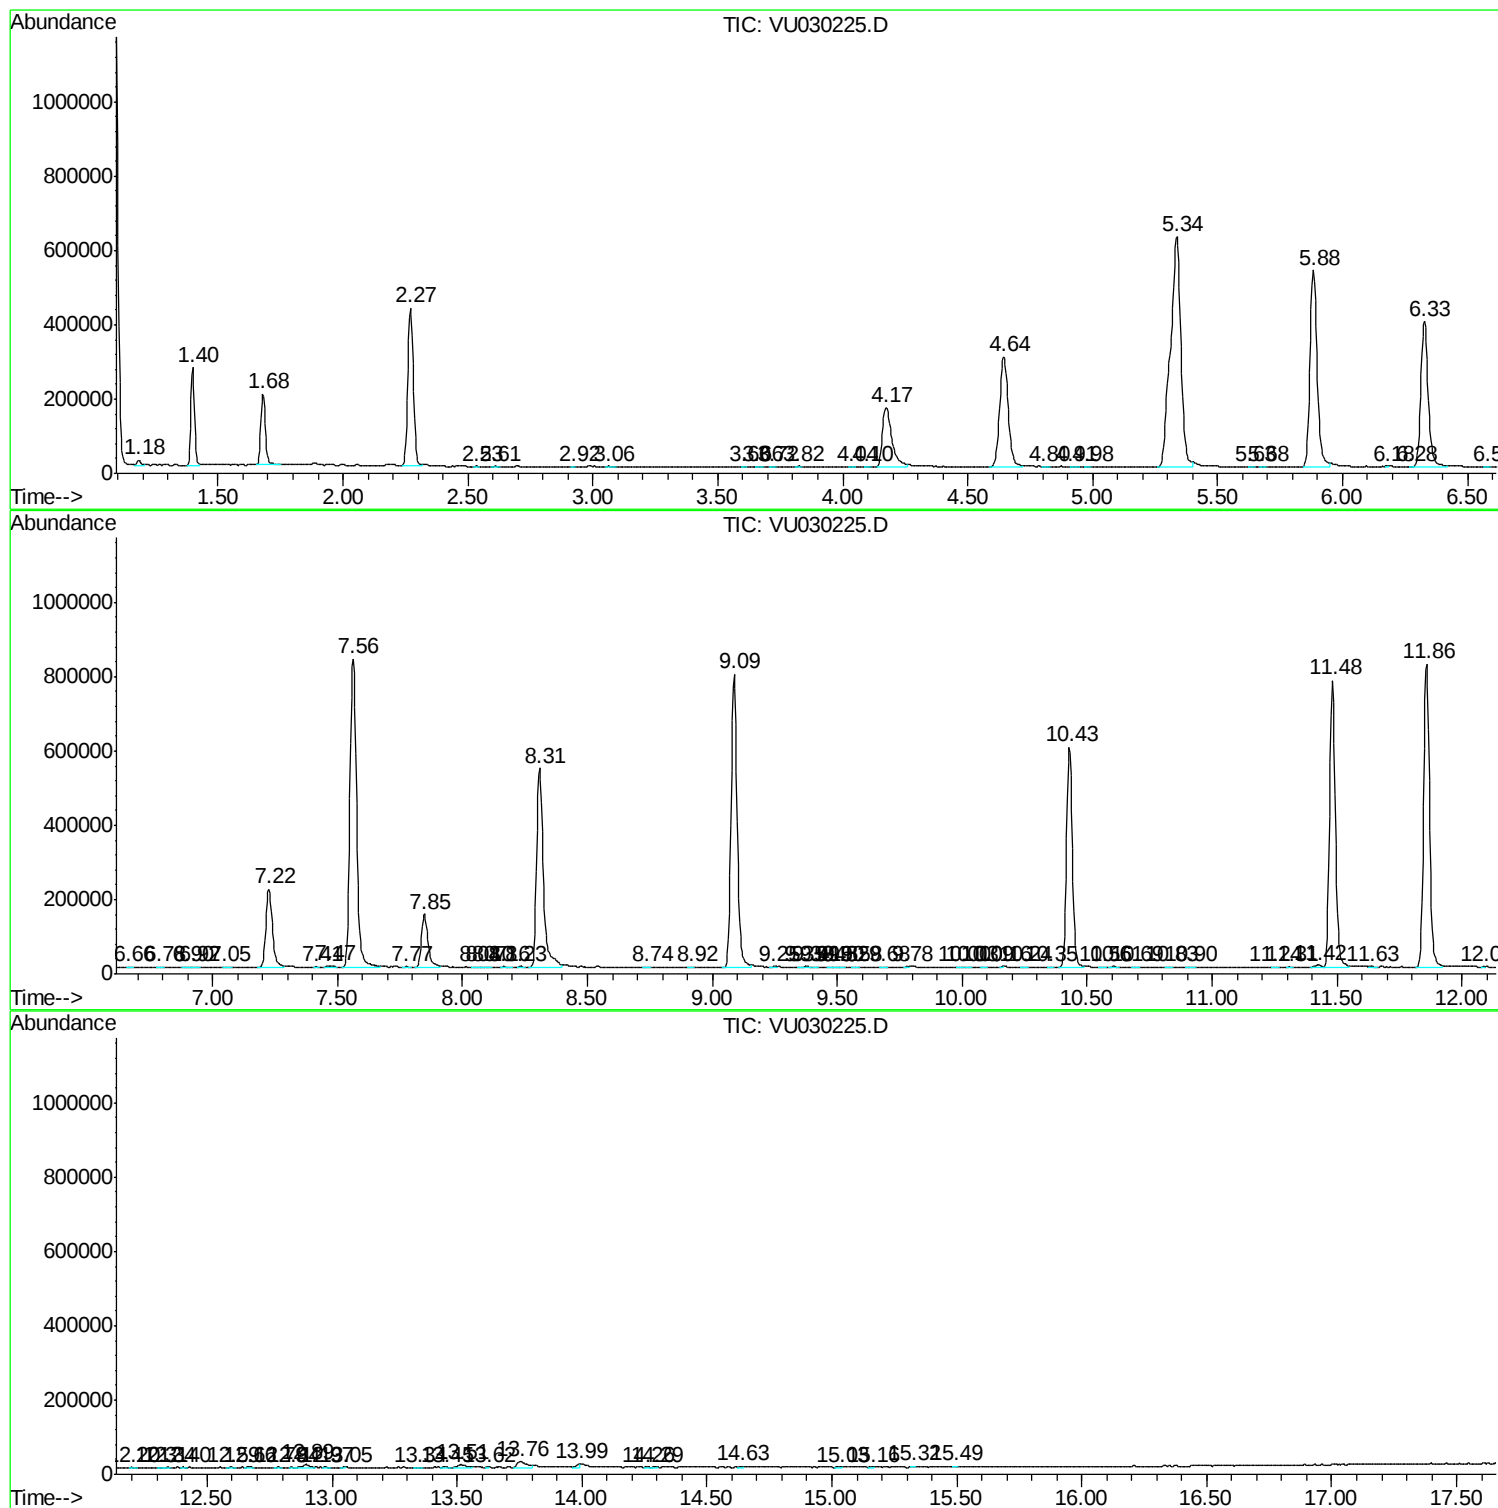

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030225.D
Acq On : 20 Mar 2019 16:21
Operator : JC/SP
Sample : VU0320WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK42

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030225.D
Acq On : 20 Mar 2019 16:21
Operator : JC/SP
Sample : VU0320WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK42

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc