

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030226.D
 Acq On : 20 Mar 2019 16:43
 Operator : JC/SP
 Sample : VU0320MBL02
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	108	rBV	253085	252995	14.19%	1.829%
2	1.678	176	183	199	rBV	182398	230134	12.91%	1.664%
3	2.270	358	367	382	rVB	411053	621082	34.85%	4.491%
4	2.868	550	553	555	rBV	1286	877	0.05%	0.006%
5	3.032	601	604	607	rBV	1318	895	0.05%	0.006%
6	3.167	643	646	651	rBV	1701	1268	0.07%	0.009%
7	3.257	671	674	678	rBV	1286	990	0.06%	0.007%
8	3.305	686	689	693	rBV2	940	905	0.05%	0.007%
9	3.476	740	742	745	rBV	1022	623	0.03%	0.005%
10	3.772	830	834	836	rBV	1054	848	0.05%	0.006%
11	3.948	886	889	891	rBV	388	230	0.01%	0.002%
12	4.000	898	905	909	rBV	1811	2469	0.14%	0.018%
13	4.045	915	919	920	rBV	953	655	0.04%	0.005%
14	4.177	948	960	989	rBV	160392	422554	23.71%	3.055%
15	4.485	1053	1056	1058	rBV	818	615	0.03%	0.004%
16	4.556	1075	1078	1082	rVB	1029	796	0.04%	0.006%
17	4.646	1091	1106	1132	rBV	292994	686436	38.51%	4.963%
18	4.981	1204	1210	1213	rBV	2002	2144	0.12%	0.016%
19	4.997	1213	1215	1218	rVV	1429	827	0.05%	0.006%
20	5.013	1218	1220	1224	rVB	935	547	0.03%	0.004%
21	5.045	1224	1230	1232	rBV2	801	917	0.05%	0.007%
22	5.080	1237	1241	1243	rBV	1622	1189	0.07%	0.009%
23	5.135	1254	1258	1260	rBV	1151	708	0.04%	0.005%
24	5.196	1270	1277	1280	rBV2	1408	1904	0.11%	0.014%
25	5.247	1290	1293	1296	rBV	1301	992	0.06%	0.007%
26	5.337	1299	1321	1353	rVV2	603351	1782346	100.00%	12.887%
27	5.807	1465	1467	1471	rVB2	1353	877	0.05%	0.006%
28	5.839	1471	1477	1478	rBV	1394	1072	0.06%	0.008%
29	5.884	1479	1491	1521	rVV	524363	1055276	59.21%	7.630%
30	6.231	1595	1599	1605	rBV	2298	3257	0.18%	0.024%
31	6.328	1617	1629	1649	rBV	380985	770359	43.22%	5.570%
32	6.652	1728	1730	1733	rBV2	985	609	0.03%	0.004%
33	6.697	1741	1744	1747	rBV	1466	1058	0.06%	0.008%
34	6.868	1794	1797	1799	rBV	861	517	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030226.D
 Acq On : 20 Mar 2019 16:43
 Operator : JC/SP
 Sample : VU0320MBL02
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.926	1812	1815	1821	rBV2	1217	1549	0.09%	0.011%
36	6.955	1822	1824	1829	rVB	1786	1051	0.06%	0.008%
37	6.984	1829	1833	1837	rBV	1061	1110	0.06%	0.008%
38	7.051	1851	1854	1857	rBV	1182	907	0.05%	0.007%
39	7.122	1873	1876	1877	rBV2	933	534	0.03%	0.004%
40	7.148	1882	1884	1886	rBV	919	370	0.02%	0.003%
41	7.225	1897	1908	1931	rBV	207888	381729	21.42%	2.760%
42	7.562	2001	2013	2034	rBV	828081	1457792	81.79%	10.541%
43	7.849	2092	2102	2127	rBV	142843	255065	14.31%	1.844%
44	8.234	2219	2222	2223	rBV	982	579	0.03%	0.004%
45	8.308	2234	2245	2274	rBV	555136	1002919	56.27%	7.252%
46	8.826	2402	2406	2408	rBV	1134	827	0.05%	0.006%
47	8.858	2413	2416	2417	rBV	765	411	0.02%	0.003%
48	8.919	2431	2435	2438	rBV	1320	1062	0.06%	0.008%
49	8.935	2438	2440	2442	rBV2	524	314	0.02%	0.002%
50	9.035	2468	2471	2473	rBV	1016	590	0.03%	0.004%
51	9.086	2474	2487	2516	rBV	776842	1313606	73.70%	9.498%
52	9.292	2548	2551	2560	rBV	1527	1872	0.11%	0.014%
53	9.434	2591	2595	2599	rBV	1002	1067	0.06%	0.008%
54	9.546	2627	2630	2634	rBV	999	957	0.05%	0.007%
55	9.646	2655	2661	2665	rBV	1561	2064	0.12%	0.015%
56	9.713	2678	2682	2685	rVB2	765	667	0.04%	0.005%
57	9.733	2685	2688	2690	rBV2	1659	989	0.06%	0.007%
58	9.913	2742	2744	2746	rBV	452	217	0.01%	0.002%
59	9.932	2746	2750	2757	rVV	1532	1457	0.08%	0.011%
60	9.964	2757	2760	2763	rBV	1149	759	0.04%	0.005%
61	10.057	2786	2789	2791	rBV2	811	509	0.03%	0.004%
62	10.096	2798	2801	2802	rBV2	821	528	0.03%	0.004%
63	10.144	2812	2816	2819	rBV	1480	976	0.05%	0.007%
64	10.176	2819	2826	2832	rVB2	1824	2398	0.13%	0.017%
65	10.209	2832	2836	2843	rBV2	1400	2038	0.11%	0.015%
66	10.266	2850	2854	2859	rBV	1351	1048	0.06%	0.008%
67	10.311	2865	2868	2870	rBV	890	611	0.03%	0.004%
68	10.363	2881	2884	2891	rBV2	1132	1127	0.06%	0.008%
69	10.427	2891	2904	2929	rBV	595538	969195	54.38%	7.008%
70	10.739	2998	3001	3004	rBV	1111	868	0.05%	0.006%
71	10.771	3008	3011	3012	rBV2	1021	639	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030226.D
Acq On : 20 Mar 2019 16:43
Operator : JC/SP
Sample : VU0320MBL02
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Title : VOC Analysis

72	10.823	3021	3027	3029	rBV	961	1018	0.06%	0.007%
73	10.935	3058	3062	3064	rBV2	1210	1006	0.06%	0.007%
74	10.987	3074	3078	3081	rBV2	1298	1146	0.06%	0.008%
75	11.016	3084	3087	3090	rBV2	1434	1178	0.07%	0.009%
76	11.099	3110	3113	3115	rBV	905	600	0.03%	0.004%
77	11.266	3161	3165	3169	rBV2	1046	921	0.05%	0.007%
78	11.289	3169	3172	3177	rVB	899	577	0.03%	0.004%
79	11.315	3177	3180	3182	rBV	934	588	0.03%	0.004%
80	11.344	3187	3189	3191	rBV	357	209	0.01%	0.002%
81	11.360	3191	3194	3197	rBV2	1259	897	0.05%	0.006%
82	11.482	3220	3232	3253	rBV	741795	1224805	68.72%	8.856%
83	11.855	3336	3348	3372	rBV	798320	1337172	75.02%	9.669%
84	12.559	3565	3567	3570	rBV	855	671	0.04%	0.005%


Sum of corrected areas: 13830160

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030226.D
Acq On : 20 Mar 2019 16:43
Operator : JC/SP
Sample : VU0320MBL02
Misc : 5.00q/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

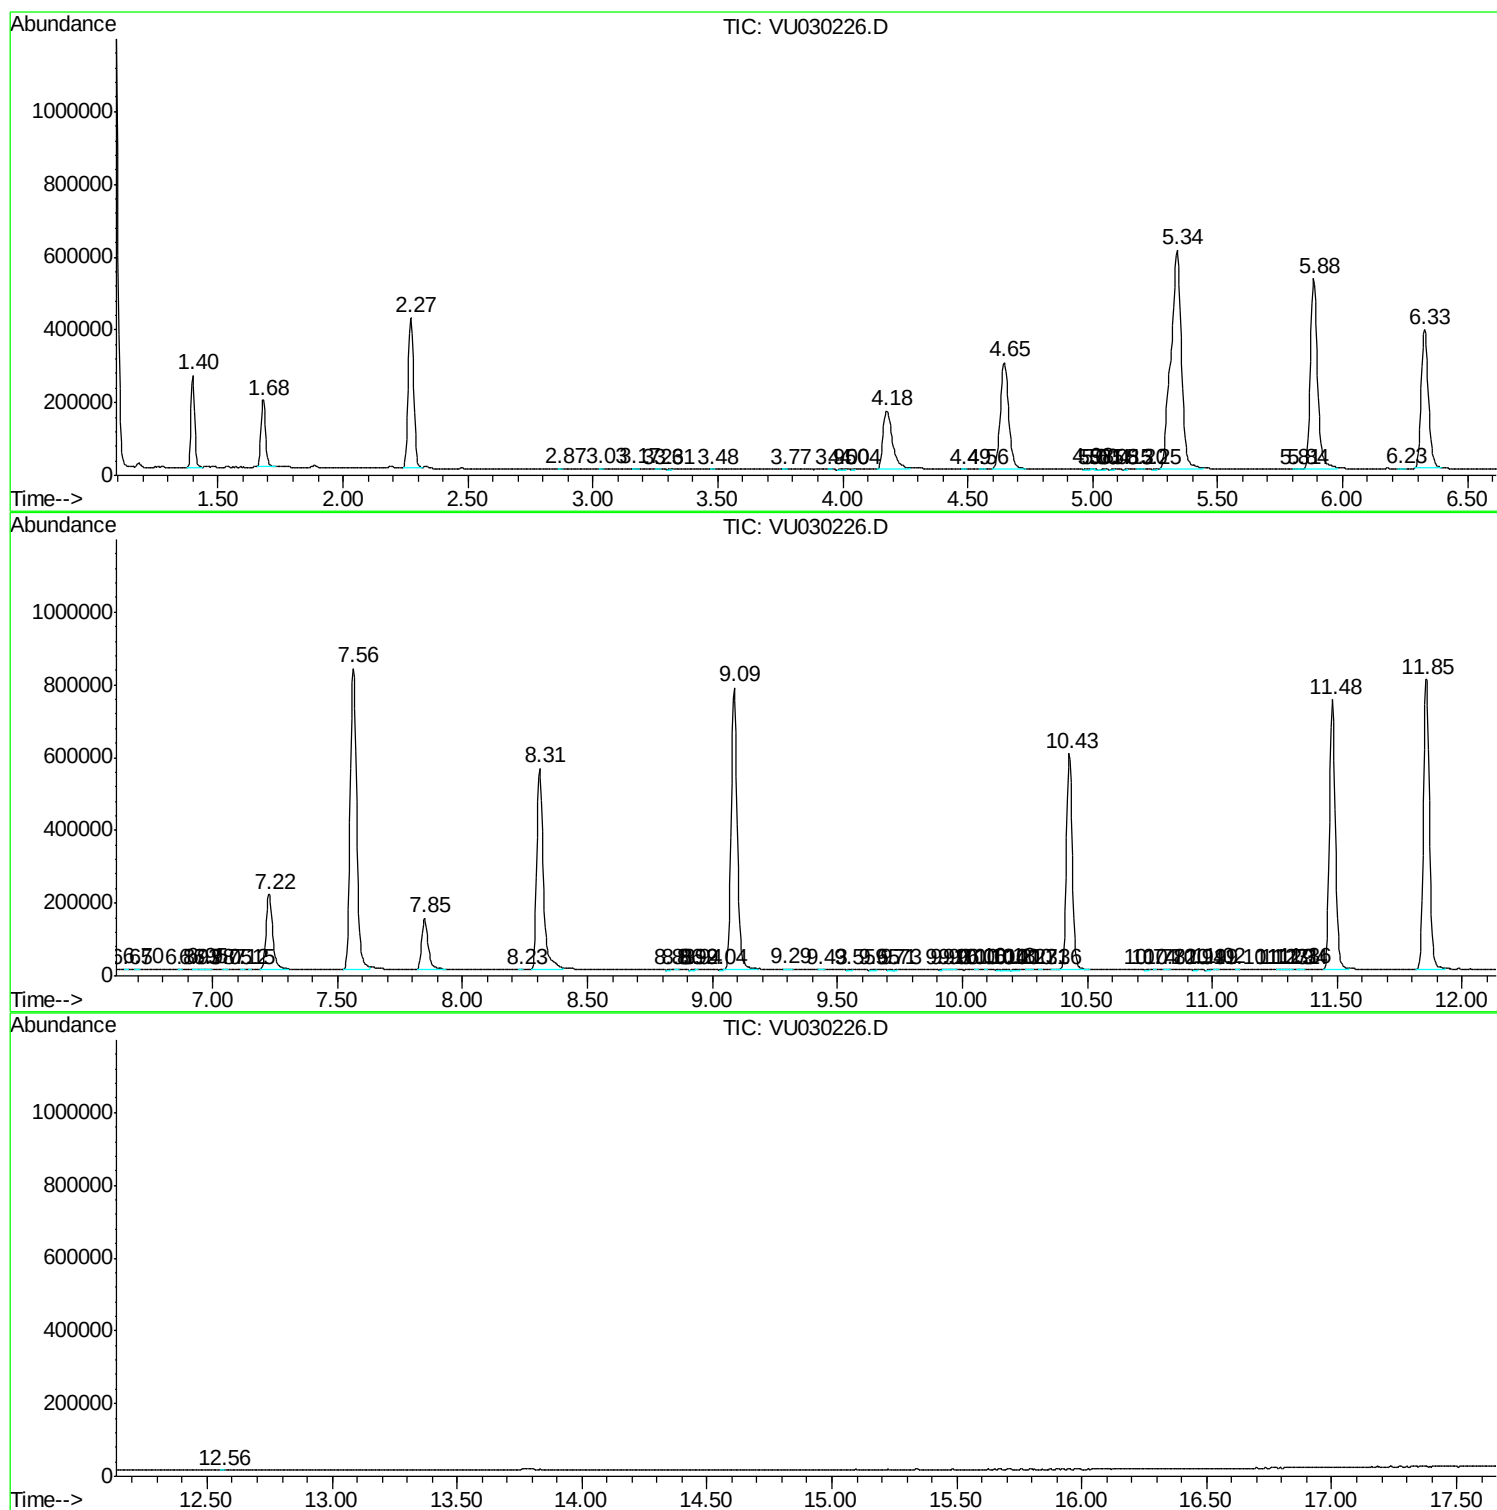

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030226.D
Acq On : 20 Mar 2019 16:43
Operator : JC/SP
Sample : VU0320MBL02
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030226.D
Acq On : 20 Mar 2019 16:43
Operator : JC/SP
Sample : VU0320MBL02
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc