

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030239.D
 Acq On : 20 Mar 2019 21:41
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rVB2	10738	10553	0.62%	0.074%
2	1.399	89	96	107	rBV	230542	230676	13.47%	1.614%
3	1.679	175	183	199	rBV	174275	223204	13.03%	1.561%
4	2.270	357	367	378	rBV	375597	567047	33.11%	3.966%
5	2.444	412	421	439	rVB2	21253	39075	2.28%	0.273%
6	2.553	450	455	458	rBV2	1538	1853	0.11%	0.013%
7	2.688	493	497	506	rBV4	1245	1881	0.11%	0.013%
8	2.749	513	516	521	rBV2	1182	1089	0.06%	0.008%
9	2.836	532	543	558	rVB2	28573	60979	3.56%	0.427%
10	2.936	570	574	579	rBV2	1452	1283	0.07%	0.009%
11	3.161	642	644	648	rVB	1448	953	0.06%	0.007%
12	3.508	747	752	755	rVB	1803	1674	0.10%	0.012%
13	3.540	755	762	767	rBV	1575	2259	0.13%	0.016%
14	3.617	783	786	788	rBV2	1599	1007	0.06%	0.007%
15	4.029	907	914	919	rBV	1608	2236	0.13%	0.016%
16	4.109	937	939	944	rVB	1827	1277	0.07%	0.009%
17	4.177	944	960	987	rBV2	192392	546194	31.89%	3.821%
18	4.389	1019	1026	1028	rBV3	6982	8479	0.50%	0.059%
19	4.582	1082	1086	1088	rBV	1789	1153	0.07%	0.008%
20	4.646	1090	1106	1126	rVV	285559	669162	39.07%	4.681%
21	4.868	1171	1175	1178	rBV	2043	1544	0.09%	0.011%
22	4.887	1178	1181	1186	rVV	2029	1998	0.12%	0.014%
23	4.929	1190	1194	1197	rVB	1640	1001	0.06%	0.007%
24	5.206	1274	1280	1283	rVV2	1032	1192	0.07%	0.008%
25	5.238	1287	1290	1295	rVB	1397	908	0.05%	0.006%
26	5.338	1297	1321	1358	rBV2	578512	1712665	100.00%	11.980%
27	5.720	1437	1440	1445	rBV	1116	872	0.05%	0.006%
28	5.884	1477	1491	1514	rBV	552298	1106249	64.59%	7.738%
29	6.064	1544	1547	1551	rVB	1571	1002	0.06%	0.007%
30	6.112	1559	1562	1567	rVB2	1550	1473	0.09%	0.010%
31	6.141	1567	1571	1577	rBV2	2054	2317	0.14%	0.016%
32	6.186	1581	1585	1591	rVB	1086	1146	0.07%	0.008%
33	6.328	1615	1629	1666	rBV	375929	763132	44.56%	5.338%
34	6.456	1666	1669	1679	rVB4	2573	4028	0.24%	0.028%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030239.D
 Acq On : 20 Mar 2019 21:41
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.501	1679	1683	1687	rVB2	1139	1077	0.06%	0.008%
36	6.534	1690	1693	1699	rVB	1547	1459	0.09%	0.010%
37	6.595	1707	1712	1717	rVB	1299	1483	0.09%	0.010%
38	6.878	1796	1800	1803	rBV2	1453	975	0.06%	0.007%
39	7.009	1834	1841	1844	rBV	1687	1694	0.10%	0.012%
40	7.029	1844	1847	1851	rBV	1053	1107	0.06%	0.008%
41	7.083	1856	1864	1868	rBV2	1984	2254	0.13%	0.016%
42	7.225	1897	1908	1930	rBV	207290	383275	22.38%	2.681%
43	7.363	1948	1951	1953	rBV	1172	845	0.05%	0.006%
44	7.508	1992	1996	1998	rBV	1644	1209	0.07%	0.008%
45	7.563	1998	2013	2043	rVV	768461	1385438	80.89%	9.691%
46	7.849	2091	2102	2123	rBV	141119	255196	14.90%	1.785%
47	8.000	2147	2149	2152	rVB	1469	822	0.05%	0.006%
48	8.177	2196	2204	2211	rBV5	5468	10025	0.59%	0.070%
49	8.308	2233	2245	2280	rBV	544988	995779	58.14%	6.965%
50	8.517	2307	2310	2317	rVB	1781	1884	0.11%	0.013%
51	8.601	2333	2336	2338	rBV	1884	1435	0.08%	0.010%
52	8.733	2372	2377	2378	rBV2	947	869	0.05%	0.006%
53	8.800	2395	2398	2405	rVV2	1417	1633	0.10%	0.011%
54	9.087	2474	2487	2510	rBV	804779	1415390	82.64%	9.901%
55	9.325	2557	2561	2566	rBV2	1302	1472	0.09%	0.010%
56	9.440	2591	2597	2600	rBV2	1370	1552	0.09%	0.011%
57	9.495	2607	2614	2617	rVB	1166	1334	0.08%	0.009%
58	9.559	2629	2634	2636	rBV	1408	1205	0.07%	0.008%
59	9.649	2656	2662	2665	rVB	1227	1170	0.07%	0.008%
60	9.691	2670	2675	2679	rVB	1501	1250	0.07%	0.009%
61	9.884	2732	2735	2740	rVB2	942	868	0.05%	0.006%
62	9.919	2740	2746	2749	rBV	1370	1121	0.07%	0.008%
63	10.122	2802	2809	2812	rVB	1373	1520	0.09%	0.011%
64	10.144	2812	2816	2818	rBV	1336	1099	0.06%	0.008%
65	10.276	2854	2857	2861	rVB2	1083	825	0.05%	0.006%
66	10.328	2868	2873	2875	rBV	1279	1181	0.07%	0.008%
67	10.427	2892	2904	2924	rBV	586177	948036	55.35%	6.631%
68	10.572	2946	2949	2951	rBV	1242	831	0.05%	0.006%
69	10.607	2951	2960	2967	rVV4	4752	7921	0.46%	0.055%
70	10.662	2974	2977	2979	rBV2	1032	824	0.05%	0.006%
71	10.739	2997	3001	3006	rVB	1870	1706	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030239.D
 Acq On : 20 Mar 2019 21:41
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.768	3006	3010	3011	rBV2	1685	1259	0.07%	0.009%
73	10.903	3048	3052	3060	rVB2	1678	2134	0.12%	0.015%
74	10.945	3060	3065	3069	rBV	1571	1971	0.12%	0.014%
75	11.022	3086	3089	3096	rVB	1259	1236	0.07%	0.009%
76	11.061	3097	3101	3105	rBV2	1102	1052	0.06%	0.007%
77	11.160	3127	3132	3136	rVB	971	879	0.05%	0.006%
78	11.186	3136	3140	3144	rVB	1697	1255	0.07%	0.009%
79	11.209	3144	3147	3151	rBV	1625	1192	0.07%	0.008%
80	11.234	3151	3155	3159	rBV2	958	868	0.05%	0.006%
81	11.360	3191	3194	3198	rVB3	1183	900	0.05%	0.006%
82	11.418	3204	3212	3220	rBV3	12071	20144	1.18%	0.141%
83	11.482	3220	3232	3255	rVV	804287	1397978	81.63%	9.779%
84	11.710	3301	3303	3308	rBV2	1319	1018	0.06%	0.007%
85	11.858	3337	3349	3372	rBV	794388	1385014	80.87%	9.688%
86	12.144	3435	3438	3444	rBV	1138	1105	0.06%	0.008%
87	12.398	3511	3517	3521	rBV2	1857	2182	0.13%	0.015%
88	12.453	3531	3534	3537	rBV	1314	853	0.05%	0.006%
89	12.617	3582	3585	3592	rVB	1596	1311	0.08%	0.009%
90	12.675	3600	3603	3605	rBV2	1499	1003	0.06%	0.007%
91	12.800	3638	3642	3646	rVB	2083	1798	0.10%	0.013%
92	12.839	3646	3654	3657	rBV2	1676	2857	0.17%	0.020%
93	12.987	3697	3700	3704	rBV2	1434	1120	0.07%	0.008%
94	13.083	3727	3730	3732	rBV	1198	838	0.05%	0.006%
95	13.334	3800	3808	3812	rBV2	2401	3538	0.21%	0.025%
96	13.511	3854	3863	3882	rBV4	13972	33185	1.94%	0.232%
97	13.993	4004	4013	4022	rBV4	8034	15048	0.88%	0.105%
98	14.395	4136	4138	4142	rBV	1173	916	0.05%	0.006%
99	14.704	4229	4234	4240	rBV2	1920	2517	0.15%	0.018%
100	15.000	4322	4326	4328	rBV2	1859	1586	0.09%	0.011%


Sum of corrected areas: 14296082

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030239.D
Acq On : 20 Mar 2019 21:41
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

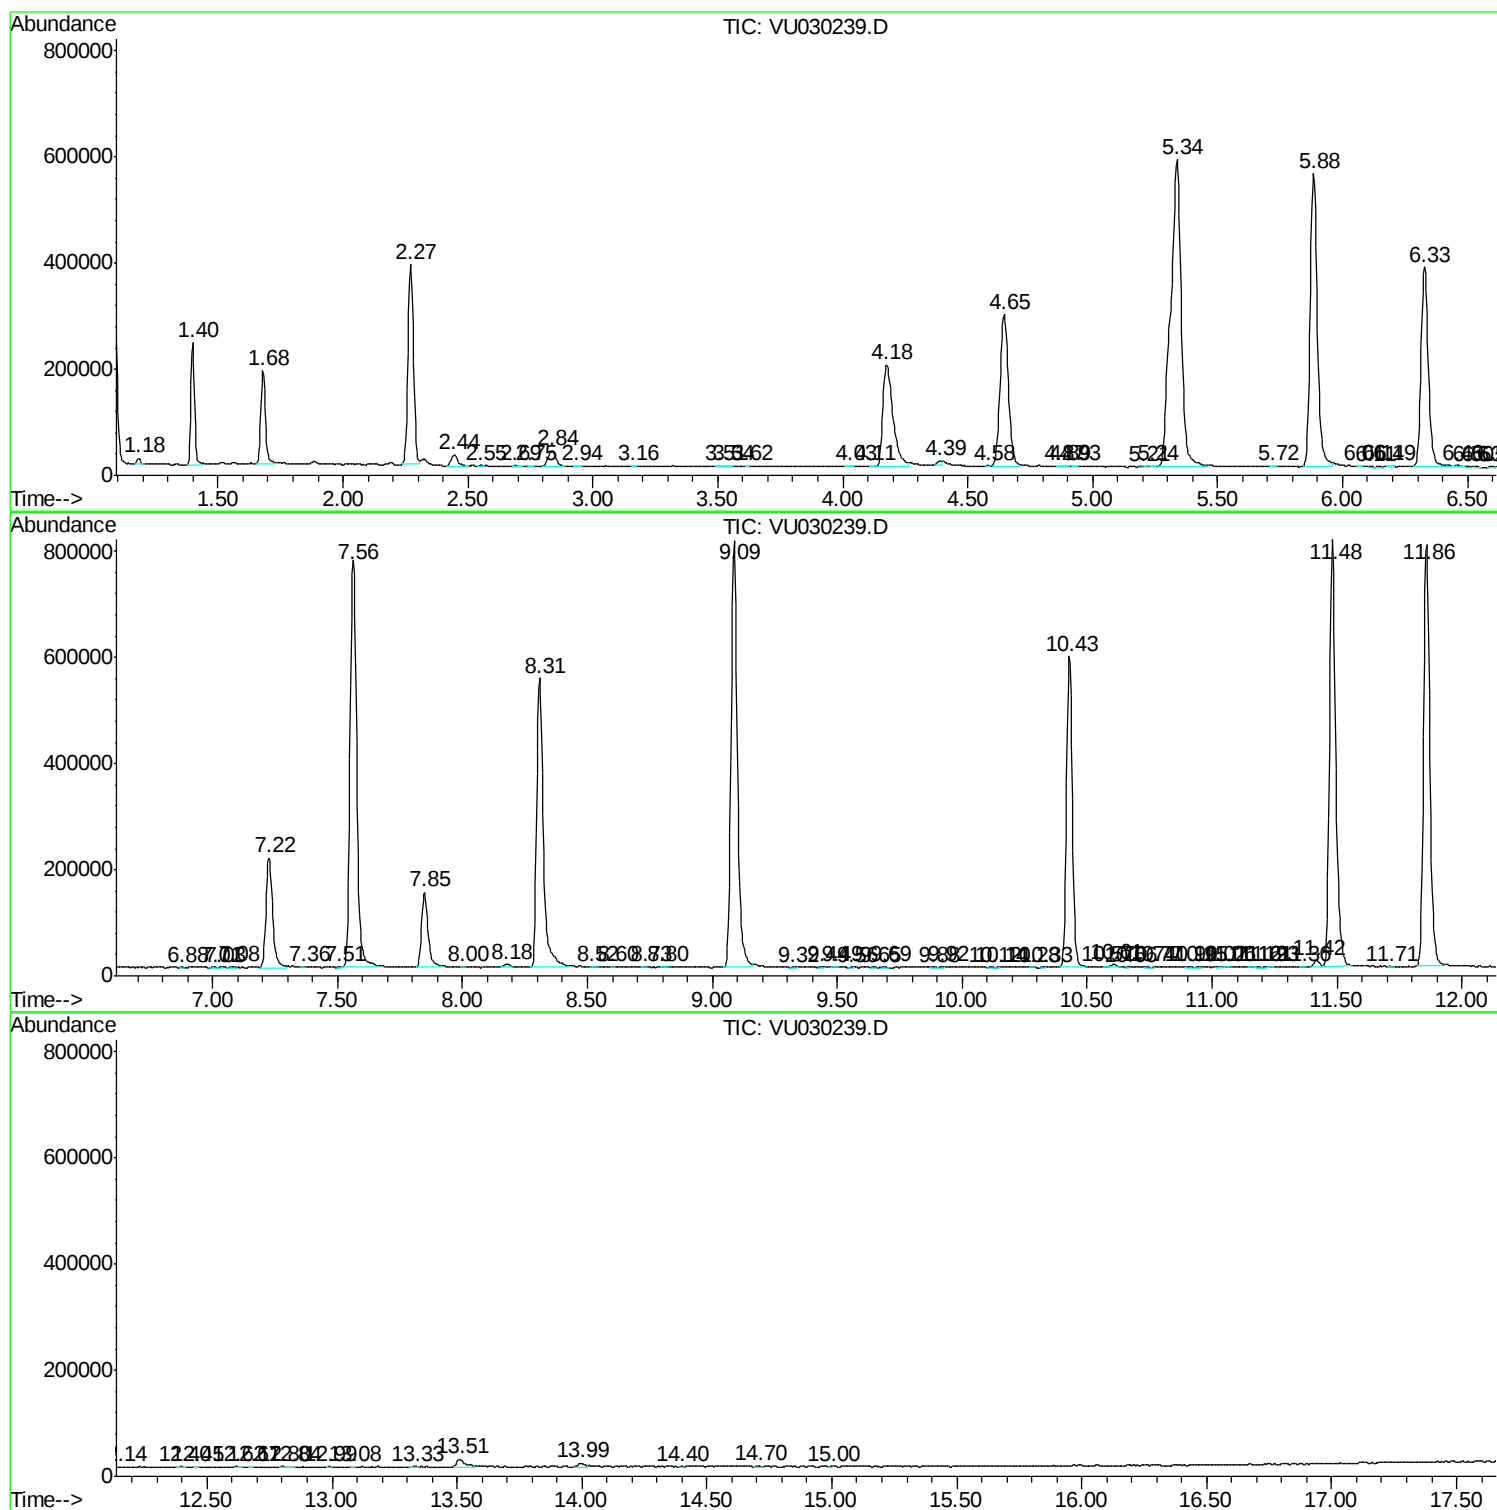

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030239.D
Acq On : 20 Mar 2019 21:41
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030239.D
Acq On : 20 Mar 2019 21:41
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
