

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030241.D
 Acq On : 20 Mar 2019 22:27
 Operator : JC/SP
 Sample : K2022-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB3	11506	11843	0.06%	0.027%
2	1.399	89	96	107	rBV	233008	234355	1.11%	0.529%
3	1.682	176	184	198	rVB	175935	226591	1.07%	0.511%
4	2.109	314	317	320	rBV2	2171	1827	0.01%	0.004%
5	2.270	357	367	379	rBV	380848	578560	2.74%	1.305%
6	2.447	414	422	438	rVB	8112	15064	0.07%	0.034%
7	2.575	460	462	466	rVB	1334	823	0.00%	0.002%
8	2.614	470	474	476	rBV	1256	951	0.00%	0.002%
9	2.691	494	498	500	rBV	1672	1342	0.01%	0.003%
10	2.733	508	511	517	rBV2	1060	963	0.00%	0.002%
11	2.759	517	519	522	rVB	1906	1020	0.00%	0.002%
12	2.778	522	525	529	rBV	1348	1187	0.01%	0.003%
13	2.804	529	533	535	rBV	1661	1325	0.01%	0.003%
14	3.183	647	651	653	rBV	1401	1123	0.01%	0.003%
15	3.260	670	675	677	rBV2	1035	915	0.00%	0.002%
16	3.350	700	703	707	rVB	1176	823	0.00%	0.002%
17	3.473	733	741	744	rBV	1193	1916	0.01%	0.004%
18	3.563	765	769	771	rBV2	1355	1065	0.01%	0.002%
19	3.672	798	803	807	rBV2	1161	1176	0.01%	0.003%
20	3.730	818	821	829	rVB	1639	2134	0.01%	0.005%
21	3.800	839	843	847	rBV	1300	1147	0.01%	0.003%
22	3.845	852	857	866	rVB	1516	2033	0.01%	0.005%
23	3.887	866	870	874	rBV	1310	990	0.00%	0.002%
24	3.929	880	883	887	rBV	1599	1599	0.01%	0.004%
25	3.977	894	898	900	rBV	1180	1037	0.00%	0.002%
26	4.051	917	921	924	rBV	1042	871	0.00%	0.002%
27	4.173	947	959	987	rBV	164301	433161	2.05%	0.977%
28	4.389	1018	1026	1049	rVB4	12474	32051	0.15%	0.072%
29	4.492	1055	1058	1063	rVB2	1451	1288	0.01%	0.003%
30	4.521	1063	1067	1074	rVB	1993	2080	0.01%	0.005%
31	4.646	1090	1106	1132	rBV	288950	693856	3.28%	1.565%
32	5.228	1283	1287	1290	rBV2	1364	1194	0.01%	0.003%
33	5.337	1298	1321	1330	rBV2	591723	1719976	8.14%	3.879%
34	5.710	1431	1437	1439	rBV2	1259	1185	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030241.D
 Acq On : 20 Mar 2019 22:27
 Operator : JC/SP
 Sample : K2022-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	5.884	1478	1491	1519	rBV	571041	1136963	5.38%	2.564%
36	6.177	1576	1582	1584	rBV2	1664	1705	0.01%	0.004%
37	6.225	1594	1597	1601	rBV	1420	1269	0.01%	0.003%
38	6.273	1607	1612	1615	rBV	1032	1118	0.01%	0.003%
39	6.328	1615	1629	1659	rVV	382923	781012	3.70%	1.762%
40	6.511	1683	1686	1692	rVB	1274	1339	0.01%	0.003%
41	6.540	1692	1695	1698	rBV	1118	891	0.00%	0.002%
42	6.591	1705	1711	1712	rBV2	1407	1239	0.01%	0.003%
43	6.630	1719	1723	1726	rBV	950	947	0.00%	0.002%
44	6.723	1749	1752	1755	rBV	1462	1046	0.00%	0.002%
45	7.058	1853	1856	1863	rVB	1527	1362	0.01%	0.003%
46	7.093	1863	1867	1870	rBV	1514	1184	0.01%	0.003%
47	7.225	1897	1908	1928	rBV	214079	386278	1.83%	0.871%
48	7.562	2000	2013	2045	rBV	786099	1421365	6.73%	3.206%
49	7.736	2063	2067	2074	rBV2	1217	1290	0.01%	0.003%
50	7.849	2091	2102	2120	rBV	146076	258404	1.22%	0.583%
51	8.176	2196	2204	2213	rBV3	5592	9657	0.05%	0.022%
52	8.225	2213	2219	2229	rVB4	3701	6495	0.03%	0.015%
53	8.308	2234	2245	2274	rBV	566573	1013561	4.80%	2.286%
54	8.556	2317	2322	2324	rBV2	901	852	0.00%	0.002%
55	8.598	2332	2335	2342	rVB2	1779	2102	0.01%	0.005%
56	8.768	2383	2388	2390	rBV	1065	1062	0.01%	0.002%
57	8.848	2408	2413	2417	rBV3	718	913	0.00%	0.002%
58	9.086	2472	2487	2490	rBV	888859	1257979	5.95%	2.837%
59	9.488	2608	2612	2615	rBV2	1450	1280	0.01%	0.003%
60	9.553	2629	2632	2637	rVB	1939	1585	0.01%	0.004%
61	9.582	2637	2641	2644	rBV2	1135	1013	0.00%	0.002%
62	9.633	2651	2657	2661	rVB	1475	1641	0.01%	0.004%
63	9.877	2729	2733	2737	rBV	1518	1207	0.01%	0.003%
64	10.022	2771	2778	2781	rBV3	1656	2472	0.01%	0.006%
65	10.119	2803	2808	2810	rBV	1218	956	0.00%	0.002%
66	10.212	2834	2837	2839	rBV	1254	911	0.00%	0.002%
67	10.311	2864	2868	2871	rBV	1101	866	0.00%	0.002%
68	10.344	2872	2878	2884	rVV2	1524	1812	0.01%	0.004%
69	10.427	2888	2904	2927	rBV	607424	980939	4.64%	2.212%
70	10.604	2949	2959	2967	rVB4	6697	10707	0.05%	0.024%
71	10.659	2971	2976	2979	rBV3	1194	1245	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032019\
 Data File : VU030241.D
 Acq On : 20 Mar 2019 22:27
 Operator : JC/SP
 Sample : K2022-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.916	3052	3056	3059	rBV	1016	832	0.00%	0.002%
73	11.016	3080	3087	3091	rBV	1121	1524	0.01%	0.003%
74	11.112	3114	3117	3122	rVB	1424	1321	0.01%	0.003%
75	11.144	3122	3127	3129	rBV2	996	980	0.00%	0.002%
76	11.282	3164	3170	3173	rBV2	990	937	0.00%	0.002%
77	11.327	3180	3184	3188	rVB	1684	1698	0.01%	0.004%
78	11.360	3188	3194	3197	rBV	1287	1514	0.01%	0.003%
79	11.414	3198	3211	3221	rBV	464534	726616	3.44%	1.639%
80	11.504	3221	3239	3259	rVB2	4296705	7987665	37.80%	18.016%
81	11.723	3304	3307	3312	rVB	1312	1235	0.01%	0.003%
82	11.765	3312	3320	3325	rBV4	4176	6541	0.03%	0.015%
83	11.877	3336	3355	3383	rBV	12743611	21130327	100.00%	47.658%
84	12.118	3427	3430	3438	rVB2	1582	1472	0.01%	0.003%
85	12.639	3581	3592	3597	rBV5	4345	7401	0.04%	0.017%
86	12.781	3633	3636	3640	rBV	1141	968	0.00%	0.002%
87	12.877	3663	3666	3668	rBV	1856	1300	0.01%	0.003%
88	13.035	3712	3715	3718	rVB	1570	1038	0.00%	0.002%
89	13.289	3789	3794	3798	rVV3	1067	1108	0.01%	0.002%
90	13.324	3802	3805	3810	rVB	969	890	0.00%	0.002%
91	13.350	3810	3813	3817	rBV	1357	1343	0.01%	0.003%
92	13.427	3832	3837	3842	rBV	1807	2343	0.01%	0.005%
93	13.498	3847	3859	3885	rBV	1269130	2076113	9.83%	4.683%
94	13.983	3998	4010	4030	rBV	473726	797462	3.77%	1.799%
95	14.401	4135	4140	4144	rBV	1690	1708	0.01%	0.004%
96	14.556	4185	4188	4191	rBV2	1482	1101	0.01%	0.002%
97	15.009	4325	4329	4331	rBV	1753	1258	0.01%	0.003%
98	15.073	4336	4349	4364	rVV4	27079	63828	0.30%	0.144%
99	15.597	4509	4512	4516	rBV2	1958	1295	0.01%	0.003%
100	15.649	4517	4528	4550	rBV2	118456	241280	1.14%	0.544%


Sum of corrected areas: 44337236

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032019\
Data File : VU030241.D
Acq On : 20 Mar 2019 22:27
Operator : JC/SP
Sample : K2022-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

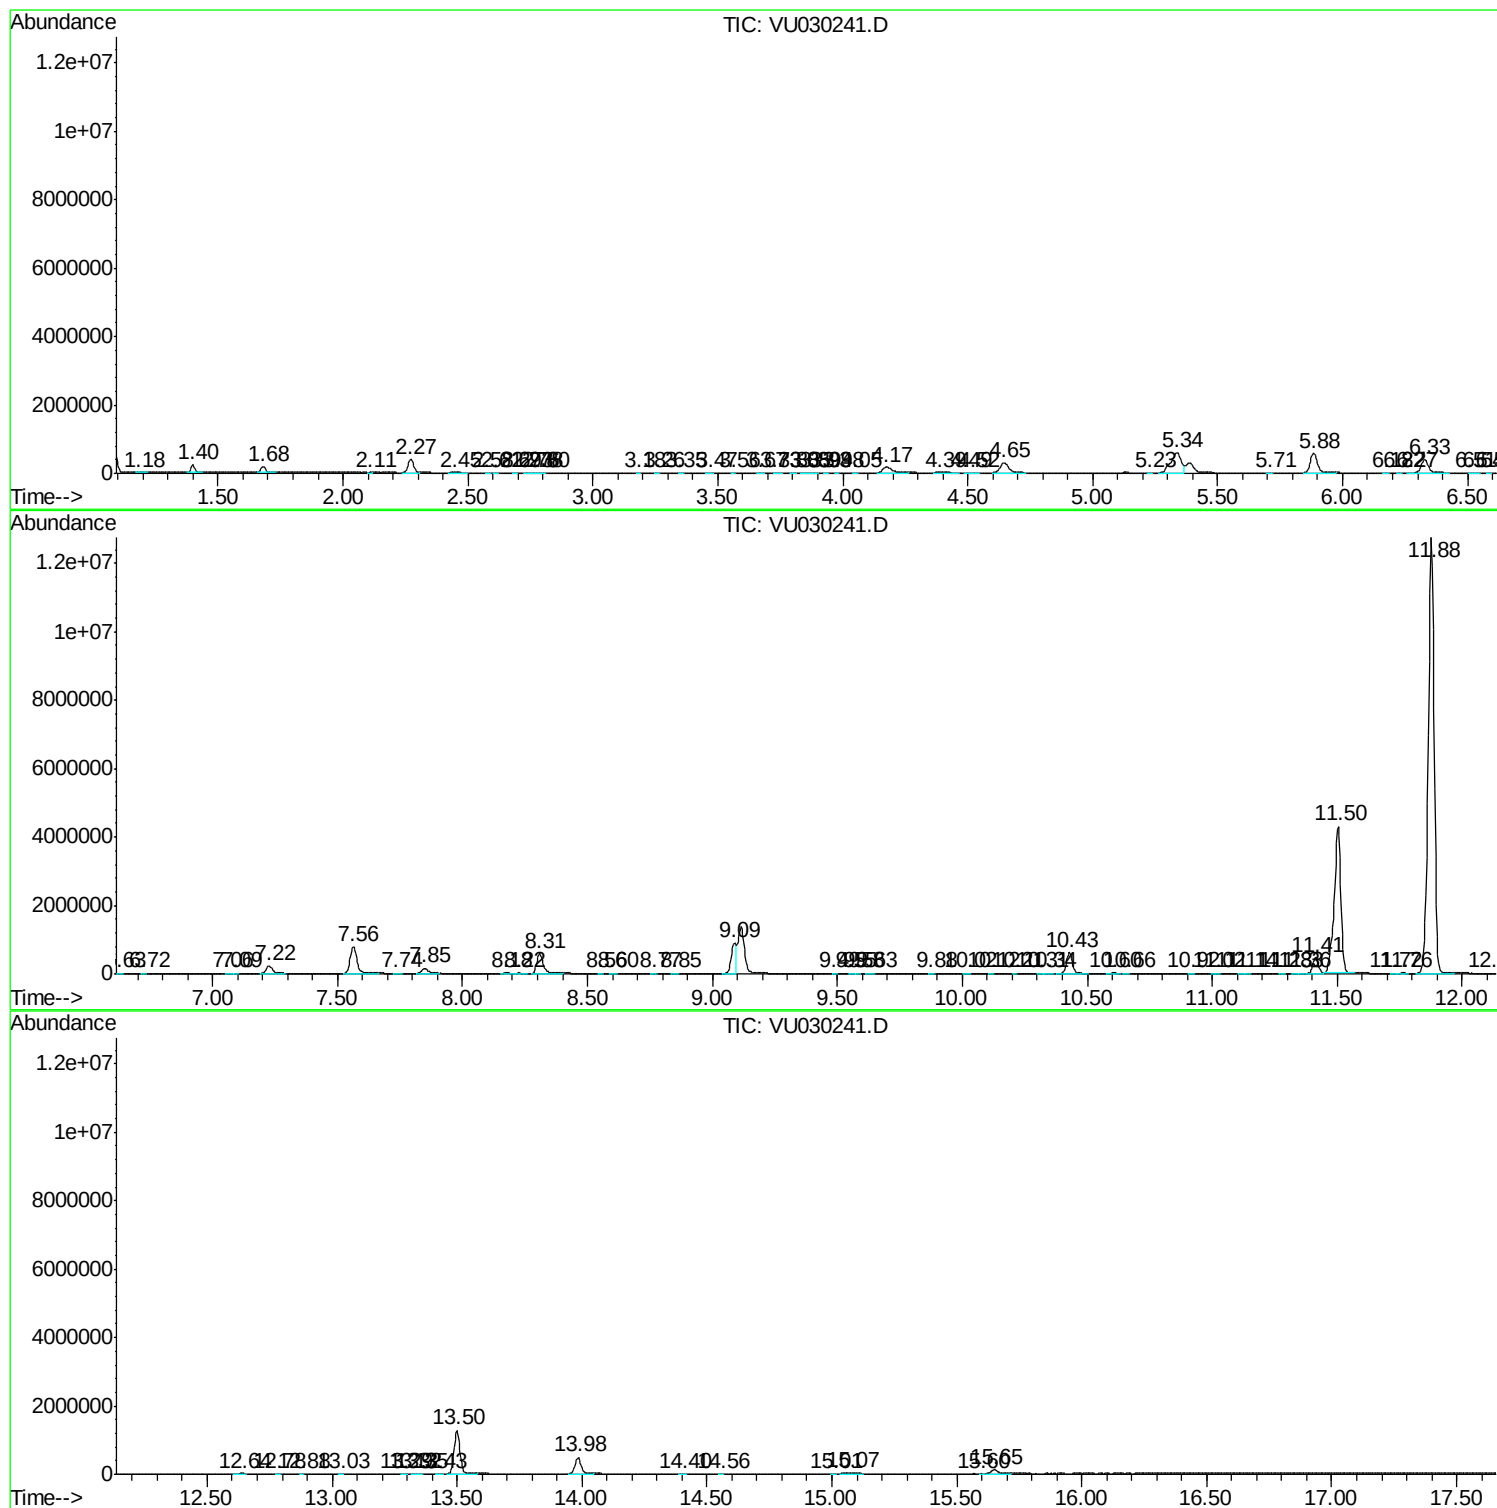

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030241.D
Acq On : 20 Mar 2019 22:27
Operator : JC/SP
Sample : K2022-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032019\
Data File : VU030241.D
Acq On : 20 Mar 2019 22:27
Operator : JC/SP
Sample : K2022-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc