


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032019\
 Data File : VU030215.D
 Acq On : 20 Mar 2019 08:23
 Operator : JC/SP
 Sample : BFB38
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis
 Last Update : Sat Mar 23 04:35:39 2019

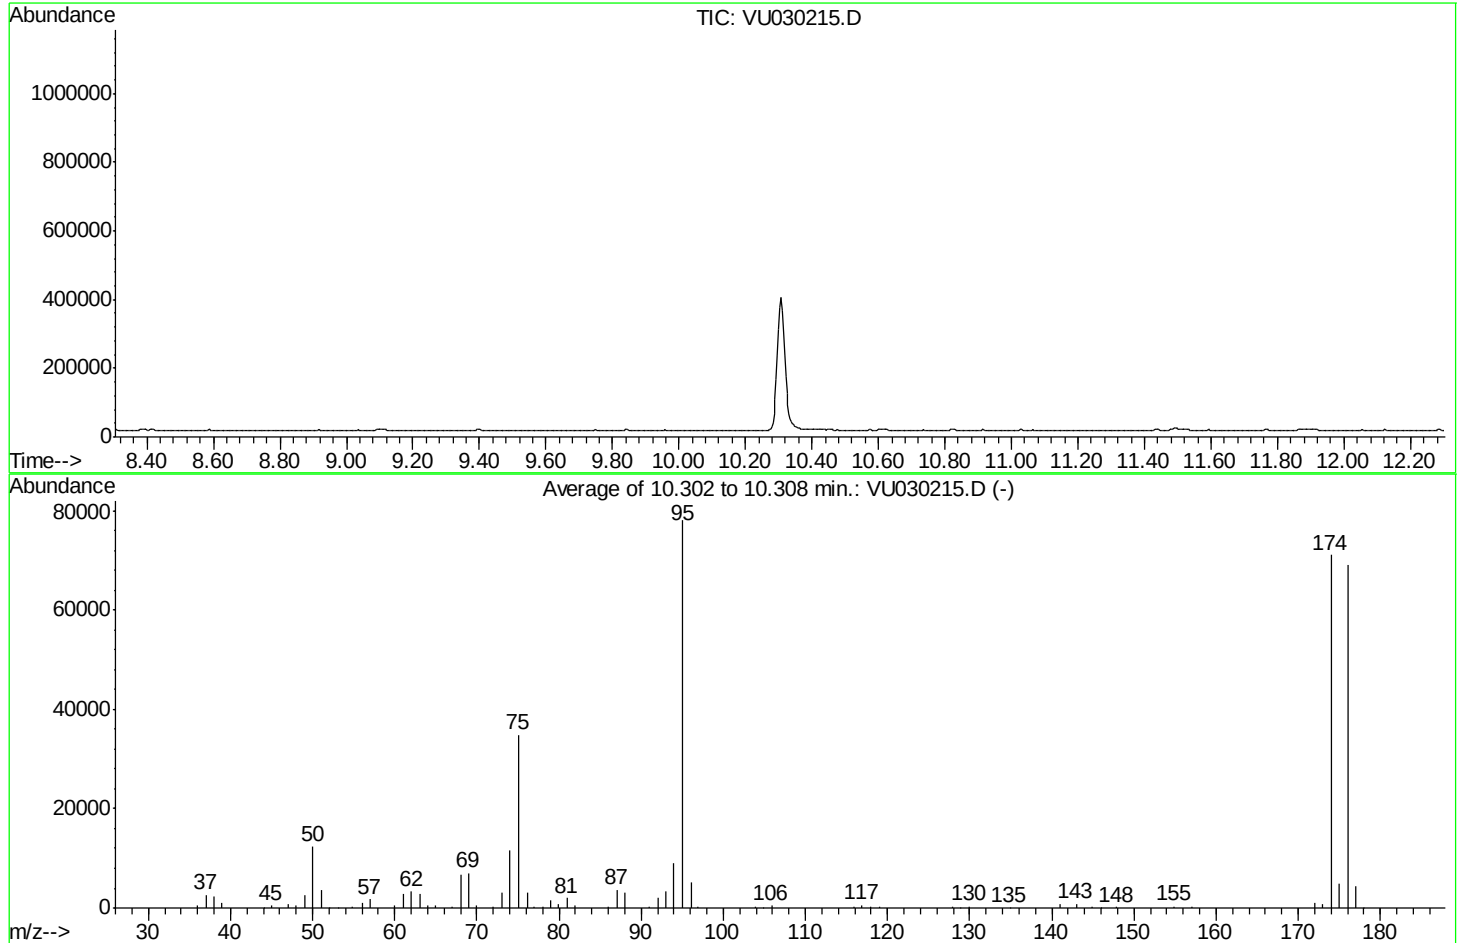

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	12365	PASS
75	95	30	80	44.7	34928	PASS
95	95	100	100	100.0	78093	PASS
96	95	5	9	6.8	5295	PASS
173	174	0.00	2	1.1	750	PASS
174	95	50	120	91.0	71074	PASS
175	174	5	9	7.0	4970	PASS
176	174	95	101	97.1	69032	PASS
177	176	5	9	6.5	4497	PASS

Scan 2854 (10.267 min): VU030215.D
BFB38

m/z	Abundance
40.00	18992.0
44.00	525.0
207.20	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	615.0
37.00	2548.0
38.00	2345.0
39.00	874.0
40.00	18792.0
44.10	638.0
45.00	513.0
47.10	746.0
48.00	412.0
49.00	2549.0
50.00	12017.0
51.10	3475.0
52.00	138.0
53.10	106.0
54.90	161.0
56.00	1046.0
57.00	1542.0
59.90	558.0
61.00	2933.0
62.00	3138.0
63.00	2822.0
64.00	399.0
65.00	616.0
66.90	201.0
68.00	6350.0
69.00	6735.0
70.00	512.0
71.90	252.0
73.10	3077.0
74.00	11017.0
75.10	33424.0
76.10	3134.0
76.90	311.0
78.00	280.0
79.00	1627.0
79.90	609.0
80.90	1939.0
81.90	572.0
86.00	176.0
87.00	3615.0
88.00	3024.0
90.90	280.0
92.00	2137.0
93.00	3305.0
94.00	8460.0
95.10	73624.0
96.00	5304.0
97.00	164.0
103.90	281.0
104.80	139.0
105.90	482.0
115.90	338.0
116.90	549.0
117.90	381.0
119.00	362.0
128.00	207.0
130.00	307.0
141.00	706.0
143.00	784.0
145.00	238.0
147.90	196.0
154.90	325.0
157.00	173.0
172.00	958.0
173.00	740.0
174.00	66040.0
175.00	4666.0
176.00	64552.0
177.00	4298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	646.0
37.00	2745.0
38.00	2518.0
39.00	937.0
40.00	18776.0
44.00	632.0
44.90	524.0
47.10	941.0
47.90	464.0
49.00	2666.0
50.00	12797.0
51.00	3837.0
52.00	105.0
54.90	166.0
56.00	1189.0
57.00	1747.0
59.90	577.0
61.00	2949.0
62.00	3433.0
63.00	2880.0
64.10	444.0
65.00	618.0
67.00	201.0
68.00	6975.0
69.00	7166.0
70.00	540.0
72.00	355.0
73.10	3281.0
74.00	12028.0
75.10	35912.0
76.10	3310.0
76.90	332.0
78.00	238.0
79.00	1690.0
79.90	694.0
81.00	2128.0
81.90	598.0
86.00	171.0
87.00	3799.0
88.00	3235.0
90.90	313.0
92.00	2205.0
93.00	3582.0
94.00	9279.0
95.00	80400.0
96.10	5445.0
97.00	160.0
103.90	259.0
104.80	111.0
105.90	501.0
115.90	329.0
116.90	569.0
117.90	351.0
119.00	332.0
128.00	241.0
128.80	100.0
130.00	356.0
141.00	836.0
143.00	821.0
145.00	233.0
147.90	212.0
154.90	331.0
157.00	183.0
172.00	1024.0
173.00	751.0
174.00	73280.0
175.00	5094.0
176.00	70984.0
177.00	4667.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	618.0
37.00	2648.0
38.00	2475.0
39.00	1001.0
40.00	18904.0
44.00	686.0
45.00	438.0
47.10	980.0
48.00	404.0
49.00	2510.0
50.00	12281.0
51.00	3803.0
54.90	165.0
56.00	1041.0
57.00	1791.0
60.00	571.0
61.00	2710.0
62.00	3477.0
63.10	2511.0
64.10	451.0
65.00	577.0
67.00	197.0
68.00	6875.0
69.00	7219.0
70.00	502.0
72.00	415.0
73.00	3022.0
74.00	11762.0
75.00	35448.0
76.10	3248.0
76.90	336.0
79.00	1658.0
79.90	800.0
81.00	2114.0
81.90	520.0
86.00	118.0
87.00	3601.0
87.90	3120.0
91.00	348.0
92.00	2129.0
93.00	3415.0
94.00	9100.0
95.00	80256.0
96.10	5138.0
96.90	135.0
103.90	256.0
105.90	441.0
115.90	278.0
116.90	536.0
117.90	291.0
119.00	289.0
127.90	308.0
128.90	131.0
130.00	312.0
134.90	144.0
140.90	760.0
143.00	853.0
144.80	201.0
146.00	111.0
147.90	225.0
154.90	253.0
157.00	137.0
172.00	1051.0
173.00	760.0
174.00	73904.0
175.00	5152.0
176.00	71560.0
177.00	4528.0
177.90	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38