


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032020\
 Data File : VU037346.D
 Acq On : 20 Mar 2020 09:42
 Operator : JC/MD
 Sample : BFB07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 21 00:26:09 2020

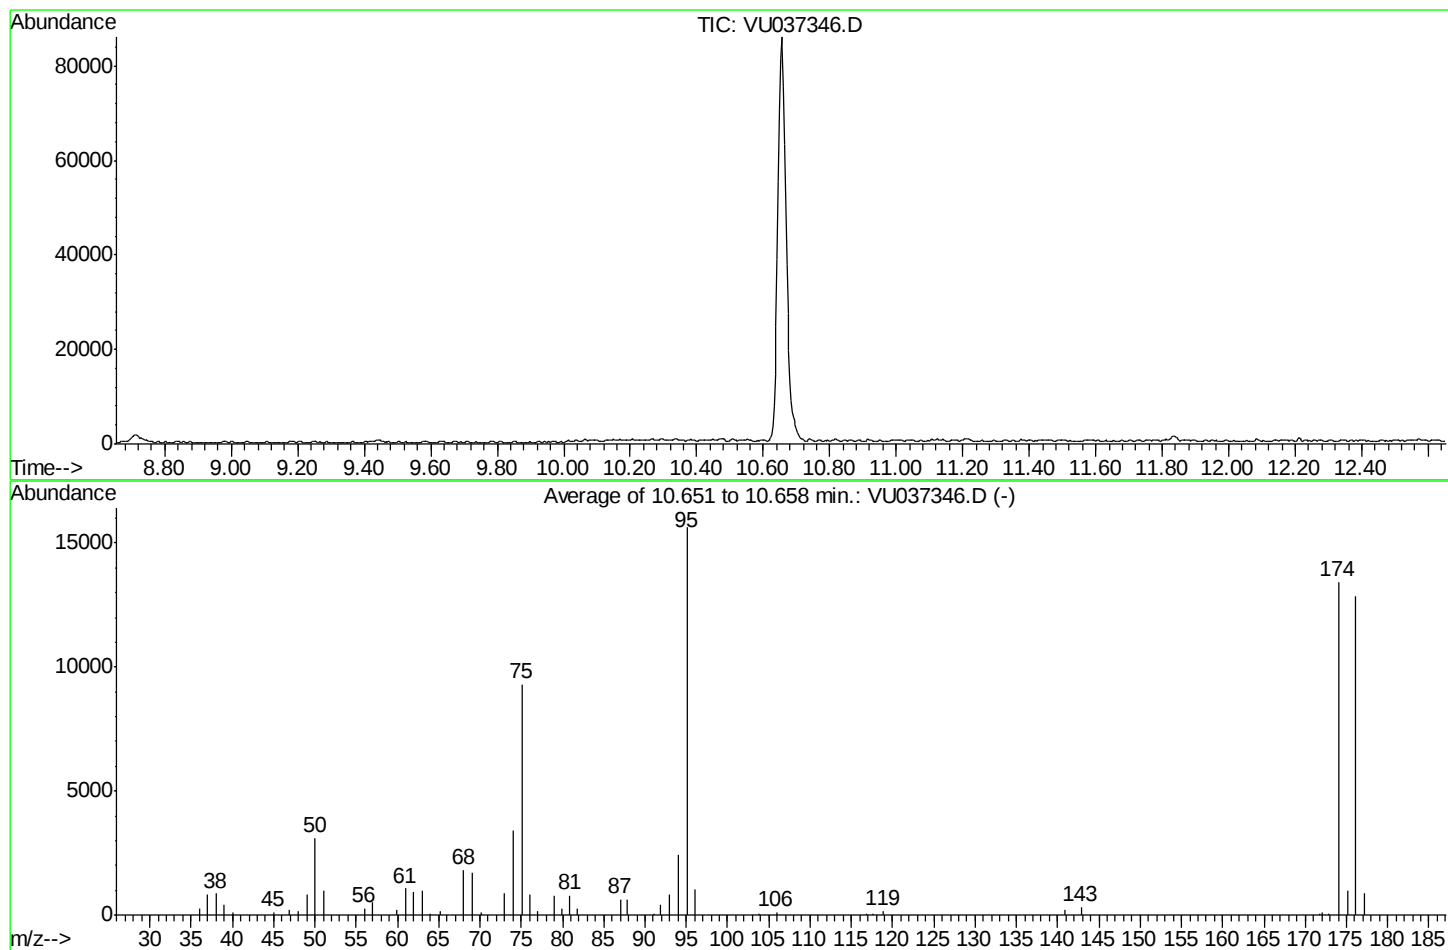

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	3106	PASS
75	95	30	80	59.5	9303	PASS
95	95	100	100	100.0	15631	PASS
96	95	5	9	6.7	1041	PASS
173	174	0.00	2	0.5	63	PASS
174	95	50	120	85.9	13427	PASS
175	174	5	9	7.2	973	PASS
176	174	95	101	95.7	12856	PASS
177	176	5	9	6.6	854	PASS

Scan 2884 (10.613 min): VU037346.D
BFB07

m/z	Abundance
35.90	209.0
43.90	429.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	433.0
37.00	850.0
38.00	916.0
39.00	423.0
40.00	141.0
44.00	476.0
45.10	108.0
46.90	221.0
47.90	136.0
49.00	785.0
50.00	2997.0
51.00	1070.0
55.90	308.0
57.00	510.0
59.90	195.0
61.00	1125.0
62.00	816.0
63.10	1008.0
63.90	122.0
65.20	152.0
68.00	1788.0
69.00	1699.0
70.20	142.0
72.90	796.0
74.00	3295.0
75.00	9302.0
76.00	839.0
77.00	121.0
79.00	774.0
79.90	235.0
80.90	676.0
81.80	199.0
87.00	603.0
87.90	564.0
91.90	357.0
93.00	755.0
94.00	2452.0
95.10	15698.0
96.10	1006.0
103.80	129.0
105.90	102.0
118.90	155.0
140.90	188.0
142.80	355.0
172.10	161.0
174.00	12593.0
175.10	935.0
176.00	12134.0
177.10	781.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	449.0
37.00	857.0
38.00	884.0
39.00	449.0
40.00	110.0
44.00	378.0
45.00	104.0
46.90	203.0
48.00	164.0
49.00	849.0
50.00	3162.0
51.00	1000.0
56.00	269.0
57.00	542.0
59.90	233.0
61.00	1089.0
62.00	986.0
63.00	1009.0
63.90	102.0
65.20	159.0
68.00	1887.0
69.00	1712.0
70.20	114.0
73.00	881.0
74.00	3503.0
75.00	9586.0
76.00	877.0
77.00	157.0
79.00	754.0
79.90	280.0
80.90	796.0
81.80	251.0
87.00	661.0
87.90	631.0
91.10	115.0
91.90	404.0
93.00	807.0
94.10	2537.0
95.10	16008.0
96.10	1064.0
103.80	106.0
105.90	130.0
118.90	170.0
140.90	214.0
142.80	344.0
172.10	136.0
174.00	13844.0
175.10	1003.0
176.00	13282.0
177.10	866.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	472.0
37.00	779.0
38.00	800.0
39.00	412.0
44.00	361.0
44.90	145.0
46.90	198.0
48.00	162.0
49.00	835.0
50.00	3160.0
51.00	915.0
56.10	242.0
57.00	522.0
60.00	221.0
61.00	977.0
62.00	1053.0
63.00	921.0
65.20	128.0
68.00	1804.0
69.00	1738.0
73.00	908.0
74.00	3444.0
75.10	9022.0
76.00	838.0
77.00	185.0
78.90	771.0
79.90	226.0
80.90	855.0
81.80	287.0
87.00	661.0
87.90	704.0
91.10	102.0
91.90	464.0
93.00	868.0
94.10	2303.0
95.10	15187.0
96.00	1053.0
105.90	123.0
116.90	127.0
117.60	103.0
118.90	149.0
140.90	234.0
142.90	295.0
171.80	112.0
172.90	191.0
174.00	13845.0
175.10	982.0
176.10	13154.0
177.10	915.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07