

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053300.D
 Acq On : 20 Mar 2023 12:18
 Operator : JC/MD
 Sample : 01930-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0DL

Quant Time: Mar 21 01:29:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 21 01:25:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	117413	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	105735	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	49447	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	40180	37.094	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.180%		
7) Chloroethane-d5	1.912	69	35580	40.608	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.220%		
11) 1,1-Dichloroethene-d2	2.568	63	55524	29.590	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	59.180%#		
21) 2-Butanone-d5	4.613	46	49704	98.934	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.930%		
24) Chloroform-d	5.057	84	76499	42.878	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.760%		
26) 1,2-Dichloroethane-d4	5.697	65	51788	46.740	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.480%		
32) Benzene-d6	5.722	84	160080	46.677	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.360%		
36) 1,2-Dichloropropane-d6	6.684	67	54103	48.879	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.760%		
41) Toluene-d8	7.893	98	142005	44.474	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.940%		
43) trans-1,3-Dichloroprop...	8.172	79	24507	44.875	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.760%		
47) 2-Hexanone-d5	8.626	63	36312	104.933	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.930%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	70294	49.024	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.040%		
66) 1,2-Dichlorobenzene-d4	12.188	152	46751	48.830	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.660%		
Target Compounds					Qvalue	
33) Benzene	5.771	78	162613	44.360	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053300.D
Acq On : 20 Mar 2023 12:18
Operator : JC/MD
Sample : 01930-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0DL

Quant Time: Mar 21 01:29:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 21 01:25:41 2023
Response via : Initial Calibration

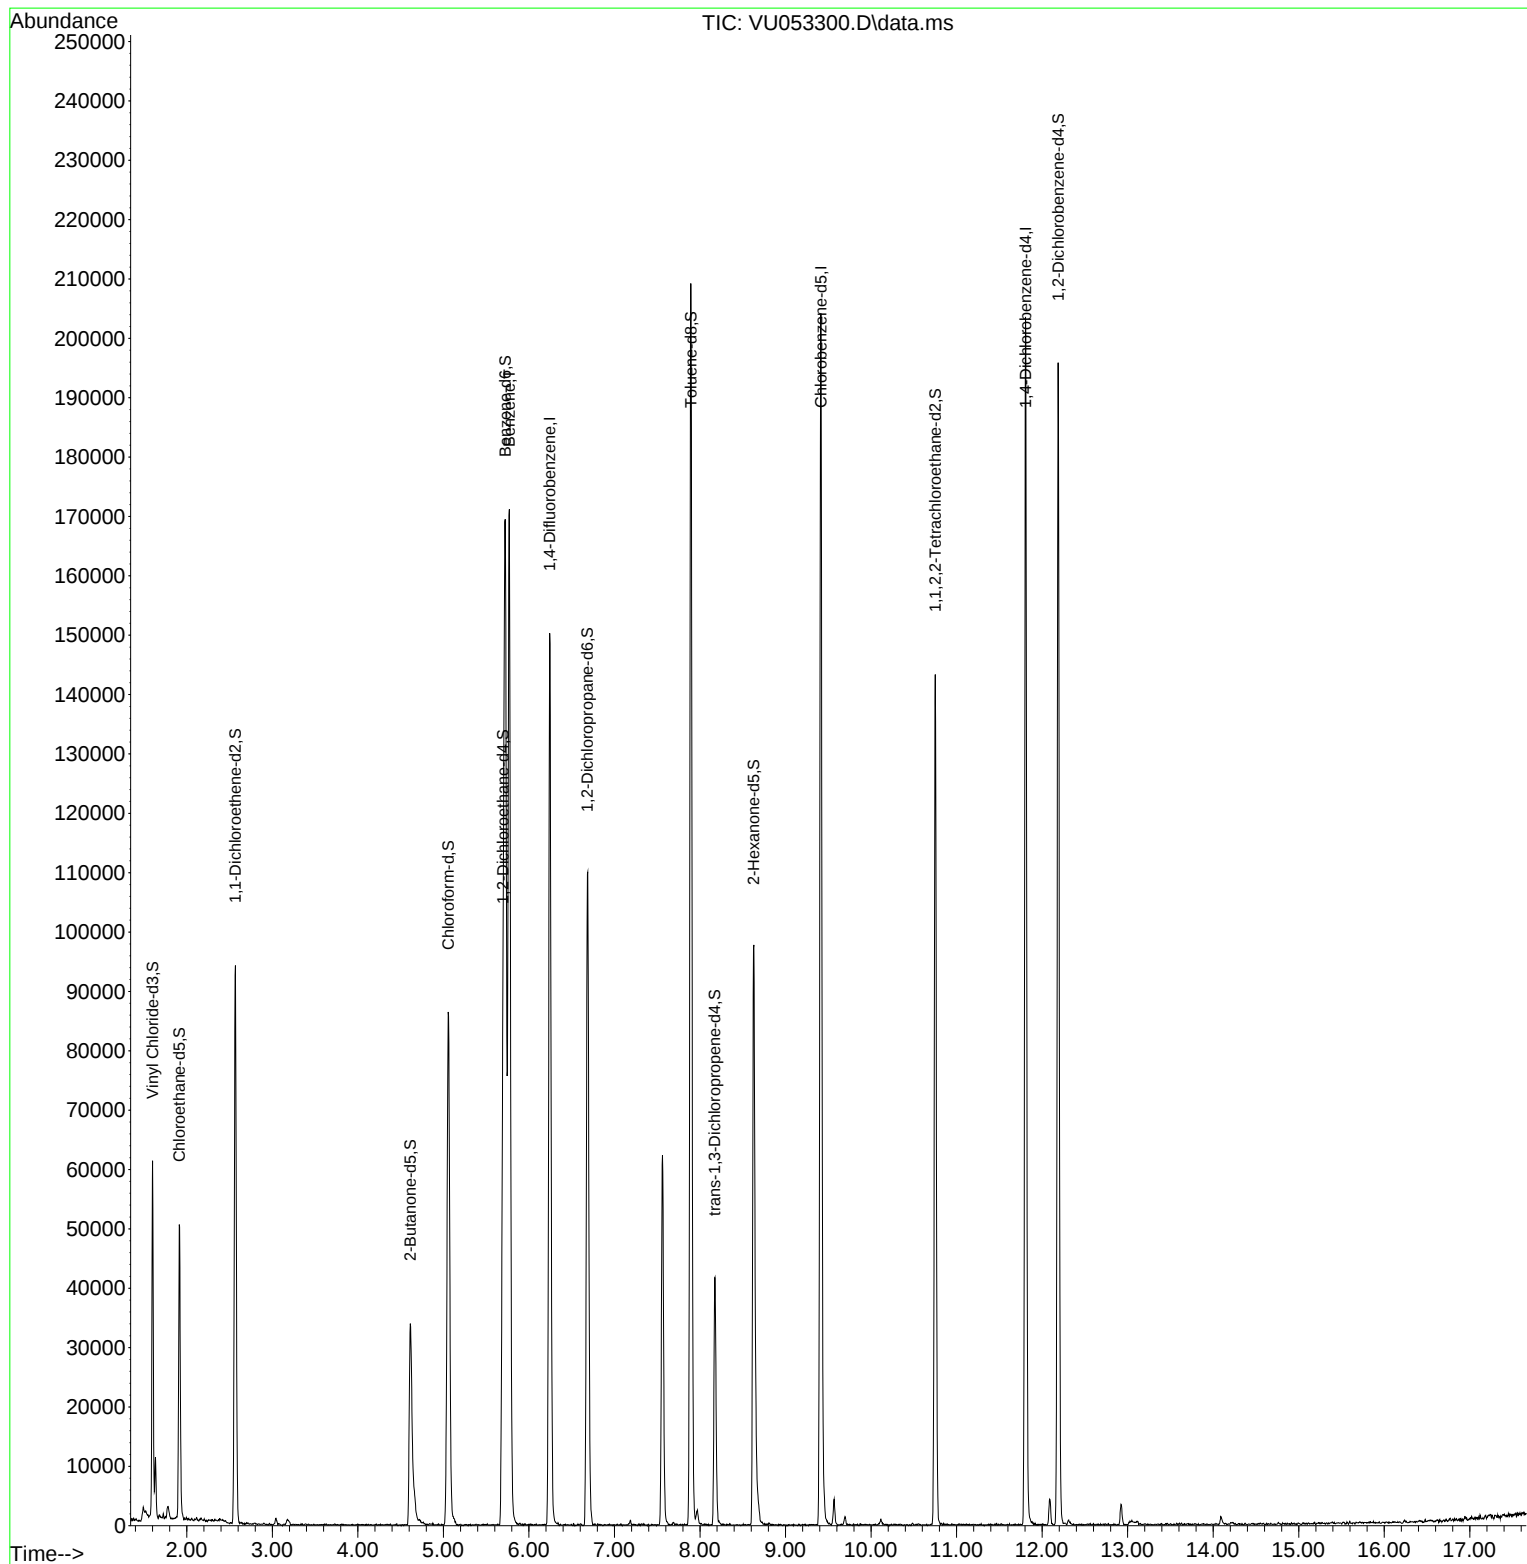

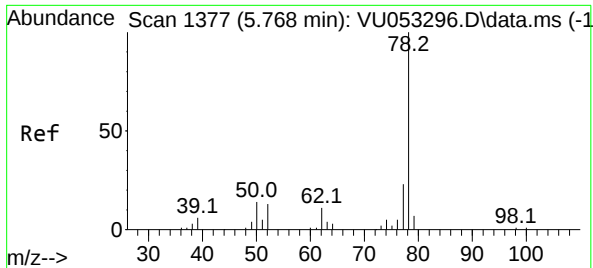

#33
Benzene
Concen: 44.360 ug/L
RT: 5.771 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU053300.D
Acq: 20 Mar 2023 12:18

Tgt Ion: 78 Resp: 162613

Instrument :
MSVOA_U
ClientSampleId :
EYFG0DL

