

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053298.D
 Acq On : 20 Mar 2023 11:31
 Operator : JC/MD
 Sample : 01929-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

Signal : TIC: VU053298.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	90	rBV2	190690	230430	15.49%	4.474%
2	1.916	171	179	192	rVB	54861	72160	4.85%	1.401%
3	2.568	370	382	397	rBV	101770	164033	11.03%	3.185%
4	2.871	472	476	480	rBV2	208	182	0.01%	0.004%
5	3.183	566	573	581	rBV3	692	1285	0.09%	0.025%
6	3.350	621	625	635	rVB4	1395	1937	0.13%	0.038%
7	3.488	665	668	673	rBV	177	154	0.01%	0.003%
8	3.816	765	770	774	rBB	196	233	0.02%	0.005%
9	3.842	774	778	780	rBV	159	164	0.01%	0.003%
10	4.334	929	931	937	rBB	169	173	0.01%	0.003%
11	4.388	943	948	953	rVV2	195	211	0.01%	0.004%
12	4.494	977	981	984	rBV	222	144	0.01%	0.003%
13	4.662	1009	1033	1066	rBV	626118	1487266	100.00%	28.879%
14	4.890	1102	1104	1105	rBV	210	107	0.01%	0.002%
15	5.057	1141	1156	1182	rBV2	89786	196760	13.23%	3.821%
16	5.202	1195	1201	1205	rBV2	270	376	0.03%	0.007%
17	5.292	1225	1229	1232	rBV	177	177	0.01%	0.003%
18	5.340	1240	1244	1249	rBV	177	241	0.02%	0.005%
19	5.395	1259	1261	1265	rVB2	251	174	0.01%	0.003%
20	5.433	1268	1273	1274	rBV	279	213	0.01%	0.004%
21	5.456	1278	1280	1284	rVB	242	145	0.01%	0.003%
22	5.533	1299	1304	1307	rBV	172	207	0.01%	0.004%
23	5.591	1317	1322	1323	rBV	183	175	0.01%	0.003%
24	5.723	1342	1363	1374	rBV2	175767	482615	32.45%	9.371%
25	5.845	1399	1401	1405	rVB	269	189	0.01%	0.004%
26	5.909	1419	1421	1423	rBV	168	110	0.01%	0.002%
27	6.041	1459	1462	1464	rBV2	354	190	0.01%	0.004%
28	6.115	1483	1485	1488	rVB2	244	113	0.01%	0.002%
29	6.192	1508	1509	1512	rBV	218	116	0.01%	0.002%
30	6.243	1512	1525	1549	rVV	152054	285420	19.19%	5.542%
31	6.414	1572	1578	1582	rBV3	371	425	0.03%	0.008%
32	6.504	1601	1606	1607	rBV	165	164	0.01%	0.003%
33	6.539	1608	1617	1628	rVB6	4686	8513	0.57%	0.165%
34	6.584	1628	1631	1632	rBV6	239	122	0.01%	0.002%
35	6.687	1648	1663	1683	rBV	111942	215930	14.52%	4.193%
36	6.887	1720	1725	1727	rBV	288	225	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053298.D
 Acq On : 20 Mar 2023 11:31
 Operator : JC/MD
 Sample : 01929-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.925	1734	1737	1738	rBV	144	100	0.01%	0.002%
38	7.157	1805	1809	1811	rBV2	169	155	0.01%	0.003%
39	7.182	1811	1817	1826	rVV4	921	1161	0.08%	0.023%
40	7.292	1846	1851	1859	rBB	211	322	0.02%	0.006%
41	7.372	1873	1876	1878	rBV	171	139	0.01%	0.003%
42	7.562	1923	1935	1955	rBV	63439	110989	7.46%	2.155%
43	7.684	1970	1973	1975	rBV	547	355	0.02%	0.007%
44	7.729	1984	1987	1990	rBV	170	101	0.01%	0.002%
45	7.822	2013	2016	2019	rBB	165	126	0.01%	0.002%
46	7.838	2019	2021	2023	rBV	152	104	0.01%	0.002%
47	7.893	2024	2038	2055	rBV	219643	374761	25.20%	7.277%
48	8.009	2070	2074	2076	rBV	338	229	0.02%	0.004%
49	8.034	2079	2082	2085	rVB2	320	207	0.01%	0.004%
50	8.173	2114	2125	2139	rBV2	41563	71260	4.79%	1.384%
51	8.295	2161	2163	2166	rBV	268	194	0.01%	0.004%
52	8.443	2206	2209	2210	rBV	156	114	0.01%	0.002%
53	8.584	2250	2253	2256	rBV	198	194	0.01%	0.004%
54	8.629	2256	2267	2295	rBV3	104499	201331	13.54%	3.909%
55	8.960	2367	2370	2375	rVB2	277	298	0.02%	0.006%
56	8.983	2375	2377	2378	rBV2	232	110	0.01%	0.002%
57	9.147	2425	2428	2432	rVB2	157	104	0.01%	0.002%
58	9.247	2453	2459	2465	rBV	243	474	0.03%	0.009%
59	9.414	2498	2511	2531	rBV	205357	346317	23.29%	6.725%
60	9.542	2549	2551	2552	rBV	273	108	0.01%	0.002%
61	9.568	2555	2559	2563	rVB2	321	297	0.02%	0.006%
62	9.639	2573	2581	2587	rBB	233	436	0.03%	0.008%
63	9.674	2588	2592	2596	rBV	187	253	0.02%	0.005%
64	9.877	2650	2655	2663	rBB2	301	488	0.03%	0.009%
65	9.915	2664	2667	2672	rBV	223	253	0.02%	0.005%
66	9.976	2683	2686	2689	rBB2	263	207	0.01%	0.004%
67	10.002	2690	2694	2697	rBB	167	127	0.01%	0.002%
68	10.025	2698	2701	2703	rBV	188	153	0.01%	0.003%
69	10.115	2724	2729	2730	rBV	328	213	0.01%	0.004%
70	10.224	2760	2763	2765	rBV	170	143	0.01%	0.003%
71	10.259	2771	2774	2775	rBV	223	119	0.01%	0.002%
72	10.298	2783	2786	2789	rBV2	220	153	0.01%	0.003%
73	10.394	2813	2816	2819	rBV	287	197	0.01%	0.004%
74	10.488	2841	2845	2850	rBV	222	295	0.02%	0.006%
75	10.578	2870	2873	2875	rBV2	287	177	0.01%	0.003%
76	10.636	2889	2891	2895	rVB	327	203	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053298.D
 Acq On : 20 Mar 2023 11:31
 Operator : JC/MD
 Sample : 01929-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.665	2896	2900	2902	rBV	252	212	0.01%	0.004%
78	10.751	2915	2927	2944	rBV	142594	228634	15.37%	4.439%
79	11.144	3046	3049	3051	rBV	173	136	0.01%	0.003%
80	11.214	3067	3071	3073	rBV2	211	156	0.01%	0.003%
81	11.337	3106	3109	3111	rVV	279	185	0.01%	0.004%
82	11.407	3126	3131	3136	rBV2	284	358	0.02%	0.007%
83	11.488	3153	3156	3163	rBV	207	200	0.01%	0.004%
84	11.806	3244	3255	3277	rBV	209256	333069	22.39%	6.467%
85	11.947	3296	3299	3300	rBV	215	123	0.01%	0.002%
86	12.189	3361	3374	3392	rBV	198639	320694	21.56%	6.227%
87	12.391	3434	3437	3438	rBV	152	108	0.01%	0.002%
88	12.427	3444	3448	3452	rBV	262	186	0.01%	0.004%
89	12.449	3452	3455	3460	rVV	210	171	0.01%	0.003%
90	13.066	3644	3647	3651	rBV2	189	132	0.01%	0.003%
91	13.179	3678	3682	3685	rBV	190	148	0.01%	0.003%
92	13.594	3808	3811	3815	rVB	322	222	0.01%	0.004%
93	13.632	3821	3823	3825	rBV	192	110	0.01%	0.002%
94	13.722	3849	3851	3854	rBV2	186	105	0.01%	0.002%
95	13.867	3894	3896	3898	rBV2	184	113	0.01%	0.002%
96	13.912	3907	3910	3912	rBV	227	155	0.01%	0.003%
97	14.996	4243	4247	4250	rBV2	200	150	0.01%	0.003%
98	15.066	4268	4269	4274	rBV2	247	128	0.01%	0.002%
99	15.266	4328	4331	4335	rBV2	349	337	0.02%	0.007%
100	15.362	4358	4361	4364	rBV2	266	184	0.01%	0.004%




Sum of corrected areas: 5150062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053298.D
Acq On : 20 Mar 2023 11:31
Operator : JC/MD
Sample : 01929-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

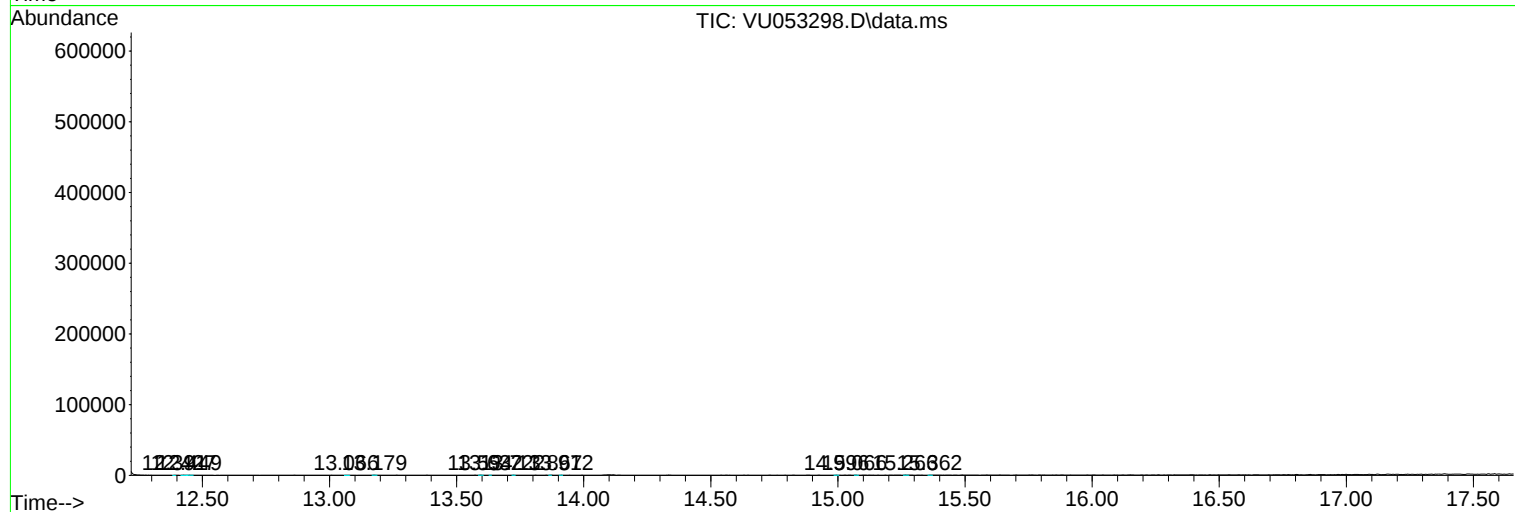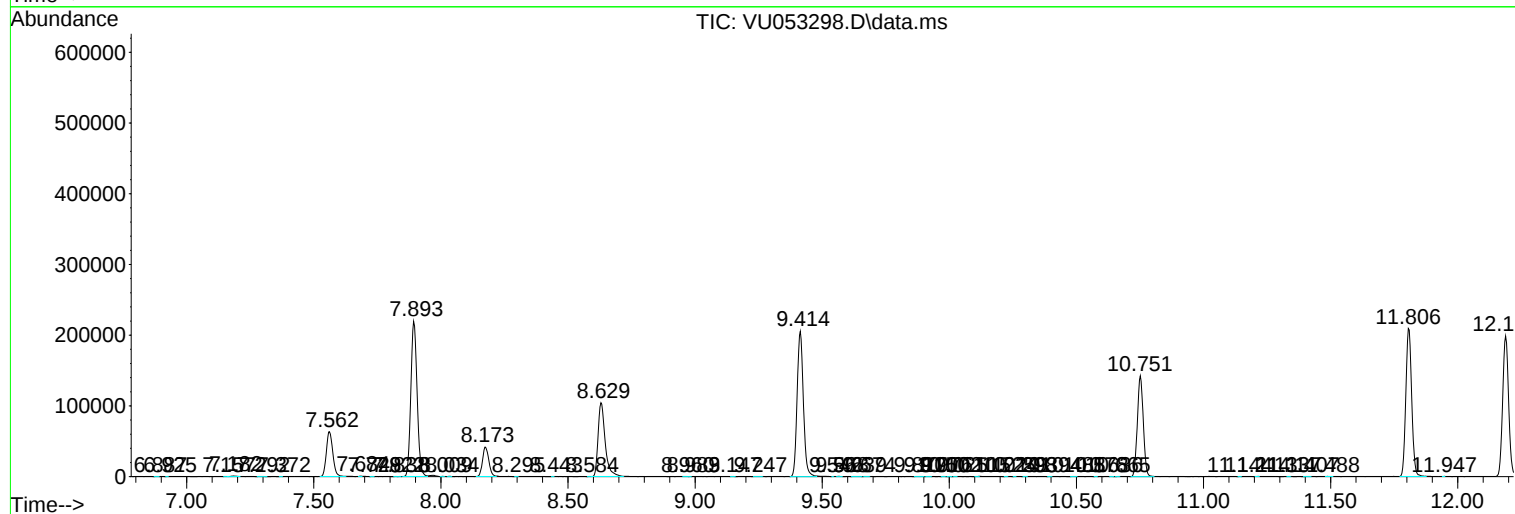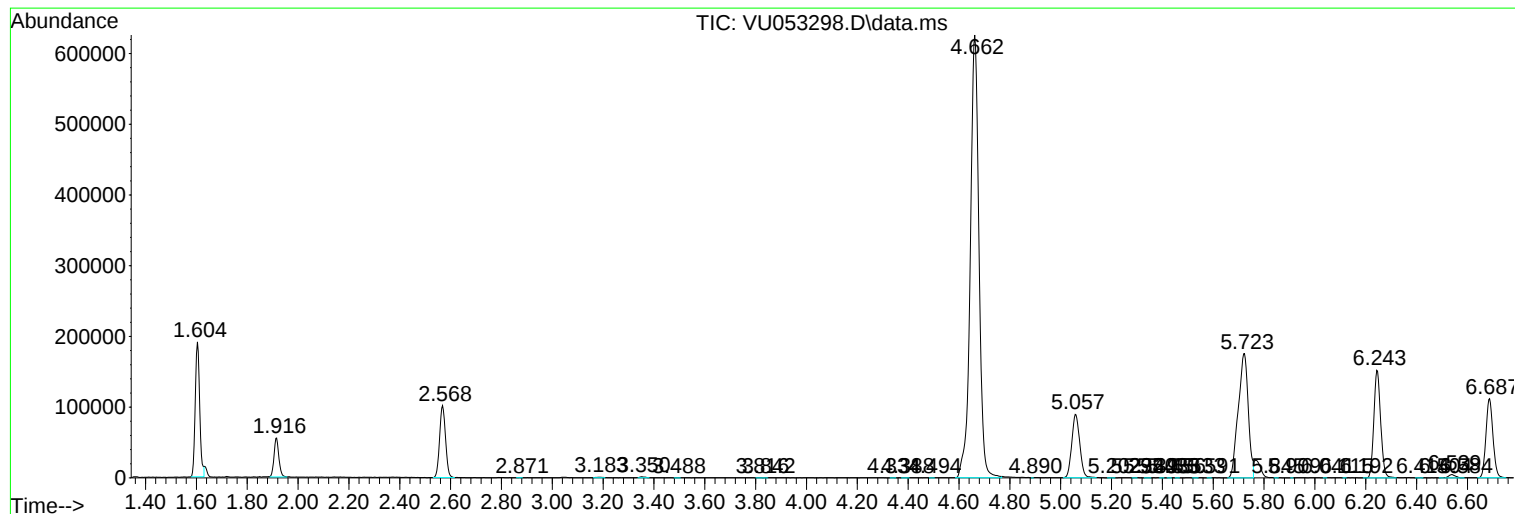

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053298.D
Acq On : 20 Mar 2023 11:31
Operator : JC/MD
Sample : 01929-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053298.D
Acq On : 20 Mar 2023 11:31
Operator : JC/MD
Sample : 01929-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc