

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053299.D
 Acq On : 20 Mar 2023 11:54
 Operator : JC/MD
 Sample : VIBLK115
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	87	rBV	57171	64765	13.63%	1.863%
2	1.912	170	178	197	rVB	49064	66396	13.97%	1.910%
3	2.568	370	382	396	rVB	92345	148400	31.22%	4.268%
4	2.990	510	513	517	rBV2	190	117	0.02%	0.003%
5	3.044	525	530	538	rVB2	995	1272	0.27%	0.037%
6	3.179	562	572	573	rBV2	1100	1343	0.28%	0.039%
7	3.488	665	668	671	rVB	205	120	0.03%	0.003%
8	4.166	876	879	882	rBV	304	227	0.05%	0.007%
9	4.218	891	895	897	rBV2	309	285	0.06%	0.008%
10	4.244	900	903	908	rVB2	219	166	0.03%	0.005%
11	4.276	908	913	914	rBV	202	201	0.04%	0.006%
12	4.414	953	956	961	rBV2	202	149	0.03%	0.004%
13	4.488	976	979	982	rBB	242	169	0.04%	0.005%
14	4.510	983	986	991	rBV	188	229	0.05%	0.007%
15	4.616	1007	1019	1051	rBV	35596	101486	21.35%	2.919%
16	5.057	1139	1156	1187	rBV	87979	192536	40.51%	5.537%
17	5.253	1214	1217	1222	rVB	300	252	0.05%	0.007%
18	5.282	1223	1226	1229	rBV	239	204	0.04%	0.006%
19	5.391	1257	1260	1262	rBV	248	149	0.03%	0.004%
20	5.452	1276	1279	1282	rBV	224	193	0.04%	0.006%
21	5.478	1285	1287	1290	rVB	206	108	0.02%	0.003%
22	5.584	1317	1320	1328	rBB	314	384	0.08%	0.011%
23	5.719	1342	1362	1374	rBV2	170277	475328	100.00%	13.671%
24	6.038	1457	1461	1465	rBV	277	290	0.06%	0.008%
25	6.243	1511	1525	1546	rBV	139657	267197	56.21%	7.685%
26	6.433	1581	1584	1587	rBV	198	167	0.04%	0.005%
27	6.478	1595	1598	1600	rBV	111	103	0.02%	0.003%
28	6.520	1608	1611	1614	rBV3	329	188	0.04%	0.005%
29	6.594	1631	1634	1637	rVB	296	189	0.04%	0.005%
30	6.613	1637	1640	1641	rBV	143	99	0.02%	0.003%
31	6.687	1649	1663	1685	rVV	109732	214190	45.06%	6.160%
32	6.764	1685	1687	1690	rBV2	175	131	0.03%	0.004%
33	6.809	1699	1701	1703	rVB	389	156	0.03%	0.004%
34	6.915	1731	1734	1738	rBV	204	212	0.04%	0.006%
35	6.944	1741	1743	1747	rBB	218	145	0.03%	0.004%
36	7.063	1773	1780	1783	rBV	177	296	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053299.D
 Acq On : 20 Mar 2023 11:54
 Operator : JC/MD
 Sample : VIBLK115
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.128	1796	1800	1804	rBV	154	203	0.04%	0.006%
38	7.186	1812	1818	1822	rBV2	1066	1089	0.23%	0.031%
39	7.231	1830	1832	1834	rBV	251	147	0.03%	0.004%
40	7.247	1834	1837	1840	rVB	200	118	0.02%	0.003%
41	7.324	1858	1861	1863	rBV2	198	117	0.02%	0.003%
42	7.456	1900	1902	1904	rBV	176	113	0.02%	0.003%
43	7.478	1907	1909	1912	rBV	150	126	0.03%	0.004%
44	7.562	1923	1935	1953	rBV	62741	110019	23.15%	3.164%
45	7.690	1970	1975	1976	rBV2	725	545	0.11%	0.016%
46	7.767	1996	1999	2001	rBV	138	113	0.02%	0.003%
47	7.812	2011	2013	2016	rBB	146	97	0.02%	0.003%
48	7.829	2016	2018	2021	rBB	160	106	0.02%	0.003%
49	7.851	2022	2025	2026	rBV	261	150	0.03%	0.004%
50	7.893	2026	2038	2054	rBV	210740	362528	76.27%	10.426%
51	8.176	2115	2126	2142	rBV	42630	71164	14.97%	2.047%
52	8.285	2158	2160	2164	rBB	130	112	0.02%	0.003%
53	8.311	2165	2168	2170	rBV2	258	163	0.03%	0.005%
54	8.578	2247	2251	2253	rBV	192	184	0.04%	0.005%
55	8.629	2256	2267	2294	rVV2	104456	202703	42.64%	5.830%
56	8.809	2320	2323	2325	rBB	166	114	0.02%	0.003%
57	9.044	2390	2396	2399	rBV	165	210	0.04%	0.006%
58	9.128	2420	2422	2425	rBV	167	135	0.03%	0.004%
59	9.202	2443	2445	2449	rVB2	189	121	0.03%	0.003%
60	9.263	2461	2464	2467	rBV	159	153	0.03%	0.004%
61	9.414	2493	2511	2535	rBV	195053	328396	69.09%	9.445%
62	9.536	2546	2549	2556	rVB2	401	394	0.08%	0.011%
63	9.574	2556	2561	2564	rBV2	289	304	0.06%	0.009%
64	9.616	2571	2574	2577	rBV	321	223	0.05%	0.006%
65	9.693	2595	2598	2599	rBV	254	129	0.03%	0.004%
66	9.738	2604	2612	2614	rBV	314	373	0.08%	0.011%
67	9.996	2689	2692	2695	rBV	219	186	0.04%	0.005%
68	10.050	2705	2709	2714	rBV	183	266	0.06%	0.008%
69	10.214	2757	2760	2764	rBV	327	252	0.05%	0.007%
70	10.259	2772	2774	2776	rBV	157	105	0.02%	0.003%
71	10.385	2810	2813	2815	rBV	290	202	0.04%	0.006%
72	10.410	2819	2821	2824	rVB	267	155	0.03%	0.004%
73	10.565	2866	2869	2872	rBV	196	173	0.04%	0.005%
74	10.751	2915	2927	2947	rVV	141543	228171	48.00%	6.562%
75	10.883	2963	2968	2974	rBV	291	437	0.09%	0.013%
76	10.999	2999	3004	3012	rBV	237	465	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053299.D
 Acq On : 20 Mar 2023 11:54
 Operator : JC/MD
 Sample : VIBLK115
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.092	3031	3033	3037	rBV	195	111	0.02%	0.003%
78	11.182	3059	3061	3065	rVB	266	161	0.03%	0.005%
79	11.201	3065	3067	3069	rBV	161	114	0.02%	0.003%
80	11.234	3074	3077	3079	rBV	199	161	0.03%	0.005%
81	11.590	3186	3188	3190	rBV	198	97	0.02%	0.003%
82	11.623	3195	3198	3200	rBV	190	161	0.03%	0.005%
83	11.684	3211	3217	3225	rBV2	331	537	0.11%	0.015%
84	11.806	3244	3255	3276	rBV	195168	310531	65.33%	8.931%
85	12.189	3362	3374	3396	rBV	194677	314157	66.09%	9.035%
86	12.311	3409	3412	3415	rBV	178	147	0.03%	0.004%
87	12.796	3561	3563	3568	rBV2	146	100	0.02%	0.003%
88	13.272	3708	3711	3714	rBV	203	117	0.02%	0.003%
89	13.301	3717	3720	3722	rBV	232	126	0.03%	0.004%
90	13.764	3861	3864	3867	rBV	171	97	0.02%	0.003%
91	13.783	3867	3870	3873	rVB	209	100	0.02%	0.003%
92	13.967	3923	3927	3930	rBV	282	224	0.05%	0.006%
93	14.401	4059	4062	4066	rBV	229	186	0.04%	0.005%
94	14.581	4115	4118	4121	rVB2	344	189	0.04%	0.005%
95	14.851	4199	4202	4203	rBV	257	146	0.03%	0.004%
96	15.098	4277	4279	4282	rVB	257	122	0.03%	0.004%
97	15.188	4304	4307	4312	rBV2	315	284	0.06%	0.008%
98	15.320	4345	4348	4352	rBV	216	219	0.05%	0.006%
99	15.449	4385	4388	4391	rVB	344	201	0.04%	0.006%
100	15.465	4391	4393	4394	rBV	231	106	0.02%	0.003%




Sum of corrected areas: 3476997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053299.D
Acq On : 20 Mar 2023 11:54
Operator : JC/MD
Sample : VIBLK115
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

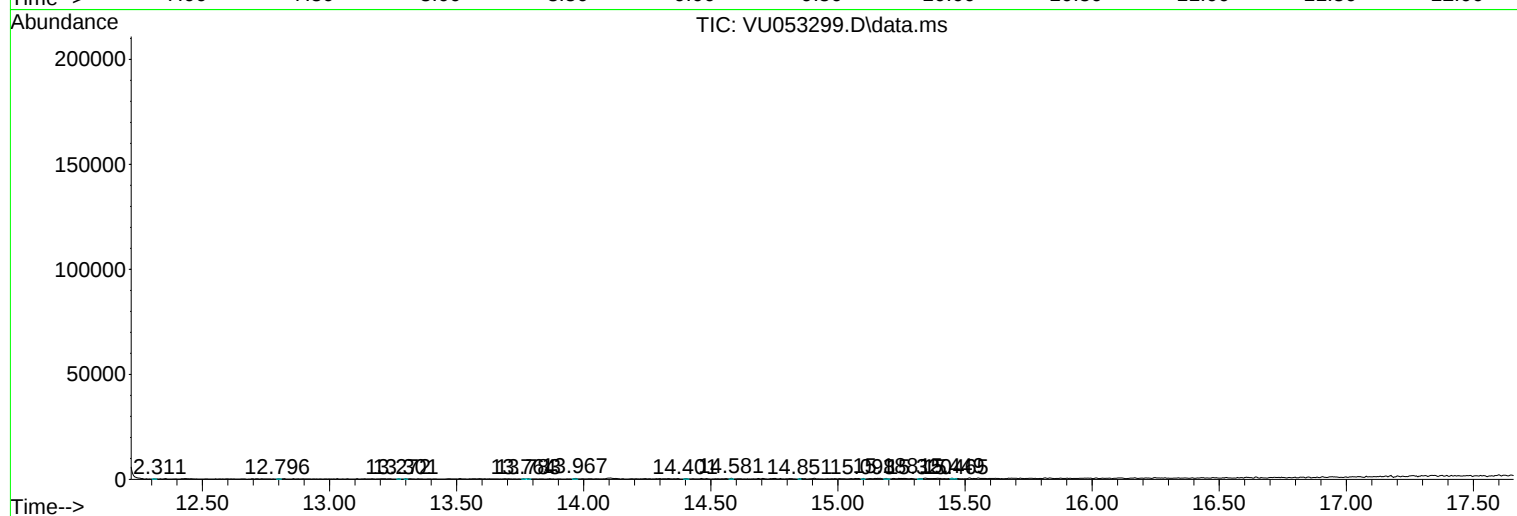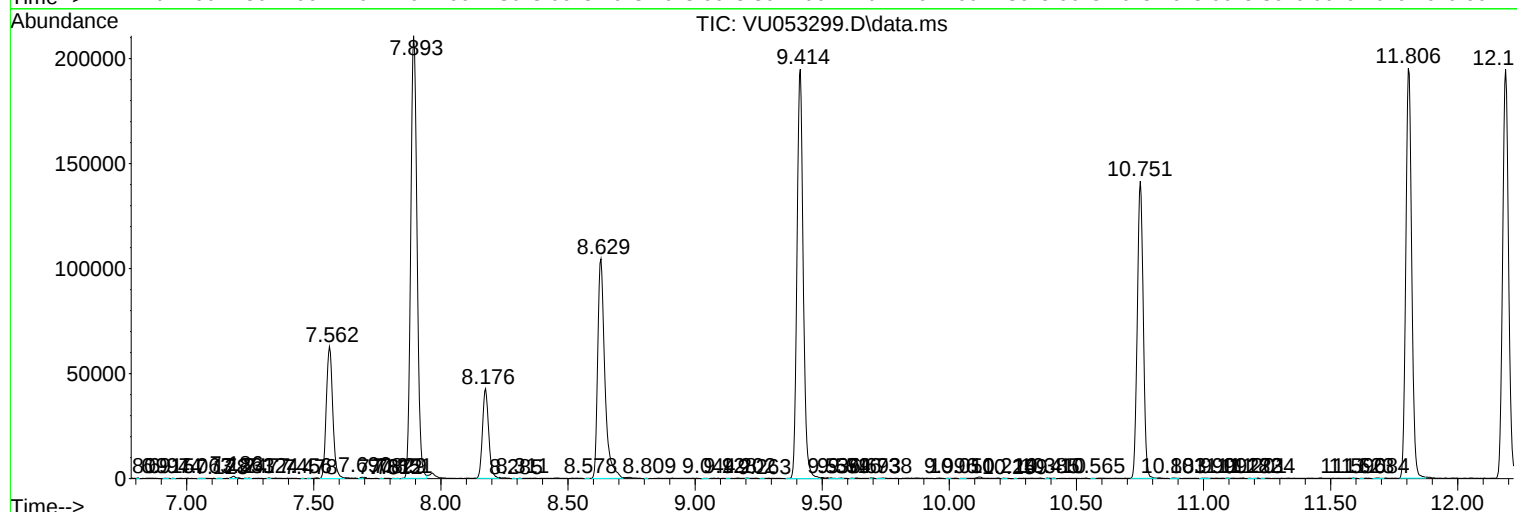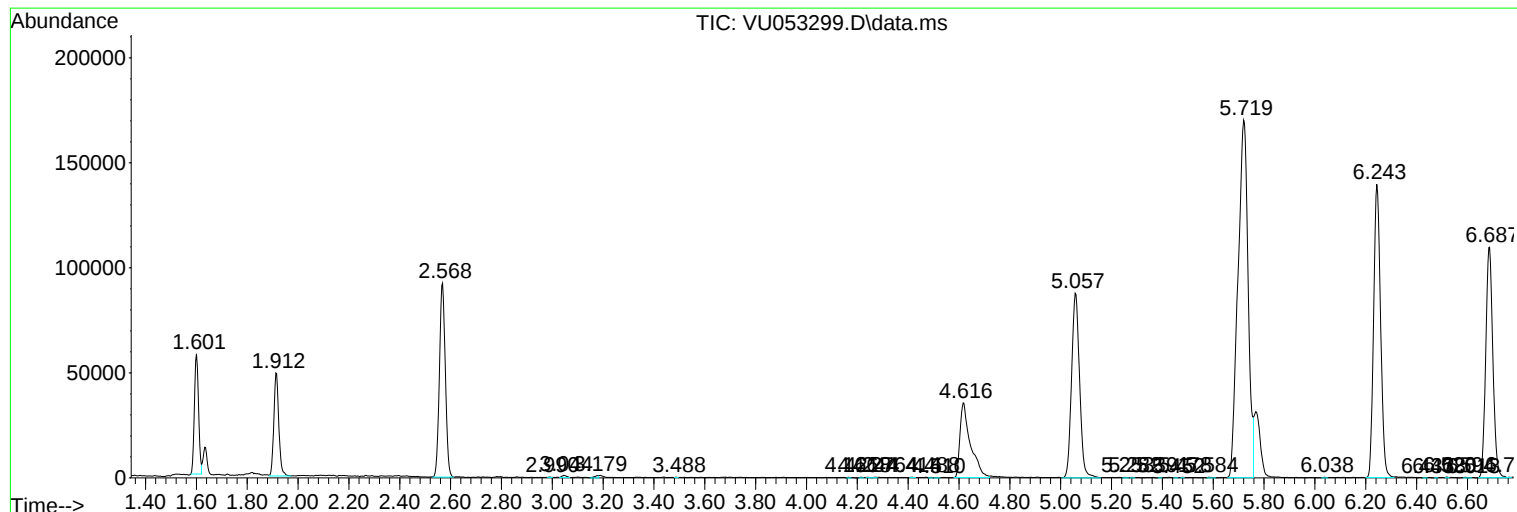

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053299.D
Acq On : 20 Mar 2023 11:54
Operator : JC/MD
Sample : VIBLK115
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053299.D
Acq On : 20 Mar 2023 11:54
Operator : JC/MD
Sample : VIBLK115
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------