

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053300.D
 Acq On : 20 Mar 2023 12:18
 Operator : JC/MD
 Sample : 01930-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	87	rBV	59087	64192	13.84%	1.835%
2	1.912	171	178	195	rVB	49771	67253	14.50%	1.922%
3	2.568	370	382	396	rBV	93967	150159	32.38%	4.292%
4	2.967	503	506	510	rBV	243	142	0.03%	0.004%
5	3.134	553	558	563	rBV	278	427	0.09%	0.012%
6	4.099	856	858	862	rVB	166	92	0.02%	0.003%
7	4.452	966	968	973	rVB2	338	257	0.06%	0.007%
8	4.546	994	997	998	rBV	203	144	0.03%	0.004%
9	4.613	1007	1018	1048	rBV2	33877	85900	18.52%	2.455%
10	4.806	1076	1078	1084	rVB	167	117	0.03%	0.003%
11	4.838	1084	1088	1093	rBV2	232	263	0.06%	0.008%
12	4.877	1099	1100	1104	rVB	326	113	0.02%	0.003%
13	4.941	1118	1120	1127	rVB2	217	155	0.03%	0.004%
14	5.057	1140	1156	1181	rBV	86387	190220	41.01%	5.437%
15	5.189	1193	1197	1199	rBV	186	194	0.04%	0.006%
16	5.256	1212	1218	1220	rBV	224	289	0.06%	0.008%
17	5.298	1228	1231	1232	rBV	188	134	0.03%	0.004%
18	5.333	1239	1242	1243	rBV	145	104	0.02%	0.003%
19	5.513	1296	1298	1304	rVB	214	137	0.03%	0.004%
20	5.636	1334	1336	1342	rVB	195	121	0.03%	0.003%
21	5.722	1342	1363	1370	rBV2	169431	463789	100.00%	13.257%
22	5.922	1422	1425	1428	rVB2	312	222	0.05%	0.006%
23	5.957	1429	1436	1441	rBV	340	520	0.11%	0.015%
24	6.018	1452	1455	1460	rVB	208	160	0.03%	0.005%
25	6.243	1512	1525	1553	rBV	150196	280487	60.48%	8.017%
26	6.369	1560	1564	1565	rBV	240	171	0.04%	0.005%
27	6.523	1610	1612	1615	rBB	385	194	0.04%	0.006%
28	6.603	1634	1637	1645	rVB2	332	413	0.09%	0.012%
29	6.687	1650	1663	1682	rVV	109990	213760	46.09%	6.110%
30	6.806	1697	1700	1703	rVB2	223	126	0.03%	0.004%
31	6.941	1739	1742	1744	rBV	172	92	0.02%	0.003%
32	6.992	1755	1758	1760	rBV	201	161	0.03%	0.005%
33	7.076	1780	1784	1788	rVB2	336	309	0.07%	0.009%
34	7.099	1788	1791	1797	rBV	182	244	0.05%	0.007%
35	7.166	1809	1812	1813	rBV	183	94	0.02%	0.003%
36	7.282	1845	1848	1851	rBV	288	223	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053300.D
 Acq On : 20 Mar 2023 12:18
 Operator : JC/MD
 Sample : 01930-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.317	1854	1859	1865	rBV2	315	446	0.10%	0.013%
38	7.343	1865	1867	1870	rVB	220	98	0.02%	0.003%
39	7.398	1880	1884	1887	rBB2	280	220	0.05%	0.006%
40	7.504	1913	1917	1920	rBV	206	219	0.05%	0.006%
41	7.562	1923	1935	1957	rVV	62337	109650	23.64%	3.134%
42	7.687	1971	1974	1979	rVB3	428	431	0.09%	0.012%
43	7.893	2025	2038	2054	rBV	209064	365034	78.71%	10.434%
44	8.095	2099	2101	2103	rVB	241	93	0.02%	0.003%
45	8.115	2104	2107	2110	rBV	177	163	0.04%	0.005%
46	8.176	2115	2126	2138	rBV2	41701	70108	15.12%	2.004%
47	8.259	2149	2152	2156	rBV2	194	119	0.03%	0.003%
48	8.349	2177	2180	2183	rVB	227	124	0.03%	0.004%
49	8.488	2220	2223	2226	rBV	145	156	0.03%	0.004%
50	8.629	2253	2267	2296	rBV2	97686	190580	41.09%	5.447%
51	8.783	2312	2315	2318	rBV	153	114	0.02%	0.003%
52	8.922	2356	2358	2359	rBV	240	95	0.02%	0.003%
53	8.980	2373	2376	2381	rBV	198	247	0.05%	0.007%
54	9.041	2391	2395	2399	rBV	209	229	0.05%	0.007%
55	9.095	2410	2412	2416	rBV	285	225	0.05%	0.006%
56	9.153	2427	2430	2436	rBB2	278	300	0.06%	0.009%
57	9.246	2457	2459	2461	rBV	147	99	0.02%	0.003%
58	9.279	2466	2469	2473	rBV	230	241	0.05%	0.007%
59	9.414	2498	2511	2534	rBV	204083	342754	73.90%	9.797%
60	9.568	2549	2559	2572	rVB	4464	6600	1.42%	0.189%
61	9.619	2572	2575	2577	rBV	164	138	0.03%	0.004%
62	9.652	2583	2585	2589	rBV	158	93	0.02%	0.003%
63	9.697	2592	2599	2606	rVB4	1426	1938	0.42%	0.055%
64	9.725	2606	2608	2614	rBV	196	129	0.03%	0.004%
65	9.796	2627	2630	2633	rBV	318	239	0.05%	0.007%
66	9.841	2643	2644	2649	rVB	232	159	0.03%	0.005%
67	9.873	2650	2654	2656	rBV	345	281	0.06%	0.008%
68	10.050	2707	2709	2715	rVB2	173	115	0.02%	0.003%
69	10.208	2755	2758	2761	rBB	178	132	0.03%	0.004%
70	10.240	2761	2768	2771	rBV	278	363	0.08%	0.010%
71	10.388	2811	2814	2819	rBV	197	226	0.05%	0.006%
72	10.452	2830	2834	2838	rBB	190	206	0.04%	0.006%
73	10.488	2839	2845	2849	rBV3	404	552	0.12%	0.016%
74	10.555	2861	2866	2868	rBV2	192	179	0.04%	0.005%
75	10.651	2894	2896	2898	rVB	246	97	0.02%	0.003%
76	10.674	2899	2903	2906	rBV	157	191	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053300.D
 Acq On : 20 Mar 2023 12:18
 Operator : JC/MD
 Sample : 01930-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2945	rVB	143214	225460	48.61%	6.444%
78	10.851	2956	2958	2962	rVB	247	100	0.02%	0.003%
79	11.115	3037	3040	3043	rBV2	162	106	0.02%	0.003%
80	11.330	3104	3107	3110	rBV	172	164	0.04%	0.005%
81	11.465	3146	3149	3152	rVB2	305	192	0.04%	0.005%
82	11.520	3164	3166	3171	rBV2	202	161	0.03%	0.005%
83	11.619	3195	3197	3204	rVB	190	99	0.02%	0.003%
84	11.684	3214	3217	3222	rBV	193	146	0.03%	0.004%
85	11.806	3244	3255	3276	rBV	203327	325055	70.09%	9.291%
86	11.912	3285	3288	3289	rBV	174	91	0.02%	0.003%
87	12.089	3335	3343	3350	rBV2	4265	6150	1.33%	0.176%
88	12.188	3359	3374	3393	rBV	195797	315896	68.11%	9.029%
89	12.311	3405	3412	3422	rBV2	786	1308	0.28%	0.037%
90	12.922	3595	3602	3612	rBV3	3422	5307	1.14%	0.152%
91	13.015	3628	3631	3632	rBV2	368	204	0.04%	0.006%
92	13.446	3762	3765	3767	rBV2	173	97	0.02%	0.003%
93	13.590	3808	3810	3812	rBV	149	93	0.02%	0.003%
94	13.632	3819	3823	3827	rVB2	320	262	0.06%	0.007%
95	13.661	3830	3832	3835	rVV	182	90	0.02%	0.003%
96	14.089	3960	3965	3978	rVB2	1270	1911	0.41%	0.055%
97	14.375	4050	4054	4057	rBV	244	180	0.04%	0.005%
98	14.812	4186	4190	4191	rBV2	299	175	0.04%	0.005%
99	15.211	4311	4314	4315	rBV2	188	111	0.02%	0.003%
100	15.597	4429	4434	4438	rBV2	468	446	0.10%	0.013%




Sum of corrected areas: 3498565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053300.D
Acq On : 20 Mar 2023 12:18
Operator : JC/MD
Sample : 01930-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

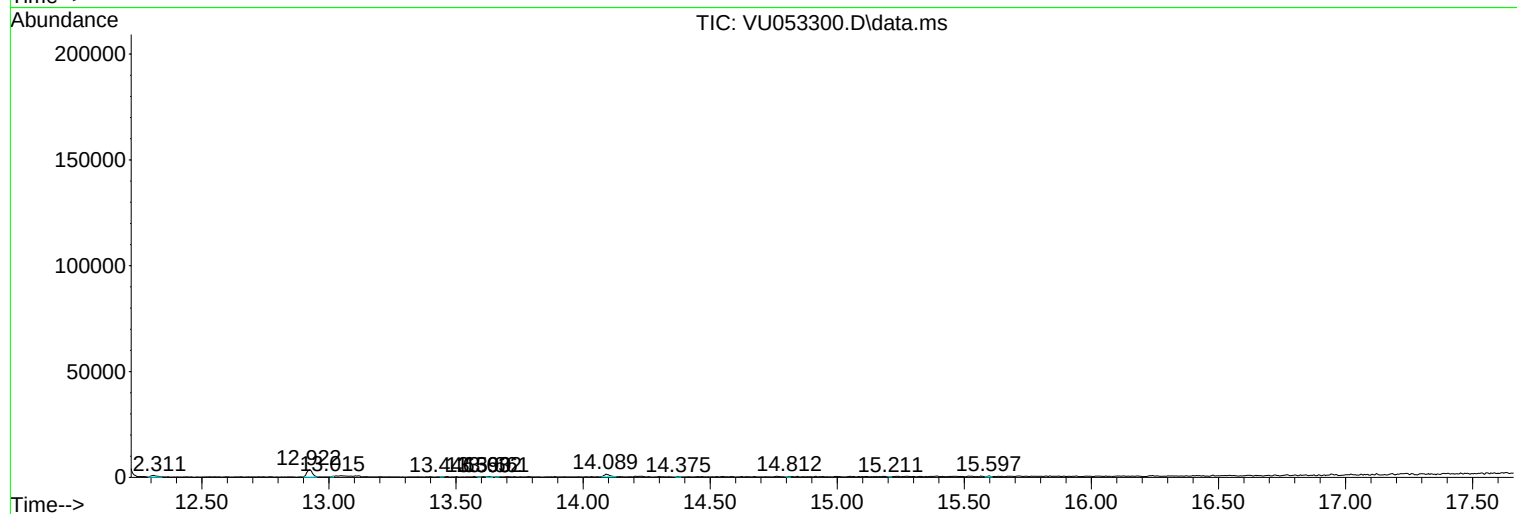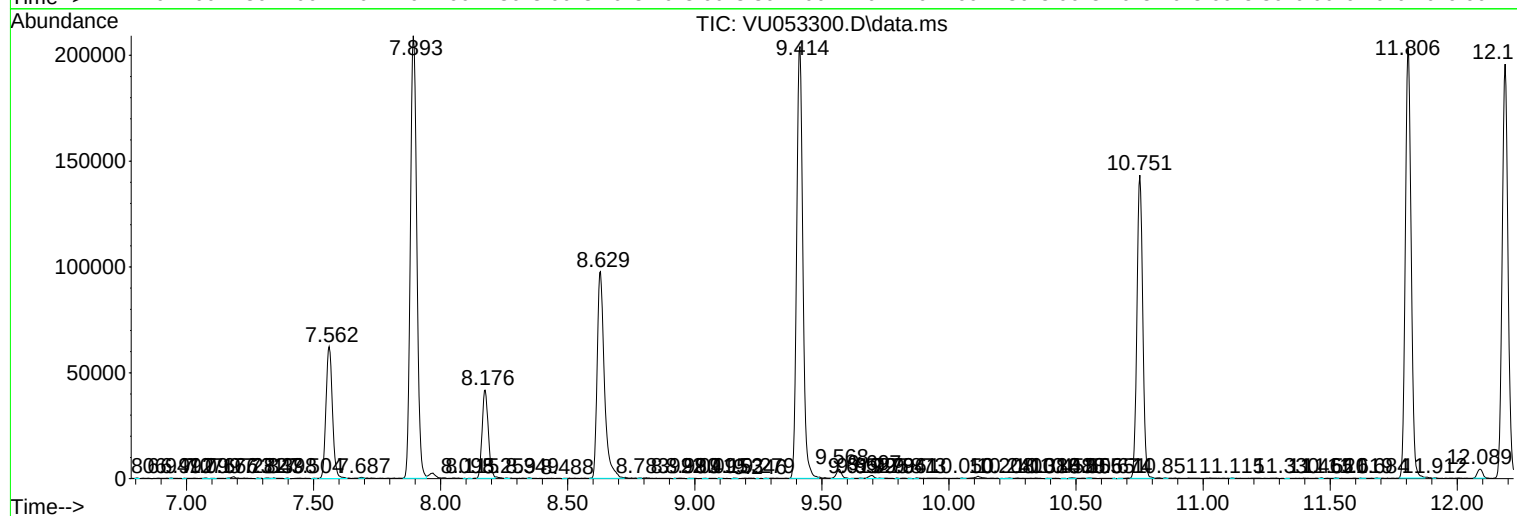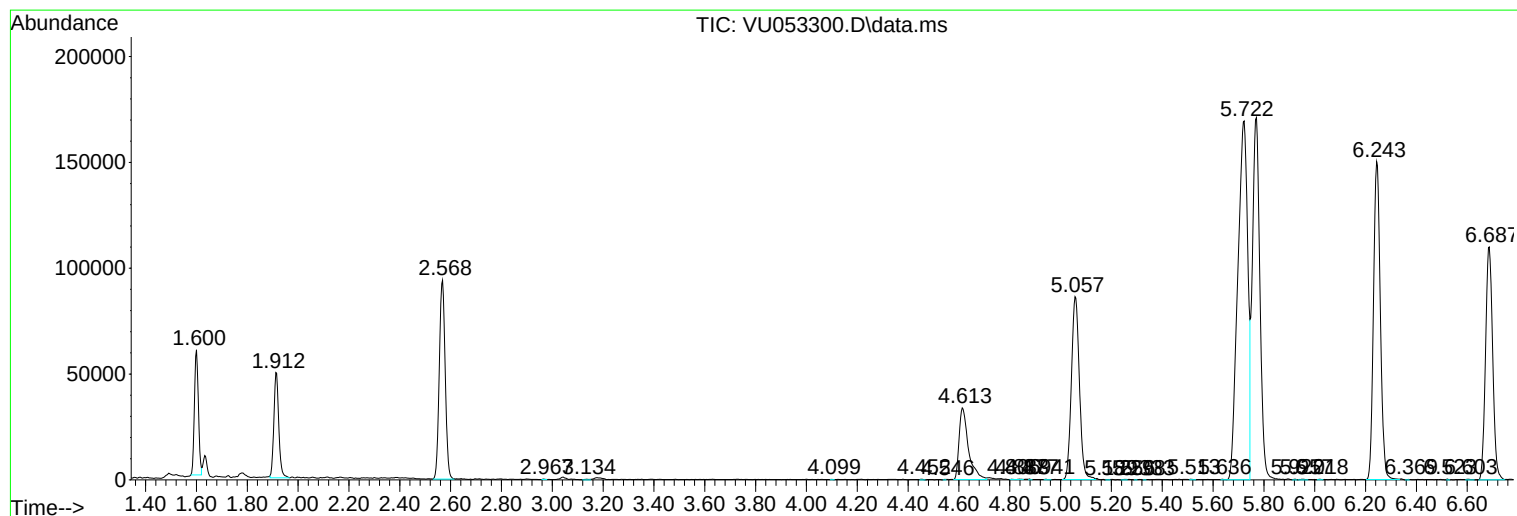

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053300.D
Acq On : 20 Mar 2023 12:18
Operator : JC/MD
Sample : 01930-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053300.D
Acq On : 20 Mar 2023 12:18
Operator : JC/MD
Sample : 01930-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------