

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053301.D
 Acq On : 20 Mar 2023 12:40
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	89	rBV2	132873	160165	33.30%	4.506%
2	1.912	171	178	191	rVB	48654	64338	13.37%	1.810%
3	2.568	370	382	396	rVB	94756	152606	31.72%	4.293%
4	2.623	396	399	402	rBV	334	285	0.06%	0.008%
5	2.990	511	513	514	rBV	170	60	0.01%	0.002%
6	3.012	518	520	521	rBV	181	80	0.02%	0.002%
7	3.047	524	531	539	rVV3	908	1377	0.29%	0.039%
8	3.121	552	554	556	rVB	160	63	0.01%	0.002%
9	3.353	622	626	628	rBV2	245	203	0.04%	0.006%
10	3.462	658	660	664	rBV	137	104	0.02%	0.003%
11	3.694	730	732	734	rBV2	118	66	0.01%	0.002%
12	4.028	835	836	837	rBV	130	50	0.01%	0.001%
13	4.195	885	888	892	rBV	224	187	0.04%	0.005%
14	4.292	916	918	923	rVB2	145	125	0.03%	0.004%
15	4.465	969	972	978	rVB	253	209	0.04%	0.006%
16	4.491	978	980	983	rVB	290	159	0.03%	0.004%
17	4.507	983	985	988	rBV	127	113	0.02%	0.003%
18	4.526	988	991	994	rBV2	173	112	0.02%	0.003%
19	4.575	1002	1006	1008	rBV	203	204	0.04%	0.006%
20	4.616	1008	1019	1024	rBV	33480	64690	13.45%	1.820%
21	4.874	1096	1099	1103	rVB	417	402	0.08%	0.011%
22	4.903	1104	1108	1114	rBB	337	306	0.06%	0.009%
23	4.944	1117	1121	1124	rBV	334	285	0.06%	0.008%
24	5.057	1141	1156	1176	rBV	87776	192483	40.01%	5.415%
25	5.192	1196	1198	1201	rBV	142	96	0.02%	0.003%
26	5.231	1207	1210	1217	rBV	198	324	0.07%	0.009%
27	5.269	1220	1222	1227	rVV	170	95	0.02%	0.003%
28	5.372	1253	1254	1256	rBV	114	63	0.01%	0.002%
29	5.411	1264	1266	1268	rBV	132	97	0.02%	0.003%
30	5.443	1273	1276	1280	rBB	147	140	0.03%	0.004%
31	5.469	1281	1284	1287	rBB	269	197	0.04%	0.006%
32	5.497	1288	1293	1295	rBV	172	174	0.04%	0.005%
33	5.549	1307	1309	1311	rBV	156	111	0.02%	0.003%
34	5.719	1341	1362	1374	rBV3	173386	481047	100.00%	13.533%
35	5.880	1408	1412	1414	rBV	158	131	0.03%	0.004%
36	5.893	1414	1416	1420	rVB	185	112	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053301.D
 Acq On : 20 Mar 2023 12:40
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	5.986	1442	1445	1446	rBV	170	115	0.02%	0.003%
38	6.051	1464	1465	1469	rBV	115	53	0.01%	0.001%
39	6.079	1471	1474	1479	rVB2	272	260	0.05%	0.007%
40	6.124	1486	1488	1490	rBV	153	109	0.02%	0.003%
41	6.186	1503	1507	1509	rBB	135	114	0.02%	0.003%
42	6.243	1510	1525	1545	rBV	143042	269677	56.06%	7.587%
43	6.517	1607	1610	1613	rBV2	229	169	0.04%	0.005%
44	6.568	1623	1626	1628	rBV	244	162	0.03%	0.005%
45	6.620	1638	1642	1646	rVB2	354	327	0.07%	0.009%
46	6.687	1647	1663	1683	rBV	109544	214400	44.57%	6.032%
47	6.790	1692	1695	1697	rBV	336	235	0.05%	0.007%
48	6.806	1698	1700	1703	rVV	237	120	0.02%	0.003%
49	6.822	1703	1705	1707	rVV	150	72	0.01%	0.002%
50	7.182	1810	1817	1818	rBV	436	360	0.07%	0.010%
51	7.475	1906	1908	1911	rVB	157	69	0.01%	0.002%
52	7.562	1923	1935	1953	rBV	63928	109651	22.79%	3.085%
53	7.655	1962	1964	1969	rBV2	162	117	0.02%	0.003%
54	7.690	1971	1975	1984	rVB3	411	517	0.11%	0.015%
55	7.722	1984	1985	1987	rBV	122	49	0.01%	0.001%
56	7.845	2019	2023	2026	rBV2	178	138	0.03%	0.004%
57	7.893	2026	2038	2053	rBV	214626	366726	76.23%	10.317%
58	8.050	2085	2087	2089	rBV2	164	92	0.02%	0.003%
59	8.118	2106	2108	2111	rBB	240	112	0.02%	0.003%
60	8.137	2111	2114	2115	rBV	136	97	0.02%	0.003%
61	8.173	2115	2125	2142	rVV	41314	71697	14.90%	2.017%
62	8.317	2167	2170	2172	rBV	284	181	0.04%	0.005%
63	8.404	2192	2197	2199	rBV	155	199	0.04%	0.006%
64	8.510	2227	2230	2231	rBV	160	112	0.02%	0.003%
65	8.629	2256	2267	2297	rBV3	99940	194331	40.40%	5.467%
66	8.912	2352	2355	2359	rBV2	194	170	0.04%	0.005%
67	9.089	2408	2410	2412	rVB	147	57	0.01%	0.002%
68	9.160	2430	2432	2436	rVB	224	120	0.02%	0.003%
69	9.208	2444	2447	2448	rBV	225	143	0.03%	0.004%
70	9.343	2485	2489	2494	rBV2	209	209	0.04%	0.006%
71	9.414	2499	2511	2538	rBV	196394	329943	68.59%	9.282%
72	9.687	2594	2596	2598	rBV	213	144	0.03%	0.004%
73	9.825	2637	2639	2640	rBV	293	138	0.03%	0.004%
74	10.037	2701	2705	2707	rBV	152	156	0.03%	0.004%
75	10.115	2724	2729	2736	rBV2	1169	1430	0.30%	0.040%
76	10.205	2755	2757	2759	rBV	119	70	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053301.D
 Acq On : 20 Mar 2023 12:40
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.240	2766	2768	2774	rVB	186	135	0.03%	0.004%
78	10.356	2801	2804	2806	rBV	175	139	0.03%	0.004%
79	10.378	2807	2811	2813	rVV	138	131	0.03%	0.004%
80	10.578	2871	2873	2876	rVB	321	183	0.04%	0.005%
81	10.600	2877	2880	2885	rBV	212	254	0.05%	0.007%
82	10.751	2915	2927	2945	rBV	141039	228202	47.44%	6.420%
83	10.854	2955	2959	2961	rBV	194	187	0.04%	0.005%
84	10.922	2978	2980	2981	rBV	134	51	0.01%	0.001%
85	10.973	2993	2996	3000	rBV2	180	181	0.04%	0.005%
86	11.086	3028	3031	3037	rVB	317	269	0.06%	0.008%
87	11.420	3133	3135	3139	rVB	198	98	0.02%	0.003%
88	11.446	3139	3143	3148	rBV2	234	188	0.04%	0.005%
89	11.722	3227	3229	3232	rBV	154	93	0.02%	0.003%
90	11.806	3244	3255	3270	rBV	200191	317801	66.06%	8.941%
91	11.935	3293	3295	3300	rVB	186	93	0.02%	0.003%
92	12.189	3362	3374	3396	rBV	198019	321202	66.77%	9.036%
93	12.478	3462	3464	3465	rBV	150	48	0.01%	0.001%
94	12.504	3471	3472	3475	rBV	122	67	0.01%	0.002%
95	12.587	3495	3498	3500	rBV	204	153	0.03%	0.004%
96	12.648	3515	3517	3521	rBV	148	105	0.02%	0.003%
97	14.362	4045	4050	4052	rBV	268	255	0.05%	0.007%
98	14.761	4172	4174	4177	rVB2	300	139	0.03%	0.004%
99	15.143	4290	4293	4297	rBV	266	185	0.04%	0.005%
100	15.732	4473	4476	4480	rBV2	347	327	0.07%	0.009%




Sum of corrected areas: 3554586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053301.D
Acq On : 20 Mar 2023 12:40
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

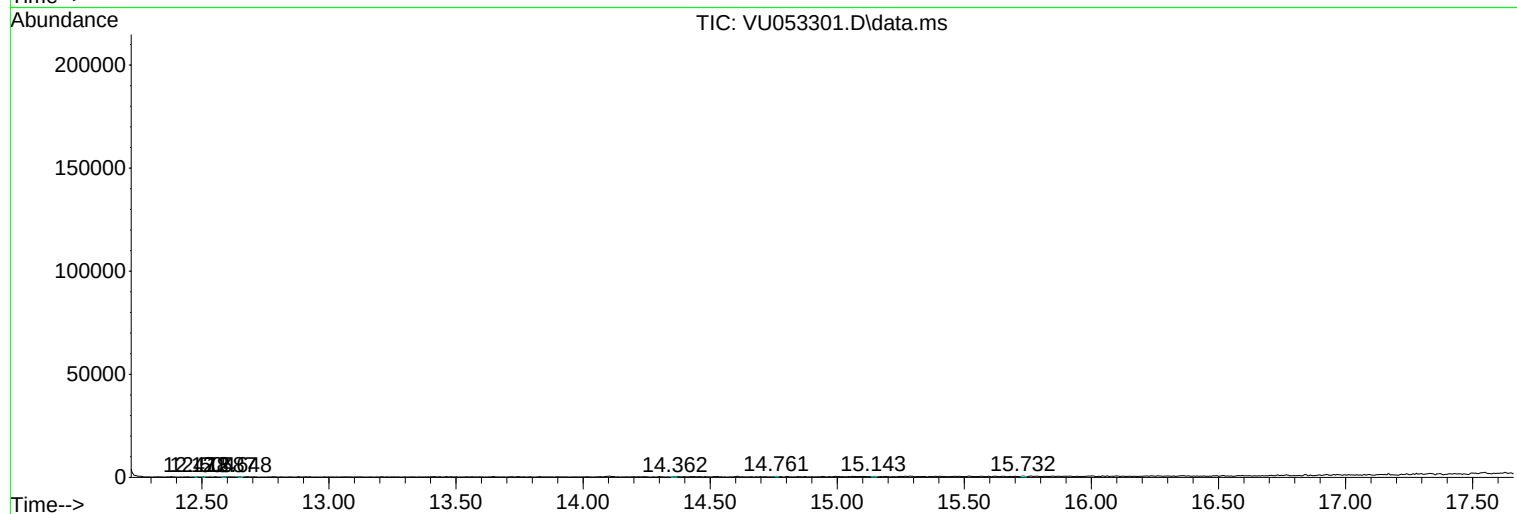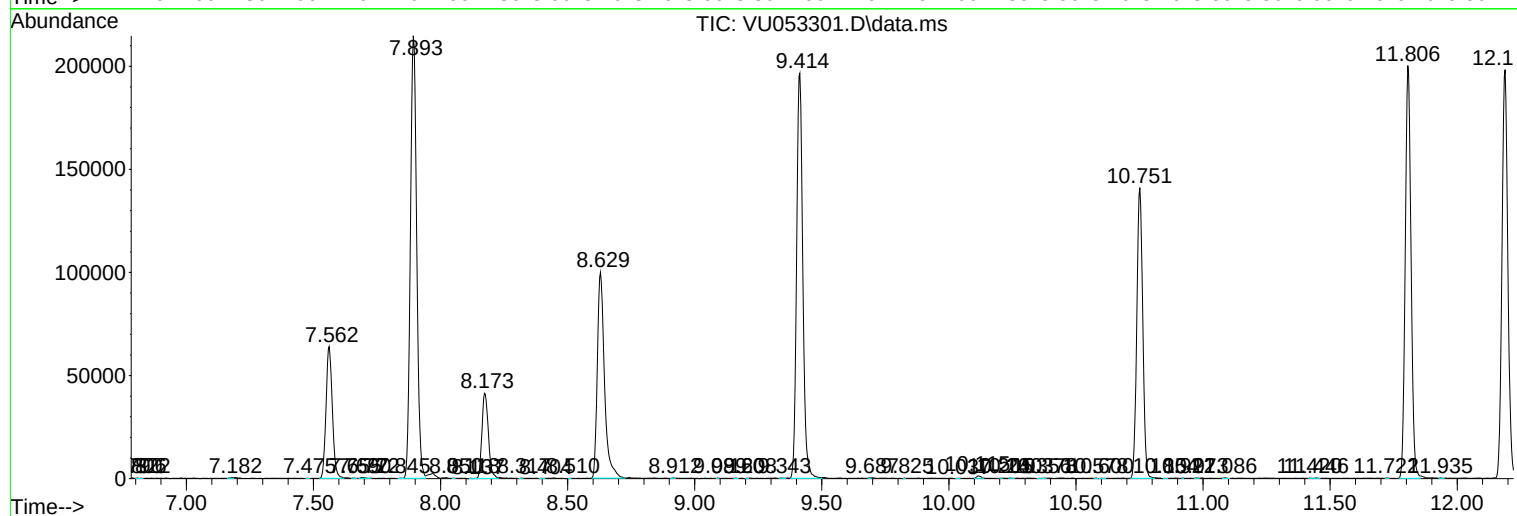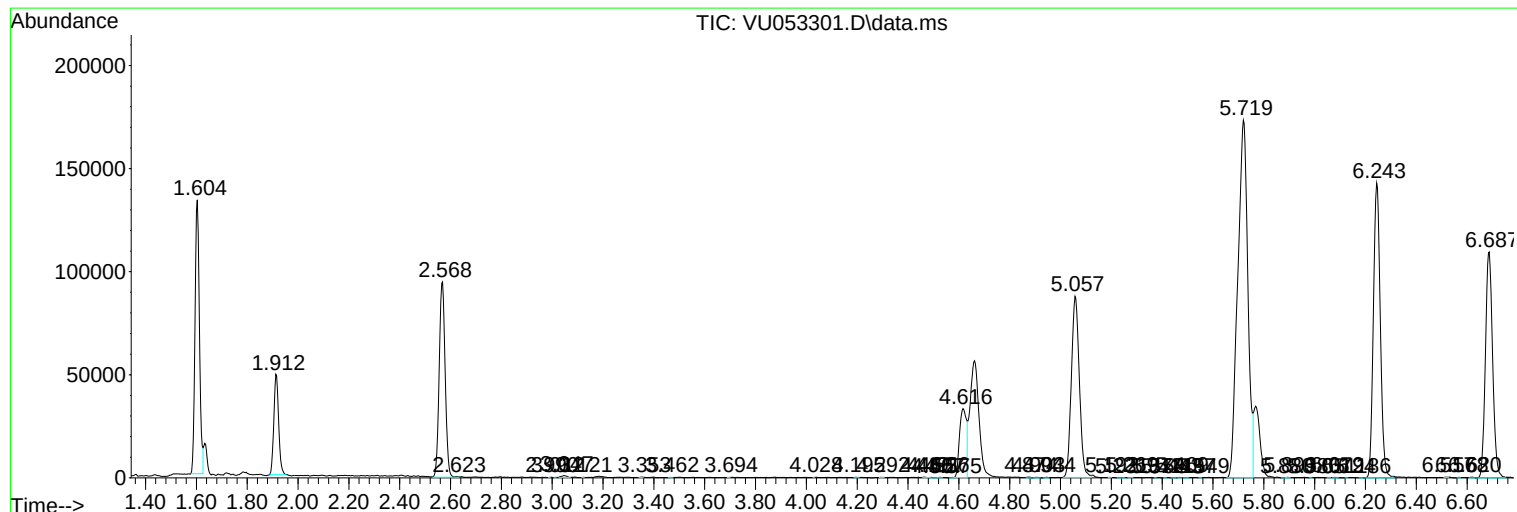

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053301.D
Acq On : 20 Mar 2023 12:40
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053301.D
Acq On : 20 Mar 2023 12:40
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------