

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053307.D
 Acq On : 20 Mar 2023 15:02
 Operator : JC/MD
 Sample : 01961-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	87	rBV	57626	66900	14.27%	2.105%
2	1.912	171	178	192	rVB	48641	64428	13.74%	2.028%
3	2.565	370	381	397	rBV	91832	146340	31.21%	4.605%
4	3.674	720	726	728	rBV	180	229	0.05%	0.007%
5	3.864	776	785	797	rVB2	551	1117	0.24%	0.035%
6	3.983	819	822	825	rBV	224	142	0.03%	0.004%
7	4.224	894	897	900	rVB	220	129	0.03%	0.004%
8	4.317	923	926	930	rBV	159	145	0.03%	0.005%
9	4.388	945	948	950	rBV	178	105	0.02%	0.003%
10	4.507	983	985	988	rVB2	233	117	0.02%	0.004%
11	4.526	988	991	993	rBV	173	146	0.03%	0.005%
12	4.616	1007	1019	1043	rBV	32372	80429	17.16%	2.531%
13	5.057	1141	1156	1172	rBV	86812	188843	40.28%	5.943%
14	5.192	1195	1198	1200	rBV	167	134	0.03%	0.004%
15	5.221	1206	1207	1210	rVB	232	106	0.02%	0.003%
16	5.259	1215	1219	1220	rBV	160	138	0.03%	0.004%
17	5.465	1279	1283	1285	rBV	294	251	0.05%	0.008%
18	5.581	1316	1319	1321	rBV	138	121	0.03%	0.004%
19	5.719	1342	1362	1371	rBV2	170177	468829	100.00%	14.755%
20	5.912	1418	1422	1424	rBV	253	168	0.04%	0.005%
21	6.044	1457	1463	1467	rBV	229	326	0.07%	0.010%
22	6.179	1503	1505	1508	rBV	189	148	0.03%	0.005%
23	6.243	1512	1525	1548	rVV2	95689	181251	38.66%	5.704%
24	6.391	1564	1571	1574	rBV	210	305	0.07%	0.010%
25	6.587	1628	1632	1633	rBV	142	125	0.03%	0.004%
26	6.619	1640	1642	1644	rBV	147	102	0.02%	0.003%
27	6.632	1644	1646	1649	rVV	285	184	0.04%	0.006%
28	6.684	1649	1662	1684	rVB	109293	210907	44.99%	6.637%
29	6.809	1698	1701	1706	rVB	348	295	0.06%	0.009%
30	6.835	1707	1709	1713	rBB	151	126	0.03%	0.004%
31	6.861	1713	1717	1720	rBV	162	193	0.04%	0.006%
32	6.906	1725	1731	1734	rBV	198	294	0.06%	0.009%
33	6.989	1754	1757	1759	rBB	160	112	0.02%	0.004%
34	7.044	1771	1774	1779	rBB	274	253	0.05%	0.008%
35	7.079	1780	1785	1787	rBV	171	204	0.04%	0.006%
36	7.124	1792	1799	1805	rBB	217	360	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053307.D
 Acq On : 20 Mar 2023 15:02
 Operator : JC/MD
 Sample : 01961-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.153	1806	1808	1811	rBV	135	117	0.02%	0.004%
38	7.185	1811	1818	1822	rBV4	870	954	0.20%	0.030%
39	7.256	1837	1840	1843	rBB	213	158	0.03%	0.005%
40	7.414	1887	1889	1891	rBV	178	120	0.03%	0.004%
41	7.558	1924	1934	1952	rBV	60312	107818	23.00%	3.393%
42	7.648	1959	1962	1965	rBV	259	156	0.03%	0.005%
43	7.684	1971	1973	1974	rBV	204	106	0.02%	0.003%
44	7.735	1986	1989	1991	rBV	156	135	0.03%	0.004%
45	7.751	1992	1994	1997	rVB	200	106	0.02%	0.003%
46	7.835	2015	2020	2022	rBV	210	236	0.05%	0.007%
47	7.893	2025	2038	2053	rBV	210939	362141	77.24%	11.397%
48	8.176	2115	2126	2145	rVV	41552	70787	15.10%	2.228%
49	8.246	2145	2148	2150	rVV	294	184	0.04%	0.006%
50	8.288	2158	2161	2163	rVB2	181	107	0.02%	0.003%
51	8.381	2187	2190	2195	rVB	216	109	0.02%	0.003%
52	8.433	2202	2206	2209	rBV	214	209	0.04%	0.007%
53	8.629	2256	2267	2293	rBV2	102010	194516	41.49%	6.122%
54	8.822	2324	2327	2330	rBV2	143	111	0.02%	0.003%
55	8.992	2377	2380	2382	rBV	177	148	0.03%	0.005%
56	9.005	2382	2384	2388	rVB	202	120	0.03%	0.004%
57	9.118	2417	2419	2423	rVB	216	102	0.02%	0.003%
58	9.269	2463	2466	2467	rBV	160	108	0.02%	0.003%
59	9.414	2499	2511	2533	rBV	136687	238550	50.88%	7.507%
60	9.568	2553	2559	2567	rBV2	571	876	0.19%	0.028%
61	9.758	2615	2618	2622	rBV2	290	298	0.06%	0.009%
62	9.832	2636	2641	2645	rBV	195	248	0.05%	0.008%
63	9.922	2664	2669	2671	rBV	216	216	0.05%	0.007%
64	9.934	2671	2673	2674	rVV	211	105	0.02%	0.003%
65	9.944	2674	2676	2683	rVB2	468	412	0.09%	0.013%
66	10.005	2691	2695	2697	rBV	310	233	0.05%	0.007%
67	10.044	2704	2707	2712	rBB	131	136	0.03%	0.004%
68	10.115	2720	2729	2741	rVV2	5653	8448	1.80%	0.266%
69	10.240	2765	2768	2774	rBV	178	269	0.06%	0.008%
70	10.619	2883	2886	2889	rBV2	195	118	0.03%	0.004%
71	10.696	2906	2910	2913	rVB2	169	129	0.03%	0.004%
72	10.751	2914	2927	2943	rBV	147178	231835	49.45%	7.296%
73	10.934	2981	2984	2986	rBV2	174	107	0.02%	0.003%
74	11.118	3039	3041	3046	rBV	164	111	0.02%	0.003%
75	11.169	3052	3057	3061	rBV	238	315	0.07%	0.010%
76	11.266	3082	3087	3090	rBV	233	278	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053307.D
 Acq On : 20 Mar 2023 15:02
 Operator : JC/MD
 Sample : 01961-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.372	3118	3120	3122	rBV	153	98	0.02%	0.003%
78	11.590	3184	3188	3191	rBV2	223	168	0.04%	0.005%
79	11.648	3204	3206	3209	rBV	147	122	0.03%	0.004%
80	11.806	3244	3255	3276	rBV	137185	220750	47.09%	6.947%
81	12.085	3339	3342	3345	rBV	225	226	0.05%	0.007%
82	12.188	3361	3374	3397	rBV2	196057	316641	67.54%	9.965%
83	12.314	3409	3413	3416	rBV3	308	266	0.06%	0.008%
84	12.635	3510	3513	3515	rBV	152	128	0.03%	0.004%
85	12.764	3549	3553	3558	rVB2	359	433	0.09%	0.014%
86	12.860	3580	3583	3587	rVB2	294	196	0.04%	0.006%
87	12.886	3588	3591	3594	rBV	246	170	0.04%	0.005%
88	12.973	3615	3618	3623	rVB2	183	132	0.03%	0.004%
89	13.044	3637	3640	3643	rBV	222	143	0.03%	0.005%
90	13.092	3652	3655	3659	rBV	217	162	0.03%	0.005%
91	13.111	3659	3661	3664	rVB2	247	137	0.03%	0.004%
92	13.233	3695	3699	3702	rBV2	259	180	0.04%	0.006%
93	13.825	3881	3883	3890	rBV	179	125	0.03%	0.004%
94	14.095	3963	3967	3969	rBV3	439	344	0.07%	0.011%
95	14.867	4204	4207	4210	rVB2	320	265	0.06%	0.008%
96	14.976	4239	4241	4245	rBV2	285	180	0.04%	0.006%
97	15.236	4315	4322	4327	rBV3	510	605	0.13%	0.019%
98	15.256	4327	4328	4333	rVB2	235	152	0.03%	0.005%
99	15.349	4354	4357	4359	rBV2	407	303	0.06%	0.010%
100	15.561	4420	4423	4427	rBV	492	362	0.08%	0.011%




Sum of corrected areas: 3177522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053307.D
Acq On : 20 Mar 2023 15:02
Operator : JC/MD
Sample : 01961-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

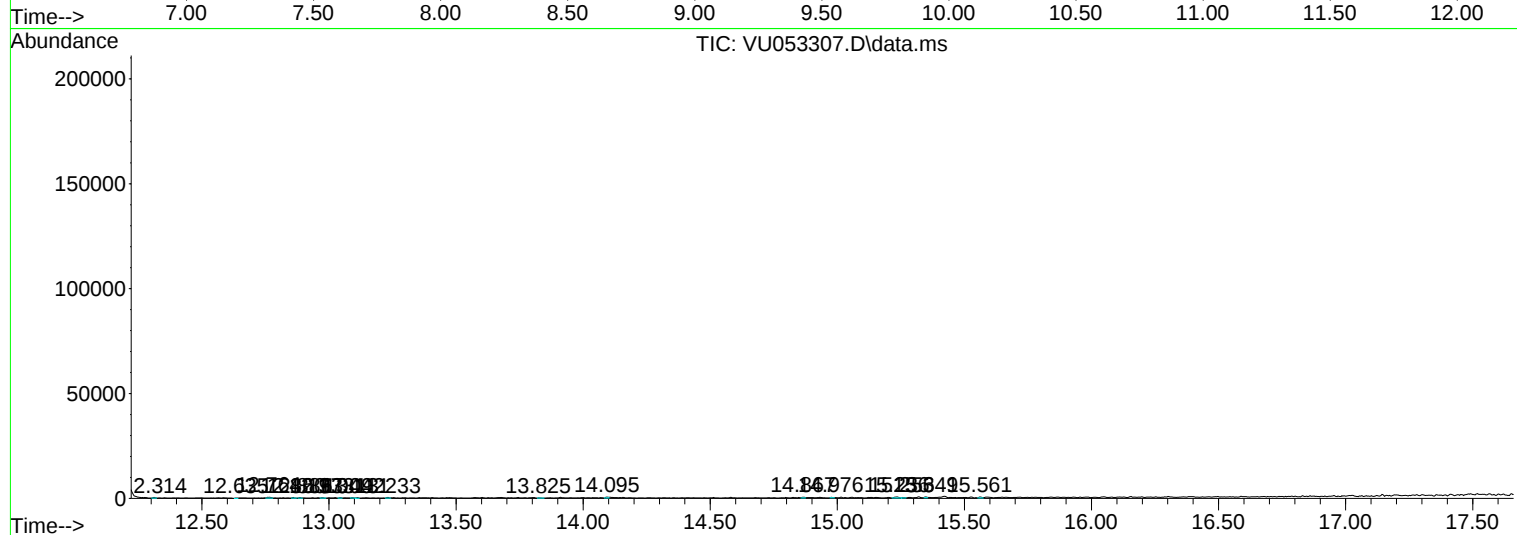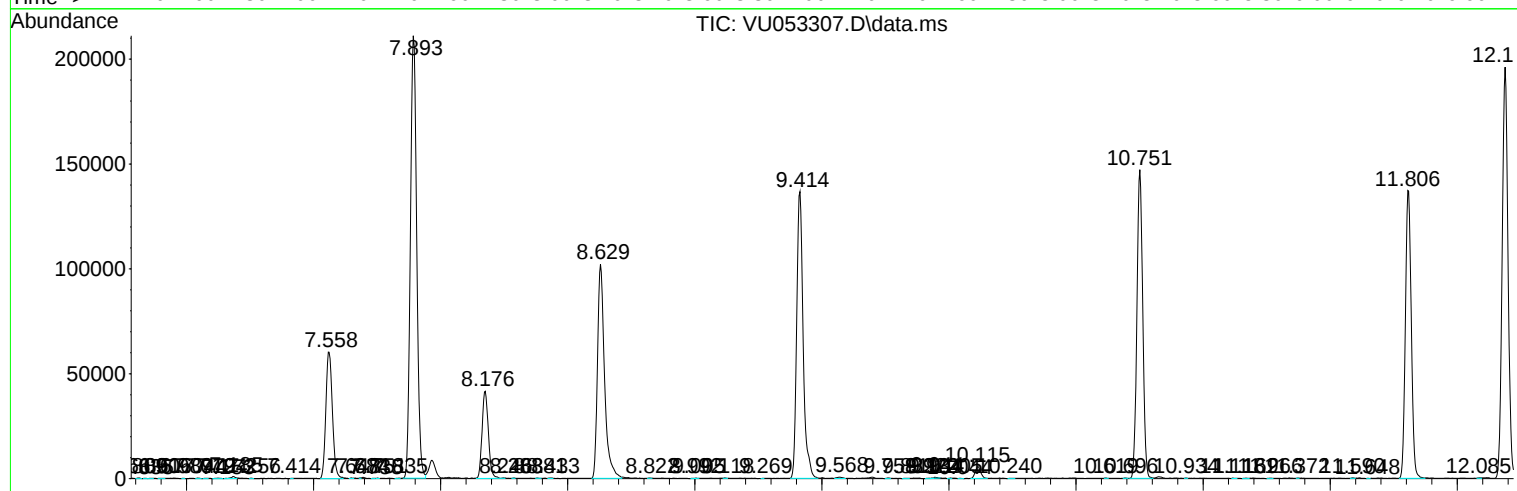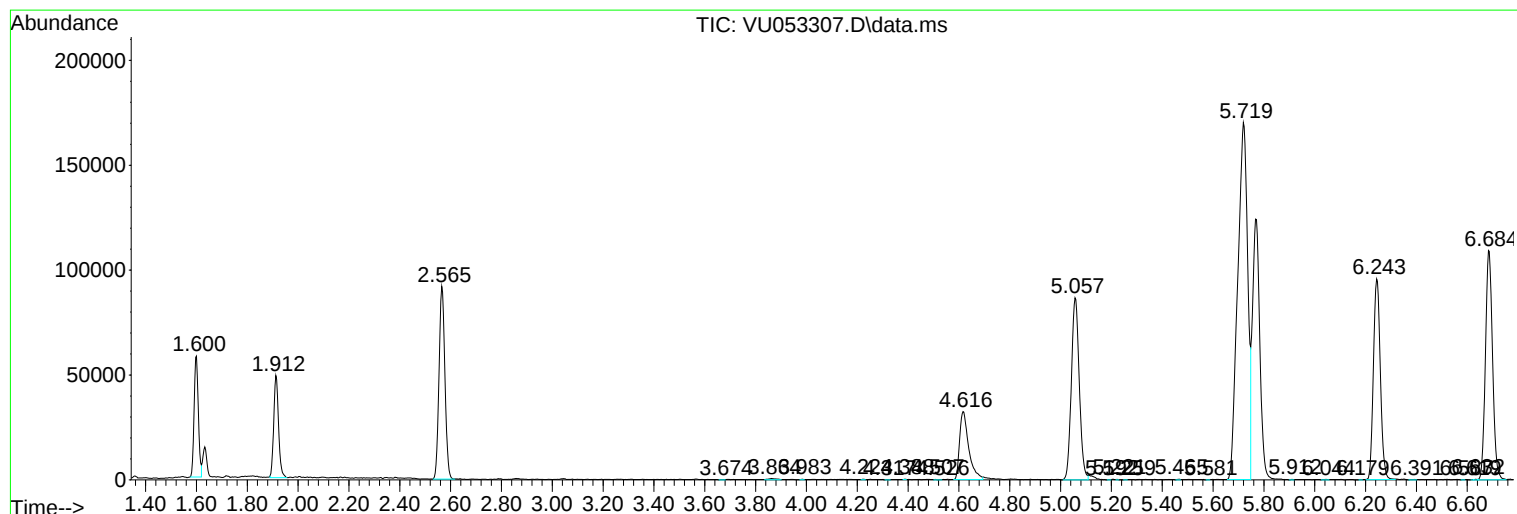

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053307.D
Acq On : 20 Mar 2023 15:02
Operator : JC/MD
Sample : 01961-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053307.D
Acq On : 20 Mar 2023 15:02
Operator : JC/MD
Sample : 01961-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------