

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053308.D
 Acq On : 20 Mar 2023 15:52
 Operator : JC/MD
 Sample : VIBLK116
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	88	rBV	67463	76755	16.93%	2.190%
2	1.912	170	178	194	rVB	54129	72830	16.06%	2.078%
3	2.565	370	381	396	rVB	102164	163149	35.98%	4.656%
4	2.854	469	471	473	rVB	363	140	0.03%	0.004%
5	3.041	519	529	544	rBV3	3885	7633	1.68%	0.218%
6	3.353	623	626	629	rVB2	236	174	0.04%	0.005%
7	3.594	699	701	707	rVB	176	111	0.02%	0.003%
8	3.861	782	784	789	rVB	322	242	0.05%	0.007%
9	3.890	790	793	795	rBV	177	156	0.03%	0.004%
10	4.063	841	847	849	rBV	274	260	0.06%	0.007%
11	4.176	879	882	884	rBV	202	114	0.03%	0.003%
12	4.292	916	918	922	rBB	168	138	0.03%	0.004%
13	4.321	923	927	929	rBV	144	153	0.03%	0.004%
14	4.481	974	977	979	rBV	209	136	0.03%	0.004%
15	4.514	984	987	992	rVB	258	130	0.03%	0.004%
16	4.620	1008	1020	1053	rBV	32621	80136	17.67%	2.287%
17	4.764	1063	1065	1068	rVB2	363	150	0.03%	0.004%
18	4.896	1103	1106	1110	rVB	203	108	0.02%	0.003%
19	5.057	1141	1156	1175	rBV2	83165	184356	40.66%	5.261%
20	5.205	1200	1202	1206	rVB2	237	153	0.03%	0.004%
21	5.231	1207	1210	1216	rBV	175	253	0.06%	0.007%
22	5.295	1223	1230	1232	rBV	206	271	0.06%	0.008%
23	5.317	1233	1237	1241	rVV2	251	205	0.05%	0.006%
24	5.343	1241	1245	1248	rVV2	176	126	0.03%	0.004%
25	5.542	1303	1307	1311	rVB2	326	302	0.07%	0.009%
26	5.571	1312	1316	1318	rBV	279	210	0.05%	0.006%
27	5.626	1328	1333	1336	rBV	158	215	0.05%	0.006%
28	5.719	1342	1362	1371	rBV2	167574	453437	100.00%	12.940%
29	5.915	1420	1423	1424	rBV	248	127	0.03%	0.004%
30	6.134	1488	1491	1494	rBV	174	177	0.04%	0.005%
31	6.243	1512	1525	1550	rVV	146483	273935	60.41%	7.818%
32	6.330	1550	1552	1554	rBV2	231	106	0.02%	0.003%
33	6.481	1597	1599	1600	rBV2	261	145	0.03%	0.004%
34	6.687	1650	1663	1681	rBV2	104762	202152	44.58%	5.769%
35	6.848	1710	1713	1717	rBB	198	181	0.04%	0.005%
36	6.903	1728	1730	1732	rBV	199	141	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053308.D
 Acq On : 20 Mar 2023 15:52
 Operator : JC/MD
 Sample : VIBLK116
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.960	1745	1748	1751	rBB2	289	232	0.05%	0.007%
38	6.996	1754	1759	1762	rBV	180	236	0.05%	0.007%
39	7.028	1767	1769	1772	rBV	123	110	0.02%	0.003%
40	7.054	1773	1777	1781	rVV2	218	207	0.05%	0.006%
41	7.124	1793	1799	1801	rBV	274	214	0.05%	0.006%
42	7.221	1824	1829	1835	rBB	274	400	0.09%	0.011%
43	7.253	1835	1839	1842	rBV	166	197	0.04%	0.006%
44	7.372	1873	1876	1881	rBV	123	114	0.03%	0.003%
45	7.465	1902	1905	1908	rBB	178	117	0.03%	0.003%
46	7.494	1909	1914	1920	rBB2	284	354	0.08%	0.010%
47	7.562	1921	1935	1951	rBV	62134	109049	24.05%	3.112%
48	7.710	1980	1981	1984	rBV	230	114	0.03%	0.003%
49	7.726	1984	1986	1989	rVV	234	147	0.03%	0.004%
50	7.745	1989	1992	1995	rVB	229	143	0.03%	0.004%
51	7.893	2021	2038	2053	rBV	217336	372975	82.26%	10.644%
52	8.057	2087	2089	2095	rVB	279	248	0.05%	0.007%
53	8.176	2114	2126	2142	rBV2	42805	73880	16.29%	2.108%
54	8.311	2165	2168	2173	rBB	179	202	0.04%	0.006%
55	8.340	2174	2177	2179	rBV	144	124	0.03%	0.004%
56	8.375	2185	2188	2189	rBV	261	130	0.03%	0.004%
57	8.542	2238	2240	2244	rBV	231	198	0.04%	0.006%
58	8.629	2256	2267	2294	rBV3	90789	173641	38.29%	4.955%
59	8.755	2303	2306	2309	rVB	330	233	0.05%	0.007%
60	8.806	2317	2322	2332	rVB2	253	359	0.08%	0.010%
61	8.983	2375	2377	2380	rBV	145	122	0.03%	0.003%
62	9.131	2414	2423	2424	rBV	183	284	0.06%	0.008%
63	9.189	2438	2441	2445	rBV	193	222	0.05%	0.006%
64	9.250	2456	2460	2464	rBV	169	194	0.04%	0.006%
65	9.311	2476	2479	2483	rBV2	317	290	0.06%	0.008%
66	9.414	2498	2511	2533	rBV	205705	354130	78.10%	10.106%
67	9.571	2552	2560	2567	rVB2	687	960	0.21%	0.027%
68	9.697	2595	2599	2607	rVB2	565	636	0.14%	0.018%
69	9.951	2670	2678	2684	rBV	1064	1368	0.30%	0.039%
70	10.115	2721	2729	2741	rBV3	6320	9976	2.20%	0.285%
71	10.308	2786	2789	2792	rBV	224	201	0.04%	0.006%
72	10.751	2915	2927	2945	rBV	138787	218376	48.16%	6.232%
73	10.822	2945	2949	2957	rVV4	979	1311	0.29%	0.037%
74	10.861	2958	2961	2964	rVB	236	118	0.03%	0.003%
75	10.928	2979	2982	2986	rVB	246	165	0.04%	0.005%
76	11.037	3009	3016	3021	rBB	163	308	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053308.D
 Acq On : 20 Mar 2023 15:52
 Operator : JC/MD
 Sample : VIBLK116
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.073	3021	3027	3032	rBV	221	326	0.07%	0.009%
78	11.214	3068	3071	3076	rBV	222	283	0.06%	0.008%
79	11.619	3194	3197	3198	rBV	174	115	0.03%	0.003%
80	11.674	3211	3214	3216	rBV	215	181	0.04%	0.005%
81	11.684	3216	3217	3222	rVB	202	115	0.03%	0.003%
82	11.809	3244	3256	3275	rBV	214417	338393	74.63%	9.657%
83	11.922	3288	3291	3295	rVB	213	133	0.03%	0.004%
84	12.188	3362	3374	3400	rVB	196249	320109	70.60%	9.135%
85	12.288	3401	3405	3407	rBV	352	192	0.04%	0.005%
86	12.311	3407	3412	3418	rBV2	464	592	0.13%	0.017%
87	12.449	3452	3455	3461	rVB2	212	211	0.05%	0.006%
88	12.909	3595	3598	3601	rVB	280	151	0.03%	0.004%
89	13.082	3648	3652	3655	rBV	198	169	0.04%	0.005%
90	13.160	3672	3676	3680	rBV2	241	247	0.05%	0.007%
91	14.240	4009	4012	4016	rVB	290	181	0.04%	0.005%
92	14.729	4161	4164	4168	rBV	232	136	0.03%	0.004%
93	14.860	4203	4205	4207	rBV	285	115	0.03%	0.003%
94	14.883	4210	4212	4215	rBV	272	174	0.04%	0.005%
95	15.076	4268	4272	4276	rBV2	326	265	0.06%	0.008%
96	15.105	4279	4281	4283	rBV	283	136	0.03%	0.004%
97	15.137	4289	4291	4295	rBV	216	135	0.03%	0.004%
98	15.320	4345	4348	4351	rBV	202	113	0.02%	0.003%
99	15.343	4351	4355	4358	rVV2	244	211	0.05%	0.006%
100	15.455	4387	4390	4393	rBV2	211	143	0.03%	0.004%




Sum of corrected areas: 3504118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053308.D
Acq On : 20 Mar 2023 15:52
Operator : JC/MD
Sample : VIBLK116
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

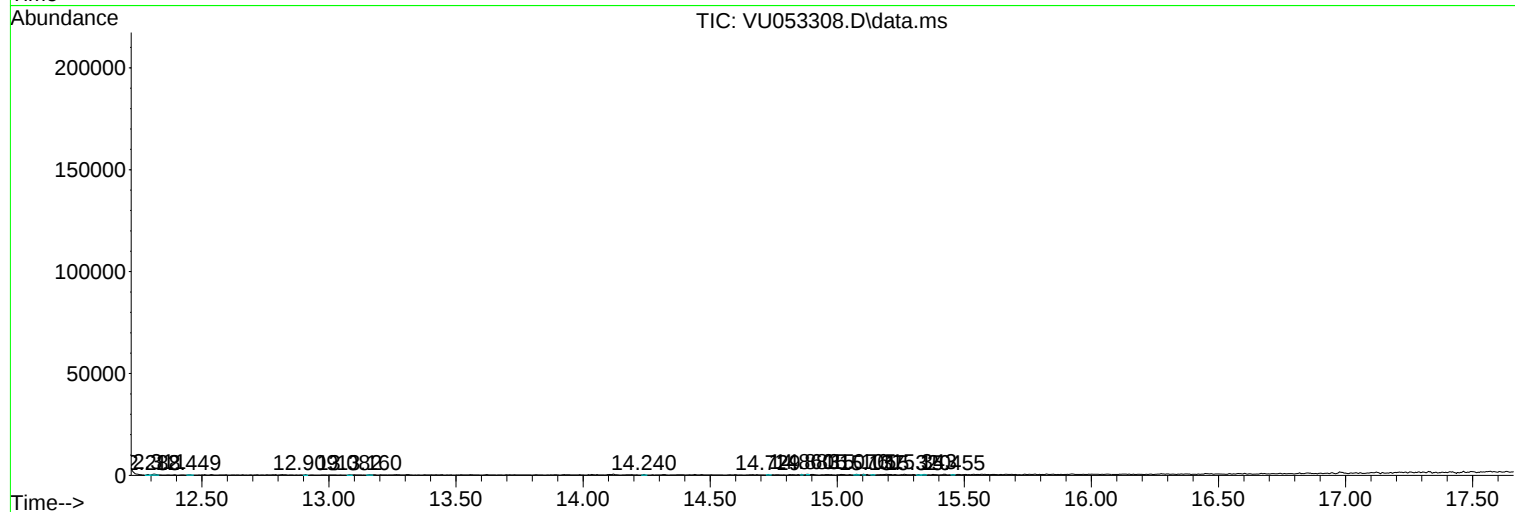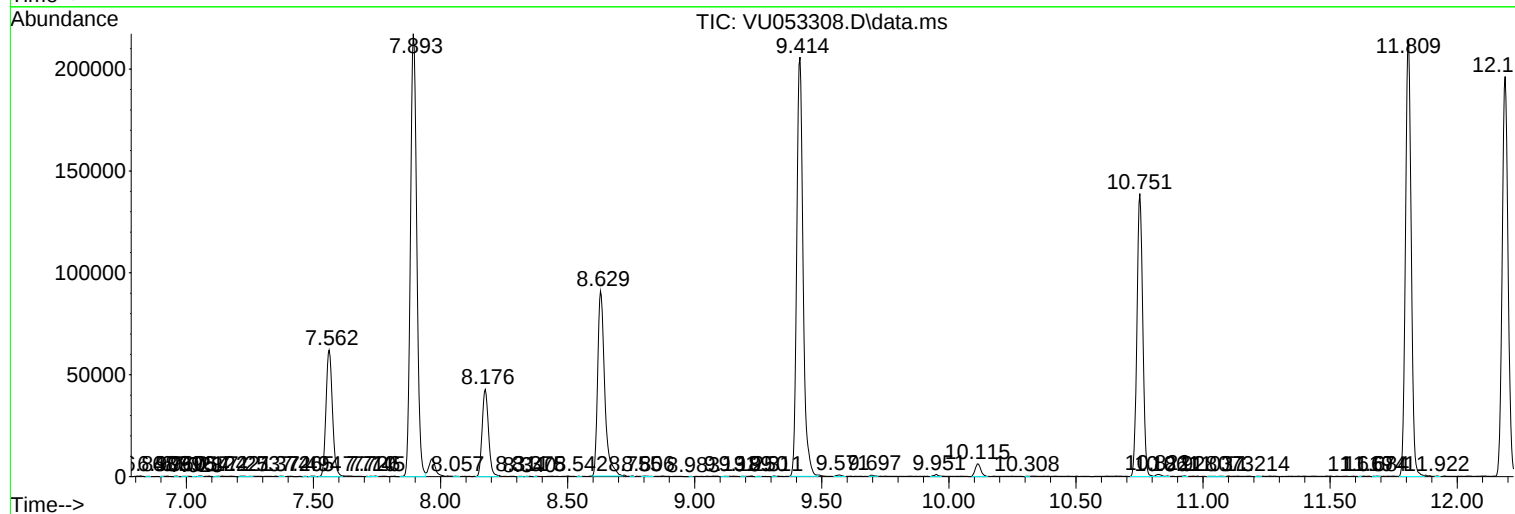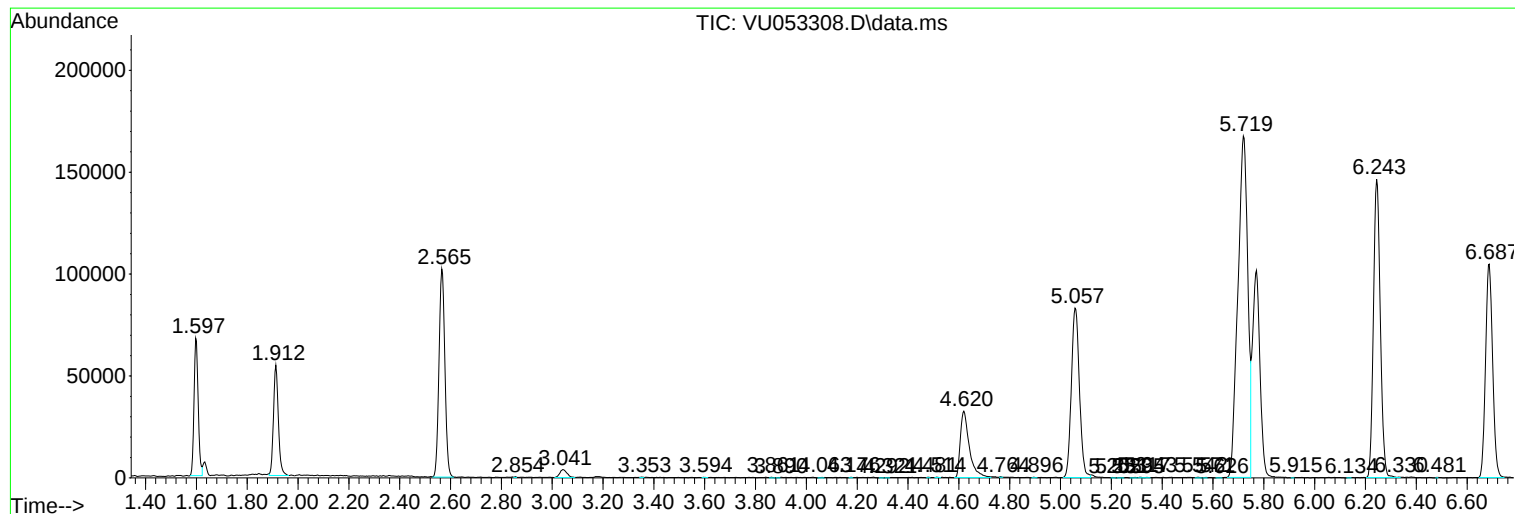

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053308.D
Acq On : 20 Mar 2023 15:52
Operator : JC/MD
Sample : VIBLK116
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053308.D
Acq On : 20 Mar 2023 15:52
Operator : JC/MD
Sample : VIBLK116
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------