

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053309.D
 Acq On : 20 Mar 2023 16:21
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	89	rBV2	78444	93057	17.52%	2.437%
2	1.912	171	178	194	rVB	52266	70180	13.21%	1.838%
3	2.565	370	381	395	rBV	89784	145126	27.32%	3.800%
4	2.797	449	453	456	rBV2	473	352	0.07%	0.009%
5	3.041	525	529	530	rBV2	442	243	0.05%	0.006%
6	3.356	620	627	633	rVB3	1018	1603	0.30%	0.042%
7	3.954	808	813	814	rBV	167	167	0.03%	0.004%
8	4.256	901	907	908	rBV	210	245	0.05%	0.006%
9	4.395	948	950	951	rBV	262	110	0.02%	0.003%
10	4.465	966	972	975	rBV	251	343	0.06%	0.009%
11	4.568	1001	1004	1006	rBV	176	136	0.03%	0.004%
12	4.620	1008	1020	1027	rBV	40285	90012	16.94%	2.357%
13	4.893	1103	1105	1108	rVB	261	141	0.03%	0.004%
14	4.928	1109	1116	1118	rBV	185	235	0.04%	0.006%
15	4.996	1135	1137	1140	rBV2	167	109	0.02%	0.003%
16	5.060	1141	1157	1173	rBV	97977	214666	40.40%	5.621%
17	5.260	1215	1219	1220	rBV	180	151	0.03%	0.004%
18	5.414	1262	1267	1269	rBB	178	171	0.03%	0.004%
19	5.607	1320	1327	1331	rBV	198	328	0.06%	0.009%
20	5.629	1331	1334	1337	rVB2	309	224	0.04%	0.006%
21	5.652	1338	1341	1342	rBV	165	111	0.02%	0.003%
22	5.719	1342	1362	1372	rBV2	188322	531289	100.00%	13.911%
23	5.944	1428	1432	1434	rBV	327	267	0.05%	0.007%
24	5.977	1439	1442	1444	rBB	165	111	0.02%	0.003%
25	6.012	1449	1453	1455	rBV	130	133	0.03%	0.003%
26	6.076	1466	1473	1476	rBB	161	234	0.04%	0.006%
27	6.102	1477	1481	1485	rBB	257	251	0.05%	0.007%
28	6.134	1485	1491	1493	rBV	182	231	0.04%	0.006%
29	6.243	1512	1525	1544	rBV	125632	237424	44.69%	6.217%
30	6.343	1553	1556	1558	rBV	241	164	0.03%	0.004%
31	6.388	1567	1570	1575	rBV3	356	287	0.05%	0.008%
32	6.411	1575	1577	1580	rVB	300	158	0.03%	0.004%
33	6.475	1595	1597	1600	rBV	125	114	0.02%	0.003%
34	6.543	1609	1618	1626	rVB5	1587	2514	0.47%	0.066%
35	6.633	1644	1646	1649	rBV	250	165	0.03%	0.004%
36	6.687	1649	1663	1685	rVB	125852	242754	45.69%	6.356%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053309.D
 Acq On : 20 Mar 2023 16:21
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.851	1711	1714	1716	rBV	161	127	0.02%	0.003%
38	6.893	1722	1727	1729	rBV	181	206	0.04%	0.005%
39	7.044	1771	1774	1776	rBV	144	124	0.02%	0.003%
40	7.182	1811	1817	1821	rBV3	867	1161	0.22%	0.030%
41	7.279	1845	1847	1853	rBV	165	197	0.04%	0.005%
42	7.562	1924	1935	1952	rBV	71602	124045	23.35%	3.248%
43	7.687	1969	1974	1977	rBV3	644	567	0.11%	0.015%
44	7.745	1990	1992	1994	rBV3	308	181	0.03%	0.005%
45	7.809	2007	2012	2014	rBV2	294	261	0.05%	0.007%
46	7.896	2023	2039	2054	rBV	241126	417700	78.62%	10.937%
47	7.967	2055	2061	2074	rVB2	9508	15316	2.88%	0.401%
48	8.121	2106	2109	2111	rBV	139	118	0.02%	0.003%
49	8.176	2115	2126	2145	rVV	50508	83061	15.63%	2.175%
50	8.378	2187	2189	2192	rBV	153	119	0.02%	0.003%
51	8.485	2219	2222	2226	rBV	145	167	0.03%	0.004%
52	8.533	2233	2237	2240	rBV2	192	126	0.02%	0.003%
53	8.549	2240	2242	2245	rVB	249	124	0.02%	0.003%
54	8.568	2245	2248	2250	rBV	301	210	0.04%	0.005%
55	8.629	2256	2267	2293	rBV2	121548	236836	44.58%	6.201%
56	9.047	2393	2397	2401	rBV	156	202	0.04%	0.005%
57	9.102	2410	2414	2419	rBV	249	313	0.06%	0.008%
58	9.147	2426	2428	2430	rBV	173	118	0.02%	0.003%
59	9.185	2439	2440	2444	rBV	242	142	0.03%	0.004%
60	9.414	2499	2511	2531	rBV	179016	314699	59.23%	8.240%
61	9.652	2580	2585	2589	rBB	221	236	0.04%	0.006%
62	9.697	2590	2599	2605	rBV3	966	1236	0.23%	0.032%
63	9.947	2671	2677	2684	rVV2	616	848	0.16%	0.022%
64	10.021	2697	2700	2703	rBV	124	131	0.02%	0.003%
65	10.115	2719	2729	2739	rBV3	7159	11666	2.20%	0.305%
66	10.198	2752	2755	2758	rBV2	200	142	0.03%	0.004%
67	10.253	2769	2772	2775	rBB	151	124	0.02%	0.003%
68	10.288	2780	2783	2784	rBV	188	127	0.02%	0.003%
69	10.330	2789	2796	2799	rBV2	253	302	0.06%	0.008%
70	10.420	2820	2824	2826	rBV	203	192	0.04%	0.005%
71	10.462	2835	2837	2842	rVB	195	152	0.03%	0.004%
72	10.751	2914	2927	2947	rBV	174960	281921	53.06%	7.382%
73	10.825	2947	2950	2957	rVB3	1241	1227	0.23%	0.032%
74	11.111	3035	3039	3043	rBB	297	230	0.04%	0.006%
75	11.185	3060	3062	3064	rBV2	273	165	0.03%	0.004%
76	11.279	3089	3091	3093	rBV	166	114	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053309.D
 Acq On : 20 Mar 2023 16:21
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3150	rBV	296	407	0.08%	0.011%
78	11.533	3164	3170	3172	rBV	221	273	0.05%	0.007%
79	11.652	3204	3207	3208	rBV	169	113	0.02%	0.003%
80	11.809	3243	3256	3278	rBV	188641	299082	56.29%	7.831%
81	11.918	3289	3290	3294	rBB	208	118	0.02%	0.003%
82	11.941	3294	3297	3300	rBV	181	182	0.03%	0.005%
83	12.086	3339	3342	3345	rBV2	346	280	0.05%	0.007%
84	12.124	3352	3354	3357	rVB2	191	110	0.02%	0.003%
85	12.189	3361	3374	3390	rBV	236870	385370	72.53%	10.091%
86	12.311	3407	3412	3420	rVB2	793	1071	0.20%	0.028%
87	12.369	3424	3430	3432	rBV	420	428	0.08%	0.011%
88	12.404	3436	3441	3444	rBV	343	355	0.07%	0.009%
89	12.488	3463	3467	3470	rBV2	222	189	0.04%	0.005%
90	13.156	3672	3675	3678	rBV	174	130	0.02%	0.003%
91	13.198	3685	3688	3690	rBV2	202	119	0.02%	0.003%
92	13.304	3718	3721	3724	rBV2	204	129	0.02%	0.003%
93	13.664	3830	3833	3837	rVB	191	165	0.03%	0.004%
94	14.102	3967	3969	3971	rBV	315	166	0.03%	0.004%
95	14.603	4119	4125	4130	rBV	291	306	0.06%	0.008%
96	15.063	4264	4268	4269	rBV	280	139	0.03%	0.004%
97	15.259	4326	4329	4334	rVB2	416	303	0.06%	0.008%
98	15.343	4352	4355	4360	rVB2	444	382	0.07%	0.010%
99	15.372	4360	4364	4369	rBV3	411	388	0.07%	0.010%
100	15.542	4414	4417	4419	rBV	282	128	0.02%	0.003%




Sum of corrected areas: 3819072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053309.D
Acq On : 20 Mar 2023 16:21
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

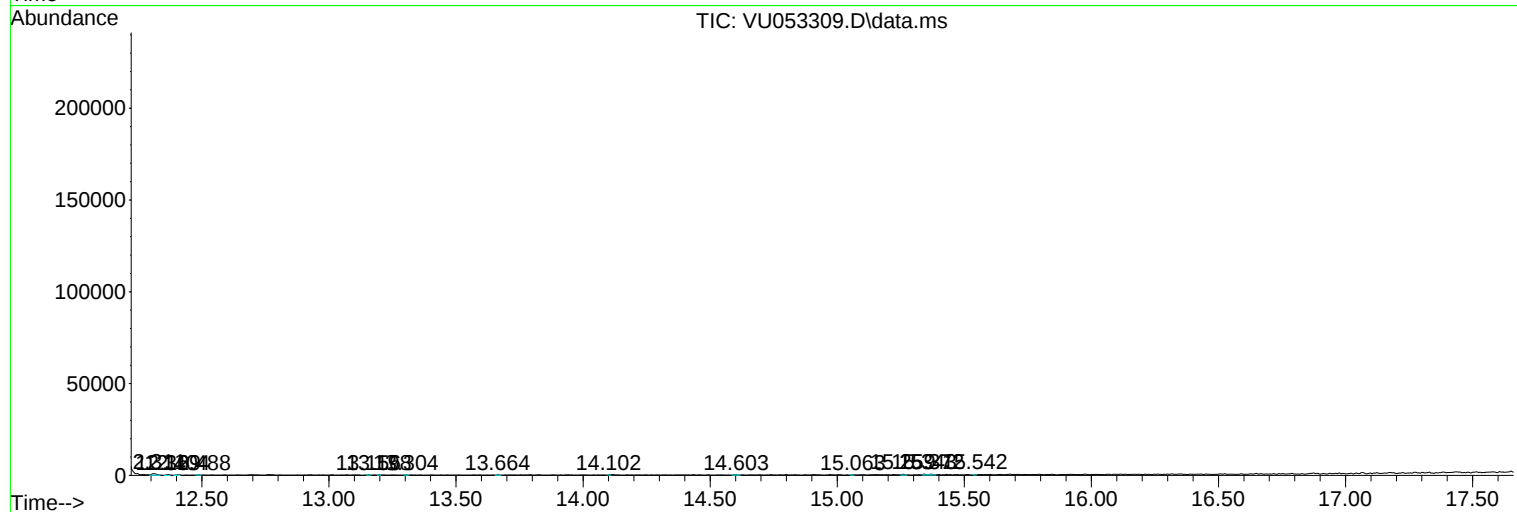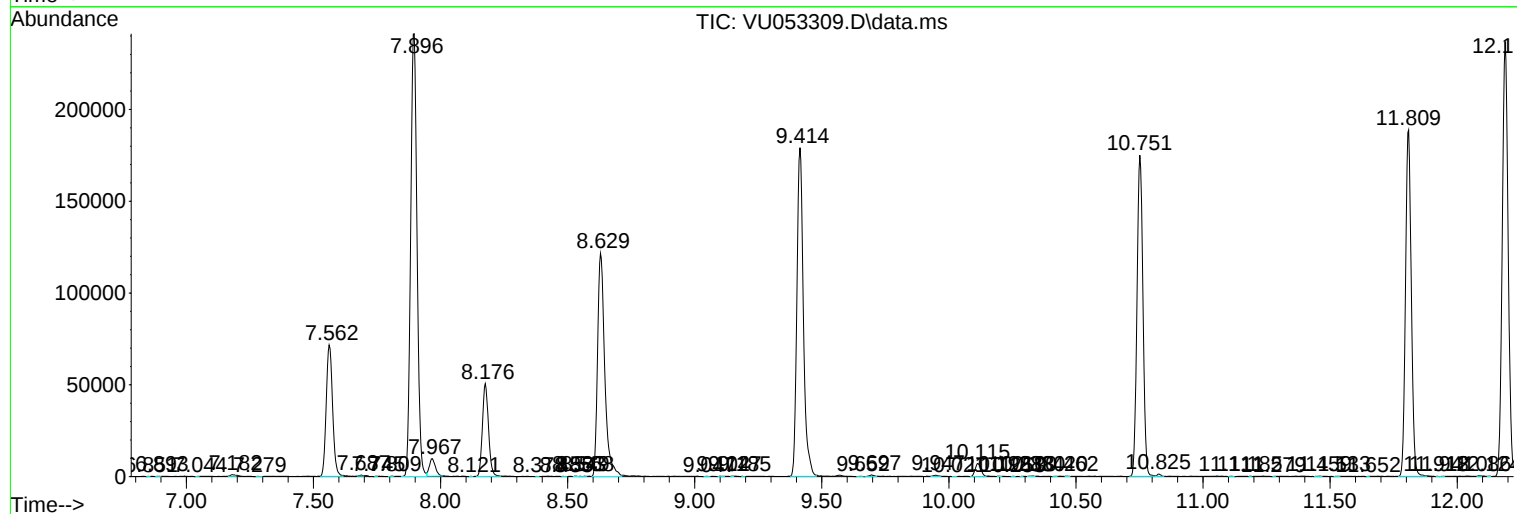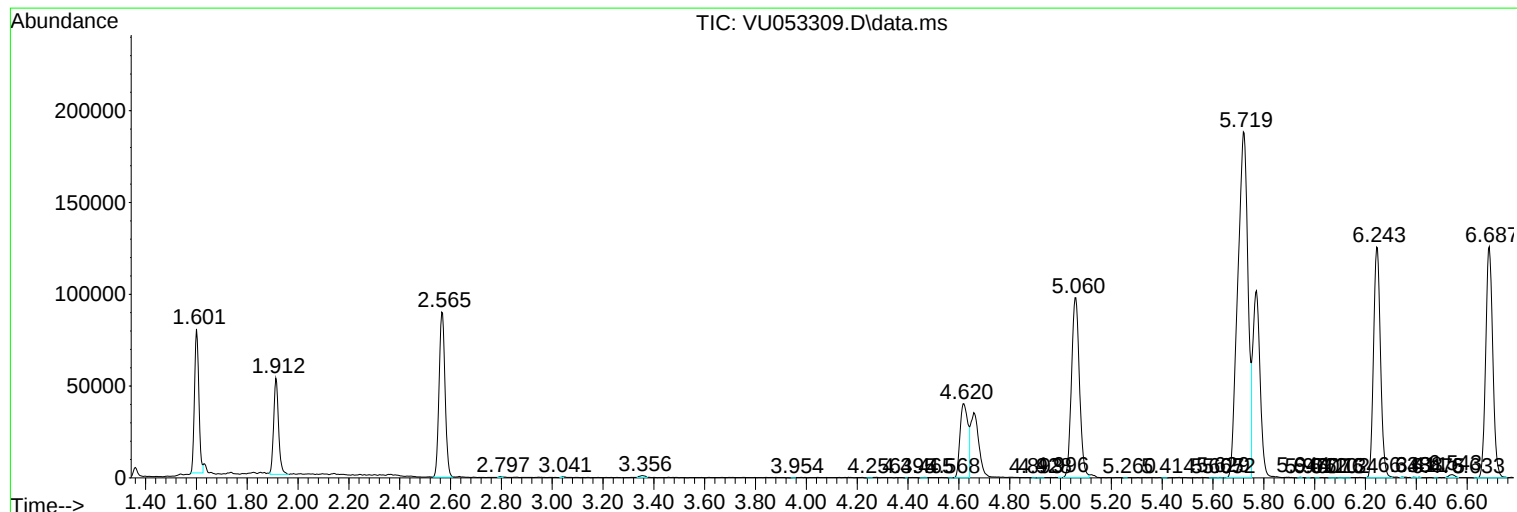

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053309.D
Acq On : 20 Mar 2023 16:21
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053309.D
Acq On : 20 Mar 2023 16:21
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------