

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053311.D
 Acq On : 20 Mar 2023 17:07
 Operator : JC/MD
 Sample : VIBLK117
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	88	rBV	64499	71953	15.52%	2.042%
2	1.912	170	178	198	rVB	58155	77804	16.78%	2.208%
3	2.565	369	381	399	rVB	98743	160263	34.56%	4.548%
4	2.706	422	425	432	rBV2	201	163	0.04%	0.005%
5	2.854	468	471	473	rBV	360	164	0.04%	0.005%
6	3.044	521	530	541	rVB3	5428	9539	2.06%	0.271%
7	3.176	566	571	574	rBV2	685	813	0.18%	0.023%
8	3.256	594	596	597	rBV2	181	76	0.02%	0.002%
9	3.269	598	600	604	rVB	186	99	0.02%	0.003%
10	3.350	623	625	628	rVB	217	87	0.02%	0.002%
11	3.858	780	783	786	rBV	225	204	0.04%	0.006%
12	3.919	799	802	804	rBV2	204	115	0.02%	0.003%
13	3.983	820	822	827	rBV	131	164	0.04%	0.005%
14	4.070	842	849	853	rBV	206	322	0.07%	0.009%
15	4.124	863	866	869	rBV	245	126	0.03%	0.004%
16	4.250	898	905	906	rBV	195	243	0.05%	0.007%
17	4.343	932	934	936	rVB	254	118	0.03%	0.003%
18	4.366	937	941	943	rBV	131	116	0.03%	0.003%
19	4.620	1009	1020	1043	rBV	32293	80625	17.39%	2.288%
20	4.880	1099	1101	1108	rVB	176	106	0.02%	0.003%
21	5.057	1142	1156	1180	rBV2	81833	182162	39.28%	5.170%
22	5.192	1195	1198	1202	rVB	300	231	0.05%	0.007%
23	5.214	1202	1205	1209	rBV	254	216	0.05%	0.006%
24	5.243	1212	1214	1217	rBB	145	100	0.02%	0.003%
25	5.285	1224	1227	1229	rBV	178	148	0.03%	0.004%
26	5.513	1296	1298	1302	rVB	240	115	0.02%	0.003%
27	5.555	1308	1311	1313	rBV	151	134	0.03%	0.004%
28	5.613	1326	1329	1331	rBV	193	162	0.03%	0.005%
29	5.719	1341	1362	1372	rBV2	168444	463744	100.00%	13.162%
30	5.909	1420	1421	1424	rVB	265	109	0.02%	0.003%
31	5.938	1428	1430	1432	rBV	153	108	0.02%	0.003%
32	5.999	1447	1449	1451	rBV	193	103	0.02%	0.003%
33	6.099	1476	1480	1481	rBV	256	194	0.04%	0.006%
34	6.134	1489	1491	1495	rVB	278	155	0.03%	0.004%
35	6.156	1496	1498	1500	rBV	162	103	0.02%	0.003%
36	6.243	1512	1525	1546	rBV	147406	280475	60.48%	7.960%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053311.D
 Acq On : 20 Mar 2023 17:07
 Operator : JC/MD
 Sample : VIBLK117
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.513	1607	1609	1611	rBV	144	101	0.02%	0.003%
38	6.684	1650	1662	1678	rBV2	104205	204967	44.20%	5.817%
39	6.774	1686	1690	1694	rBV	224	248	0.05%	0.007%
40	6.803	1696	1699	1701	rVV	253	154	0.03%	0.004%
41	6.816	1701	1703	1707	rVB	208	118	0.03%	0.003%
42	6.899	1724	1729	1732	rBV	268	278	0.06%	0.008%
43	7.044	1771	1774	1777	rBB	150	123	0.03%	0.003%
44	7.095	1788	1790	1794	rBV	148	153	0.03%	0.004%
45	7.243	1832	1836	1837	rBV	149	97	0.02%	0.003%
46	7.359	1870	1872	1874	rVB	233	109	0.02%	0.003%
47	7.468	1904	1906	1909	rVB2	153	90	0.02%	0.003%
48	7.562	1923	1935	1955	rVB	63384	109460	23.60%	3.107%
49	7.703	1977	1979	1983	rBV	220	91	0.02%	0.003%
50	7.780	2000	2003	2006	rBV	141	149	0.03%	0.004%
51	7.832	2011	2019	2023	rBV	275	367	0.08%	0.010%
52	7.893	2026	2038	2052	rBV	216355	369831	79.75%	10.496%
53	8.092	2098	2100	2103	rVB2	157	80	0.02%	0.002%
54	8.134	2110	2113	2116	rBV	134	108	0.02%	0.003%
55	8.176	2116	2126	2142	rVB	42418	70309	15.16%	1.995%
56	8.298	2162	2164	2166	rBV	205	101	0.02%	0.003%
57	8.333	2172	2175	2179	rBV	178	189	0.04%	0.005%
58	8.359	2180	2183	2185	rVV	136	78	0.02%	0.002%
59	8.475	2216	2219	2221	rVB	243	126	0.03%	0.004%
60	8.555	2241	2244	2246	rBV2	132	77	0.02%	0.002%
61	8.629	2256	2267	2291	rBV2	93408	174925	37.72%	4.965%
62	8.822	2324	2327	2330	rBV	201	204	0.04%	0.006%
63	8.954	2364	2368	2370	rBV	190	171	0.04%	0.005%
64	9.008	2383	2385	2388	rBV	131	113	0.02%	0.003%
65	9.031	2390	2392	2395	rVB	146	81	0.02%	0.002%
66	9.169	2431	2435	2438	rVB2	159	146	0.03%	0.004%
67	9.221	2449	2451	2454	rVB	297	172	0.04%	0.005%
68	9.243	2455	2458	2461	rBV	144	157	0.03%	0.004%
69	9.304	2473	2477	2479	rBV	186	178	0.04%	0.005%
70	9.414	2499	2511	2532	rBV	211351	361257	77.90%	10.253%
71	9.568	2551	2559	2566	rBV3	667	1097	0.24%	0.031%
72	9.606	2567	2571	2573	rVV	181	141	0.03%	0.004%
73	9.693	2594	2598	2605	rVB3	508	668	0.14%	0.019%
74	9.934	2668	2673	2674	rBV	319	230	0.05%	0.007%
75	10.002	2693	2694	2696	rBV	223	111	0.02%	0.003%
76	10.115	2720	2729	2741	rBV	6219	9279	2.00%	0.263%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
 Data File : VU053311.D
 Acq On : 20 Mar 2023 17:07
 Operator : JC/MD
 Sample : VIBLK117
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.404	2815	2819	2820	rBV	190	155	0.03%	0.004%
78	10.536	2853	2860	2865	rBV	200	352	0.08%	0.010%
79	10.597	2876	2879	2883	rBV2	156	107	0.02%	0.003%
80	10.632	2888	2890	2894	rVB	168	79	0.02%	0.002%
81	10.751	2915	2927	2946	rBV	142523	223958	48.29%	6.356%
82	10.860	2959	2961	2962	rBV	174	91	0.02%	0.003%
83	11.005	3004	3006	3008	rVB2	163	87	0.02%	0.002%
84	11.401	3125	3129	3136	rVB2	165	144	0.03%	0.004%
85	11.806	3244	3255	3271	rBV	213419	341350	73.61%	9.688%
86	12.188	3361	3374	3397	rBV	195761	316347	68.22%	8.978%
87	12.311	3407	3412	3420	rVB3	669	988	0.21%	0.028%
88	12.356	3423	3426	3429	rBV	208	135	0.03%	0.004%
89	12.494	3467	3469	3471	rBV	226	92	0.02%	0.003%
90	13.063	3643	3646	3654	rBV2	259	209	0.05%	0.006%
91	13.124	3662	3665	3668	rVB	226	122	0.03%	0.003%
92	13.449	3764	3766	3769	rBV	148	102	0.02%	0.003%
93	14.330	4038	4040	4044	rBV	202	95	0.02%	0.003%
94	14.507	4093	4095	4100	rVB2	267	164	0.04%	0.005%
95	14.581	4116	4118	4120	rBB	191	72	0.02%	0.002%
96	14.770	4176	4177	4180	rBV	259	163	0.04%	0.005%
97	14.870	4206	4208	4211	rBV	294	198	0.04%	0.006%
98	15.031	4255	4258	4266	rVB	433	449	0.10%	0.013%
99	15.336	4350	4353	4355	rBV	214	151	0.03%	0.004%
100	15.365	4360	4362	4365	rBV	255	136	0.03%	0.004%




Sum of corrected areas: 3523439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053311.D
Acq On : 20 Mar 2023 17:07
Operator : JC/MD
Sample : VIBLK117
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

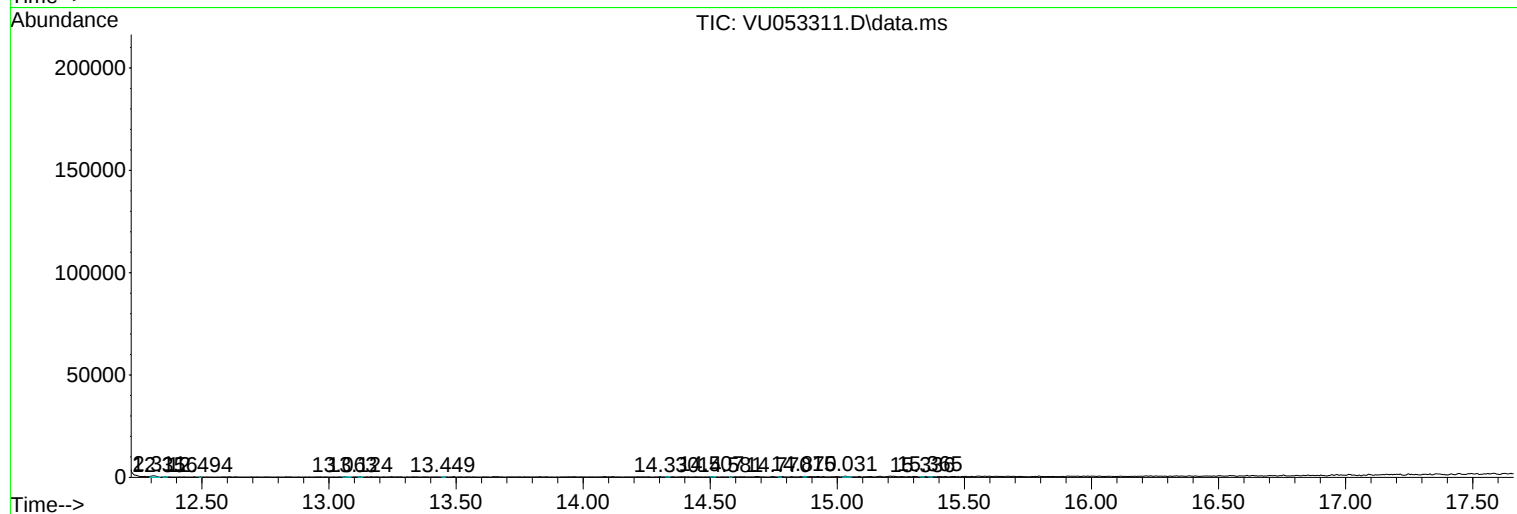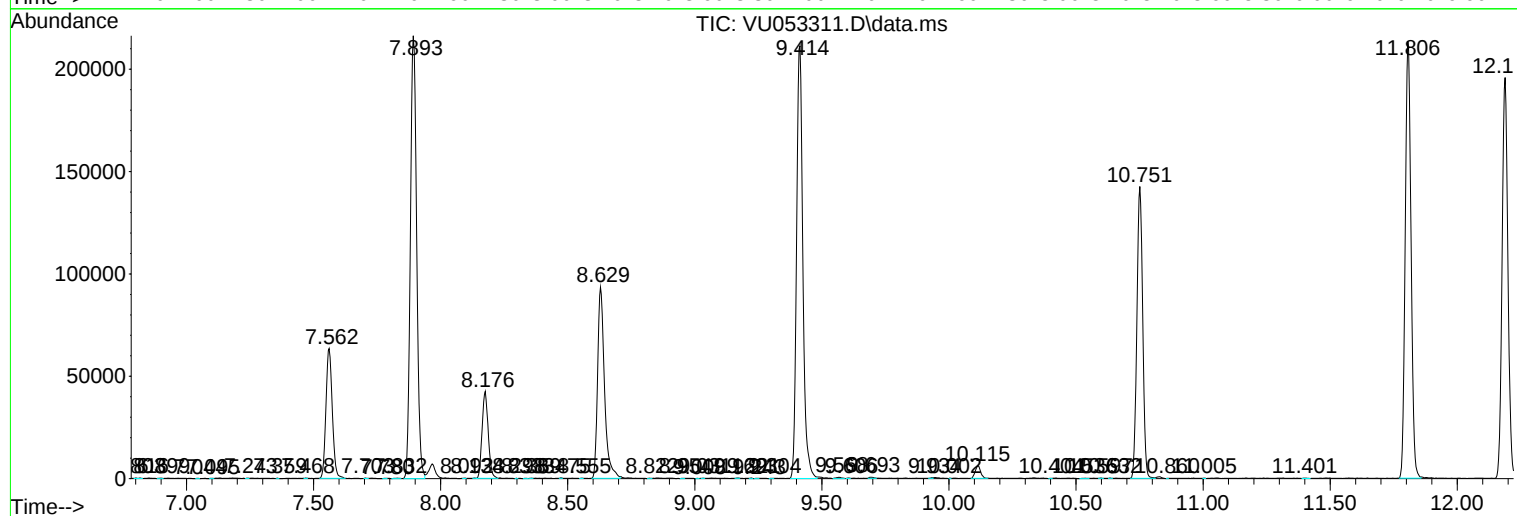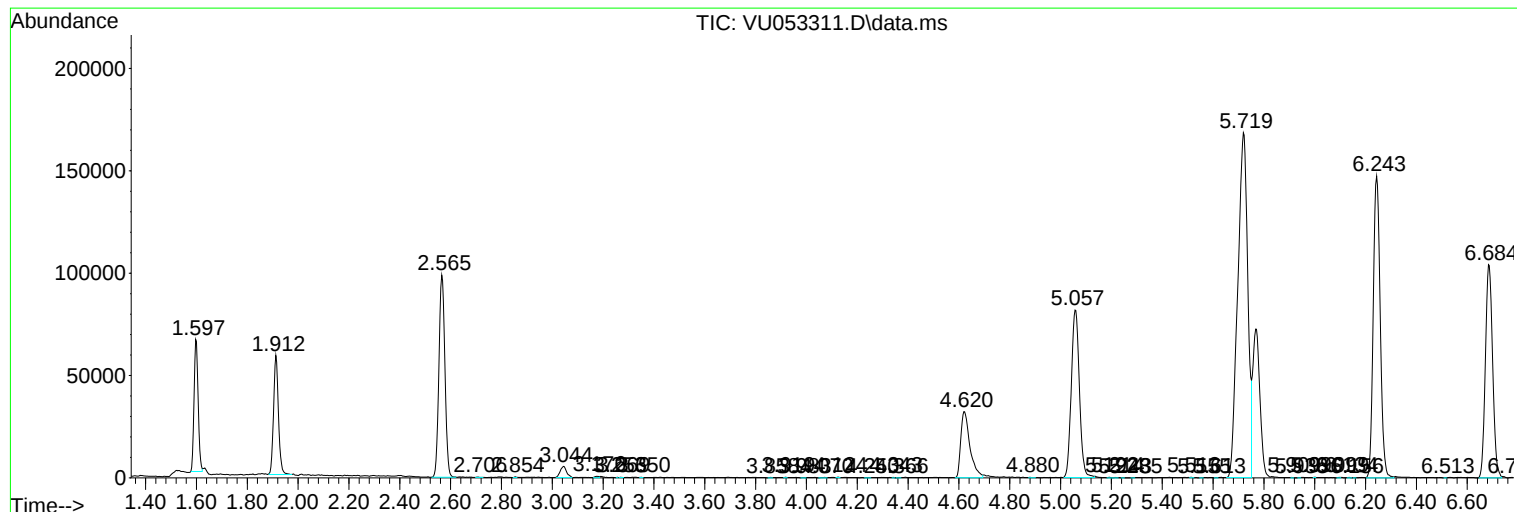

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053311.D
Acq On : 20 Mar 2023 17:07
Operator : JC/MD
Sample : VIBLK117
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053311.D
Acq On : 20 Mar 2023 17:07
Operator : JC/MD
Sample : VIBLK117
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------