


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032023\
Data File : VU053295.D
Acq On : 20 Mar 2023 09:38
Operator : JC/MD
Sample : BFB166
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB166

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Thu Mar 23 02:41:20 2023

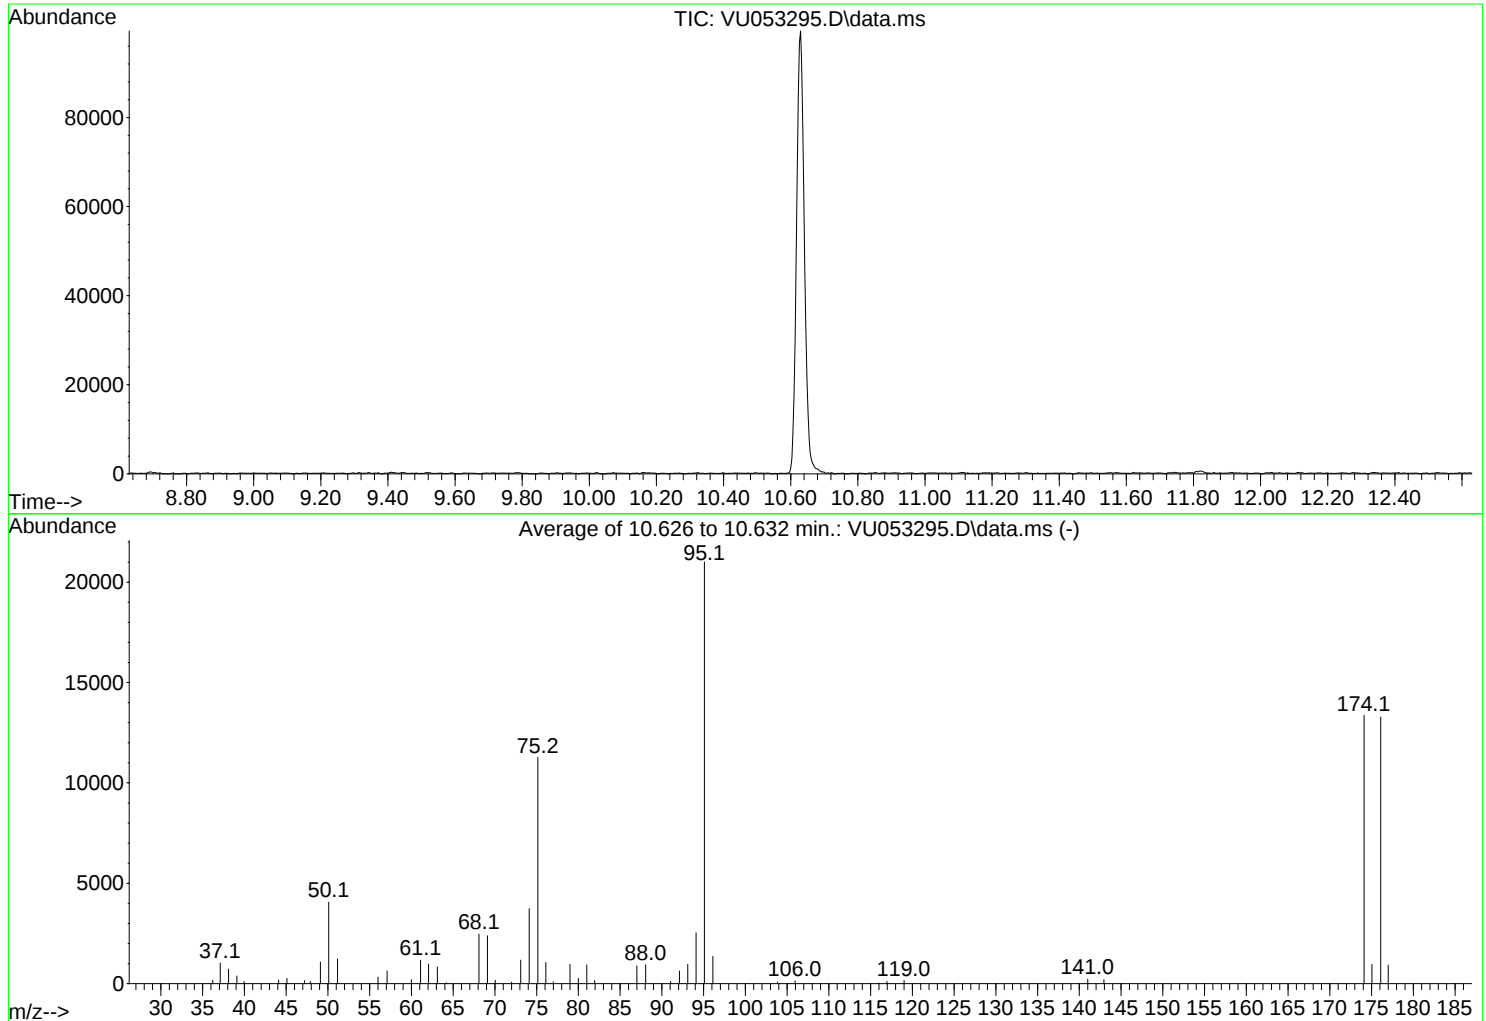

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	4061	PASS
75	95	30	80	53.6	11270	PASS
95	95	100	100	100.0	21013	PASS
96	95	5	9	6.4	1352	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.6	13364	PASS
175	174	5	9	7.2	957	PASS
176	174	95	101	99.4	13282	PASS
177	176	5	9	6.9	923	PASS

m/z	Abundance
44.20	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
36.20	158.0
37.10	1023.0
38.10	720.0
39.10	362.0
40.00	105.0
44.10	360.0
45.10	275.0
47.20	169.0
47.90	105.0
49.10	1024.0
50.10	4214.0
51.10	1274.0
56.00	329.0
57.10	619.0
60.00	189.0
61.10	1208.0
62.10	1083.0
63.10	856.0
64.20	120.0
68.10	2439.0
69.10	2321.0
70.10	168.0
72.00	106.0
73.10	1219.0
74.10	3623.0
75.20	11326.0
76.10	1159.0
77.00	141.0
79.00	992.0
80.00	263.0
81.00	985.0
82.00	164.0
87.00	882.0
88.00	958.0
91.00	101.0
92.10	570.0
93.10	980.0
94.10	2691.0
95.10	21288.0
96.10	1406.0
105.90	122.0
116.00	107.0
116.90	109.0
119.00	156.0
141.00	219.0
142.90	185.0
174.10	12940.0
175.10	987.0
176.10	13158.0
177.00	837.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
36.20	179.0
37.10	1055.0
38.10	756.0
39.10	391.0
39.90	112.0
44.10	370.0
45.10	276.0
47.20	165.0
47.90	122.0
49.10	1116.0
50.10	4134.0
51.10	1225.0
56.00	343.0
57.10	643.0
60.00	207.0
61.10	1203.0
62.00	979.0
63.10	840.0
68.10	2545.0
69.10	2490.0
70.00	170.0
73.10	1223.0
74.10	3899.0
75.10	11617.0
76.10	1102.0
77.00	126.0
79.00	970.0
80.00	281.0
81.00	944.0
82.00	151.0
87.00	891.0
88.10	965.0
91.10	114.0
92.10	647.0
93.10	975.0
94.10	2558.0
95.10	21680.0
96.10	1388.0
103.80	117.0
105.90	141.0
116.90	127.0
119.00	157.0
141.00	238.0
142.90	215.0
174.10	13871.0
175.00	950.0
176.10	13745.0
177.00	972.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
36.20	159.0
37.10	1005.0
38.10	705.0
39.10	384.0
40.00	101.0
44.10	365.0
45.10	235.0
47.20	142.0
47.90	105.0
49.10	1079.0
50.10	3836.0
51.20	1196.0
56.00	313.0
57.10	615.0
60.00	193.0
61.10	1076.0
62.00	869.0
63.10	793.0
68.10	2441.0
69.10	2338.0
70.00	173.0
72.00	112.0
73.10	1073.0
74.10	3698.0
75.10	10868.0
76.10	908.0
79.00	899.0
80.00	275.0
81.00	866.0
81.90	147.0
87.00	891.0
88.10	888.0
91.10	103.0
92.10	668.0
93.10	919.0
94.10	2366.0
95.10	20072.0
96.10	1261.0
103.90	122.0
106.00	135.0
117.00	107.0
119.00	158.0
141.00	205.0
143.00	205.0
174.10	13280.0
175.00	935.0
176.10	12944.0
177.00	960.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166