

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032024\
 Data File : VU058174.D
 Acq On : 20 Mar 2024 13:46
 Operator : MD/SY
 Sample : VU0320WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK152

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	106	rBV	41002	47813	12.86%	1.577%
2	1.911	184	193	202	rBV	44671	59900	16.11%	1.975%
3	2.557	381	394	412	rVB	75823	122048	32.82%	4.024%
4	3.036	533	543	557	rVB	6445	11886	3.20%	0.392%
5	4.624	1028	1037	1072	rBV	47905	127073	34.17%	4.190%
6	5.055	1156	1171	1189	rBV	74367	162377	43.66%	5.354%
7	5.717	1358	1377	1404	rBV2	145615	371885	100.00%	12.263%
8	6.242	1528	1540	1561	rBV	135037	256489	68.97%	8.458%
9	6.531	1619	1630	1641	rVB8	2393	4547	1.22%	0.150%
10	6.682	1665	1677	1697	rBV	91647	180536	48.55%	5.953%
11	7.560	1939	1950	1973	rBV2	36308	65209	17.53%	2.150%
12	7.891	2041	2053	2074	rBV	164858	291472	78.38%	9.611%
13	8.177	2131	2142	2160	rBV2	20030	35245	9.48%	1.162%
14	8.631	2268	2283	2315	rBV2	156465	360638	96.98%	11.892%
15	9.412	2514	2526	2555	rBV	181202	310310	83.44%	10.232%
16	10.749	2929	2942	2962	rBV	56888	94230	25.34%	3.107%
17	11.807	3260	3271	3290	rBV	167527	275382	74.05%	9.081%
18	12.190	3375	3390	3410	rBV	141444	238343	64.09%	7.859%
19	12.765	3559	3569	3581	rBV2	6106	9008	2.42%	0.297%
20	14.572	4121	4131	4141	rBV2	5323	8239	2.22%	0.272%




Sum of corrected areas: 3032630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032024\
Data File : VU058174.D
Acq On : 20 Mar 2024 13:46
Operator : MD/SY
Sample : VU0320WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

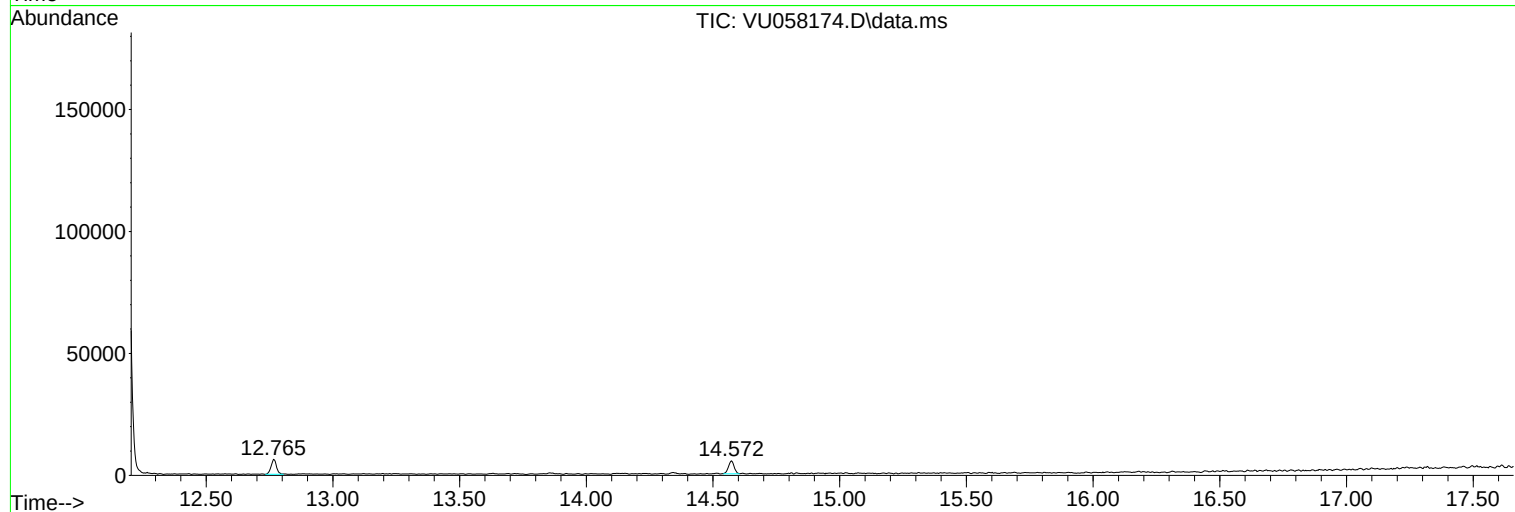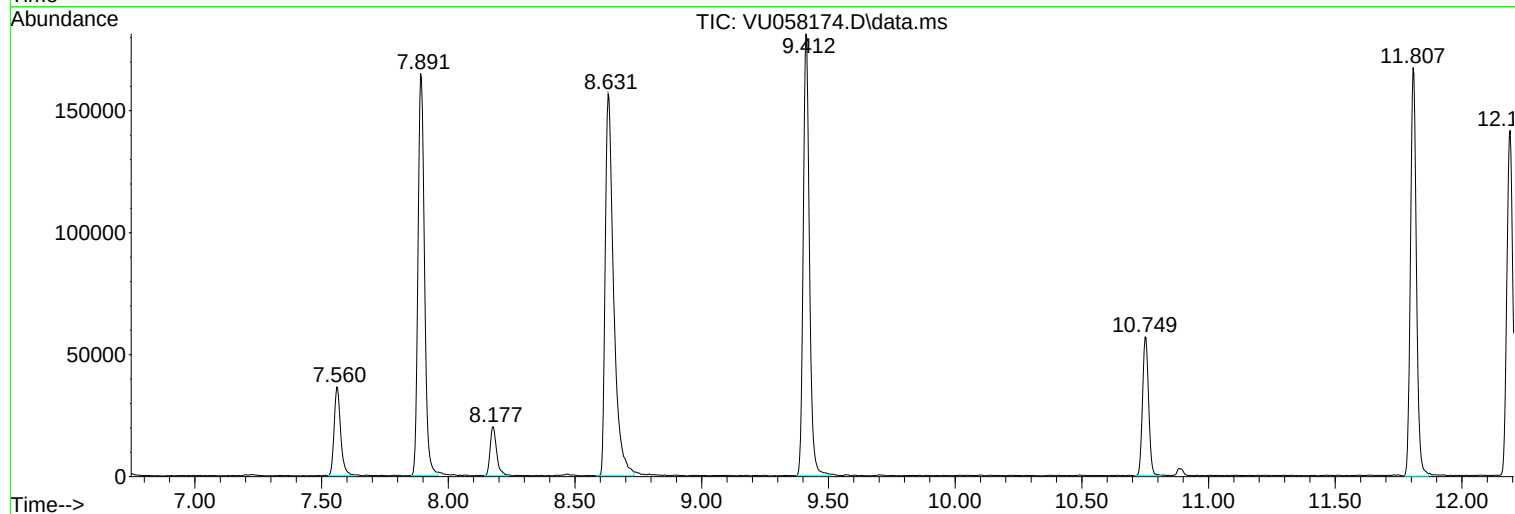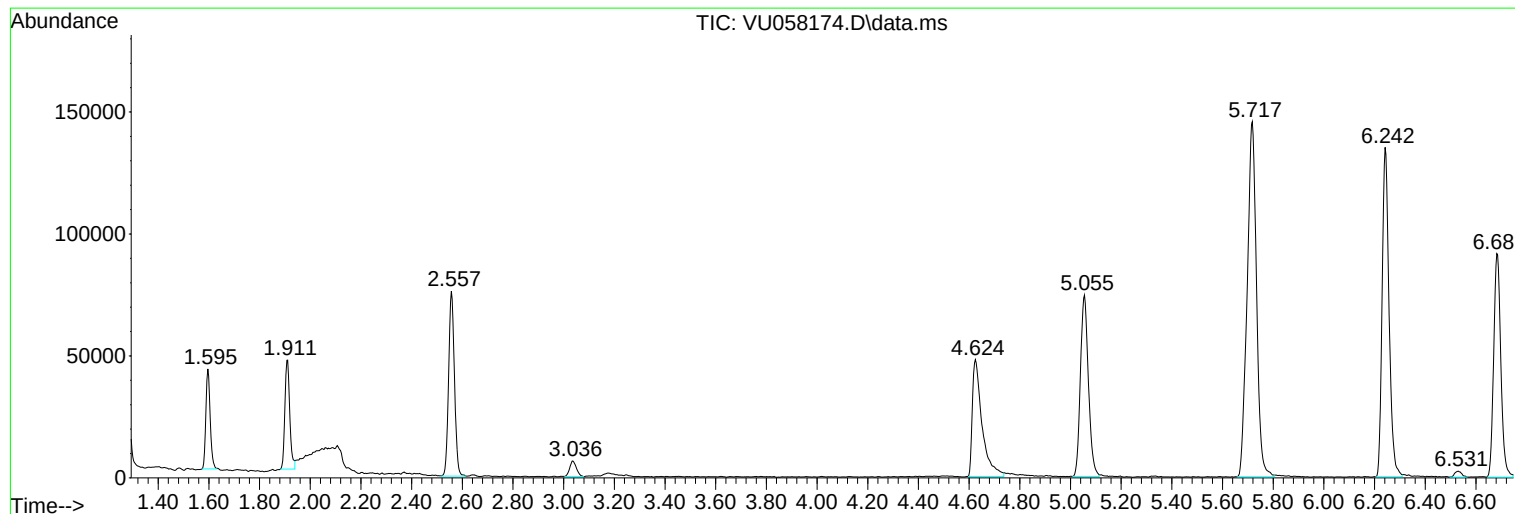

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032024\
Data File : VU058174.D
Acq On : 20 Mar 2024 13:46
Operator : MD/SY
Sample : VU0320WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032024\
Data File : VU058174.D
Acq On : 20 Mar 2024 13:46
Operator : MD/SY
Sample : VU0320WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc