


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032024\
Data File : VU058172.D
Acq On : 20 Mar 2024 11:13
Operator : MD/SY
Sample : BFB126
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB126

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 21 15:02:21 2024

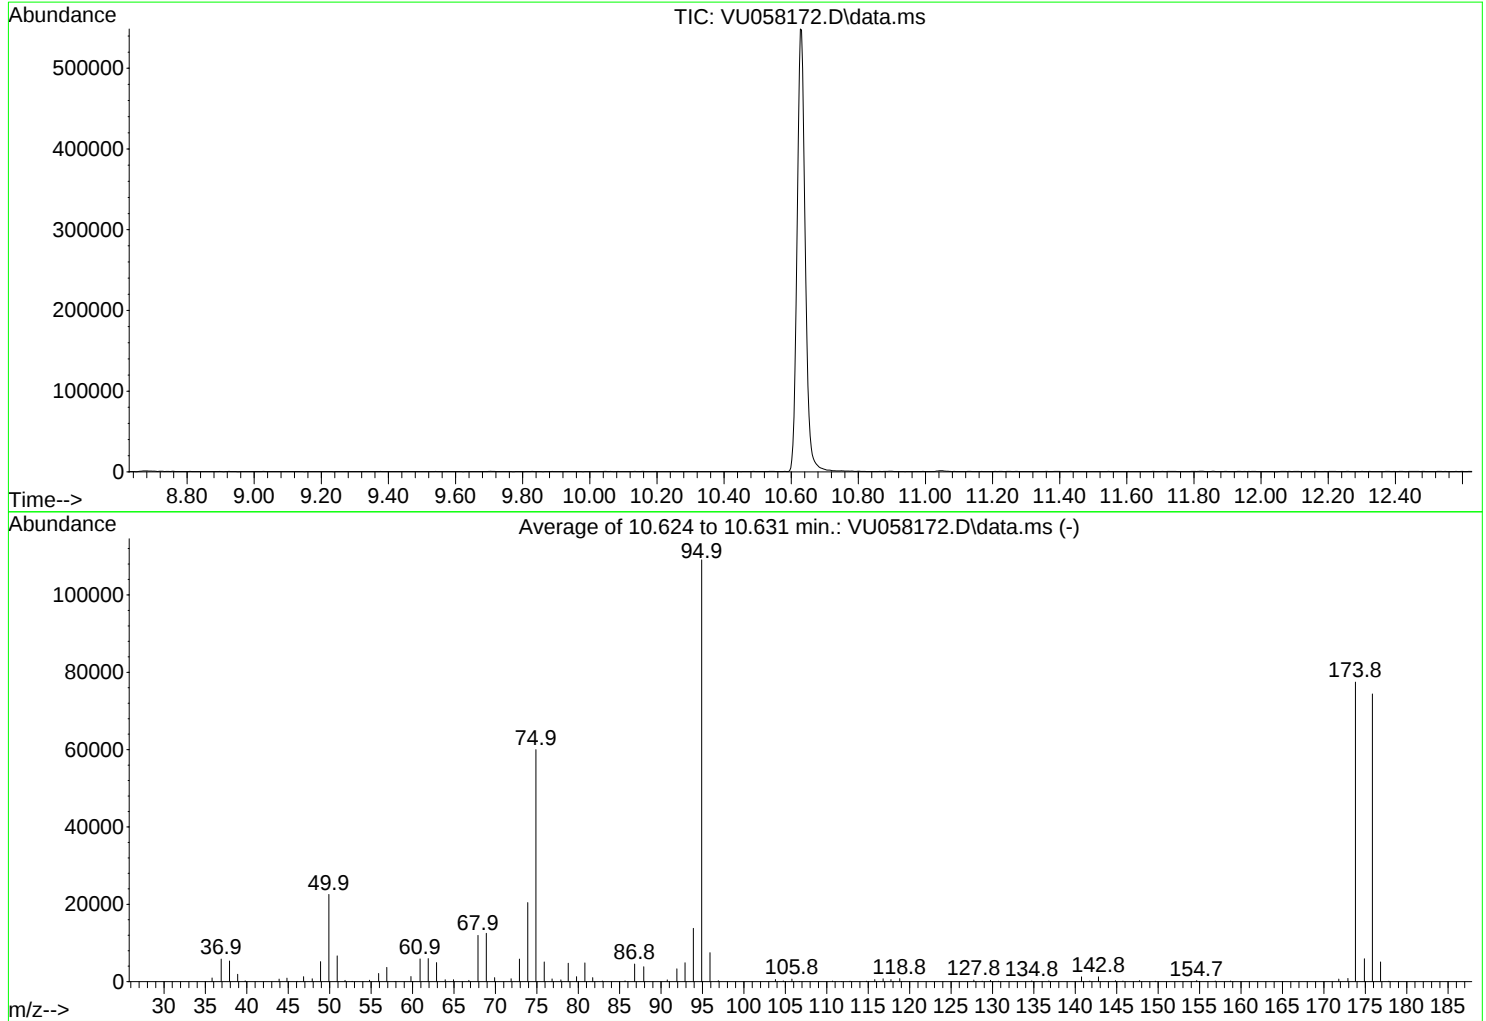

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	22539	PASS
75	95	30	80	55.0	60005	PASS
95	95	100	100	100.0	109077	PASS
96	95	5	9	6.9	7508	PASS
173	174	0.00	2	1.1	828	PASS
174	95	50	120	71.0	77467	PASS
175	174	5	9	7.6	5910	PASS
176	174	95	101	96.0	74405	PASS
177	176	5	9	6.9	5097	PASS

Scan 2891 (10.586 min): VU058172.D\data.ms
BFB126

m/z	Abundance
39.90	148.0
43.90	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB126

m/z	Abundance
35.80	902.0
36.90	5538.0
37.90	5188.0
38.90	1845.0
39.80	319.0
43.90	930.0
44.90	917.0
46.00	102.0
46.90	1167.0
47.90	799.0
48.90	4913.0
49.90	21496.0
50.90	6440.0
51.80	324.0
54.80	377.0
55.90	1984.0
56.90	3536.0
57.90	137.0
59.80	1236.0
60.90	5441.0
61.90	5816.0
62.90	4602.0
63.90	455.0
65.00	496.0
66.80	312.0
67.90	11599.0
68.90	12047.0
69.90	1065.0
71.90	645.0
72.90	5572.0
73.90	19488.0
74.90	56704.0
75.90	4864.0
76.80	697.0
77.90	408.0
78.80	4387.0
79.80	1207.0
80.80	4412.0
81.80	890.0
82.90	121.0
85.60	199.0
86.80	4446.0
87.90	3587.0
90.70	423.0
91.90	3033.0
92.90	4356.0
93.90	12837.0
94.90	103200.0
95.90	7200.0
96.90	217.0
103.80	483.0
104.70	181.0
105.80	602.0
110.70	111.0
112.80	113.0
114.80	111.0
115.80	529.0
116.80	639.0
117.70	508.0
118.80	751.0
127.80	392.0
128.80	157.0
129.70	276.0
130.80	126.0
134.80	160.0
136.80	212.0
140.70	1277.0
141.70	177.0
142.80	1099.0
144.90	227.0
145.80	134.0
147.70	252.0
149.60	136.0
154.60	192.0
155.00	127.0
156.90	169.0
158.70	148.0
171.80	589.0
172.90	789.0
173.80	71728.0
174.90	5529.0
175.90	68616.0
176.90	4797.0
177.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB126

m/z	Abundance
35.80	950.0
36.90	6048.0
37.90	5462.0
38.90	1943.0
39.80	349.0
43.90	1002.0
44.80	933.0
46.80	1332.0
47.90	758.0
48.90	5329.0
49.90	23248.0
50.90	6849.0
51.90	332.0
52.70	100.0
54.80	408.0
55.90	2205.0
56.90	3839.0
57.90	121.0
59.80	1378.0
60.90	6002.0
61.90	6127.0
62.90	5056.0
63.90	537.0
65.00	490.0
66.80	363.0
67.90	12348.0
68.90	12965.0
69.90	1089.0
71.90	758.0
72.90	6026.0
73.90	21080.0
74.90	61856.0
75.90	5209.0
76.90	724.0
77.90	455.0
78.80	4861.0
79.80	1342.0
80.80	4981.0
81.70	1030.0
82.90	166.0
85.60	222.0
86.80	4613.0
87.90	3937.0
90.70	460.0
91.90	3393.0
92.90	5087.0
93.90	14205.0
94.90	112496.0
95.90	7781.0
96.90	259.0
103.80	559.0
104.80	186.0
105.80	677.0
110.70	160.0
111.80	103.0
112.80	134.0
114.80	145.0
115.80	562.0
116.80	764.0
117.80	533.0
118.80	795.0
127.70	431.0
128.70	139.0
129.80	325.0
130.70	141.0
134.70	192.0
136.80	235.0
140.70	1294.0
141.70	166.0
142.80	1259.0
144.80	278.0
145.70	192.0
147.80	282.0
149.60	158.0
154.60	292.0
156.90	172.0
158.80	152.0
171.80	680.0
172.90	863.0
173.80	79864.0
174.90	6141.0
175.80	76768.0
176.80	5303.0
177.90	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB126

m/z	Abundance
35.80	972.0
36.90	5914.0
37.90	5348.0
38.90	1953.0
39.80	341.0
43.90	1037.0
44.80	883.0
46.10	102.0
46.80	1356.0
47.90	661.0
48.90	5254.0
49.90	22872.0
50.90	6708.0
51.80	312.0
52.70	117.0
54.80	400.0
55.90	2168.0
56.90	3658.0
59.80	1405.0
60.90	6133.0
61.90	5911.0
62.90	5156.0
64.00	545.0
64.90	503.0
66.80	377.0
67.90	11938.0
68.90	12509.0
69.90	989.0
71.90	815.0
72.90	5872.0
73.90	20776.0
74.90	61456.0
75.90	5161.0
76.90	680.0
77.90	476.0
78.80	4974.0
79.80	1333.0
80.80	5099.0
81.70	1138.0
82.90	170.0
85.70	217.0
86.80	4578.0
87.90	4070.0
90.80	476.0
91.90	3482.0
92.90	5243.0
93.90	14267.0
94.90	111536.0
95.90	7542.0
96.90	258.0
103.80	618.0
104.80	221.0
105.80	688.0
106.70	104.0
110.70	199.0
112.80	111.0
114.80	128.0
115.80	553.0
116.80	879.0
117.80	520.0
118.80	774.0
127.70	410.0
128.70	136.0
129.80	388.0
130.70	175.0
134.70	220.0
136.80	237.0
140.80	1183.0
141.80	140.0
142.80	1416.0
144.80	292.0
145.70	197.0
147.70	308.0
149.70	135.0
154.70	347.0
156.90	181.0
158.80	153.0
171.80	715.0
172.90	832.0
173.80	80808.0
174.90	6060.0
175.80	77832.0
176.80	5190.0
177.90	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB126