

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (QT Reviewed)


Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:38:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

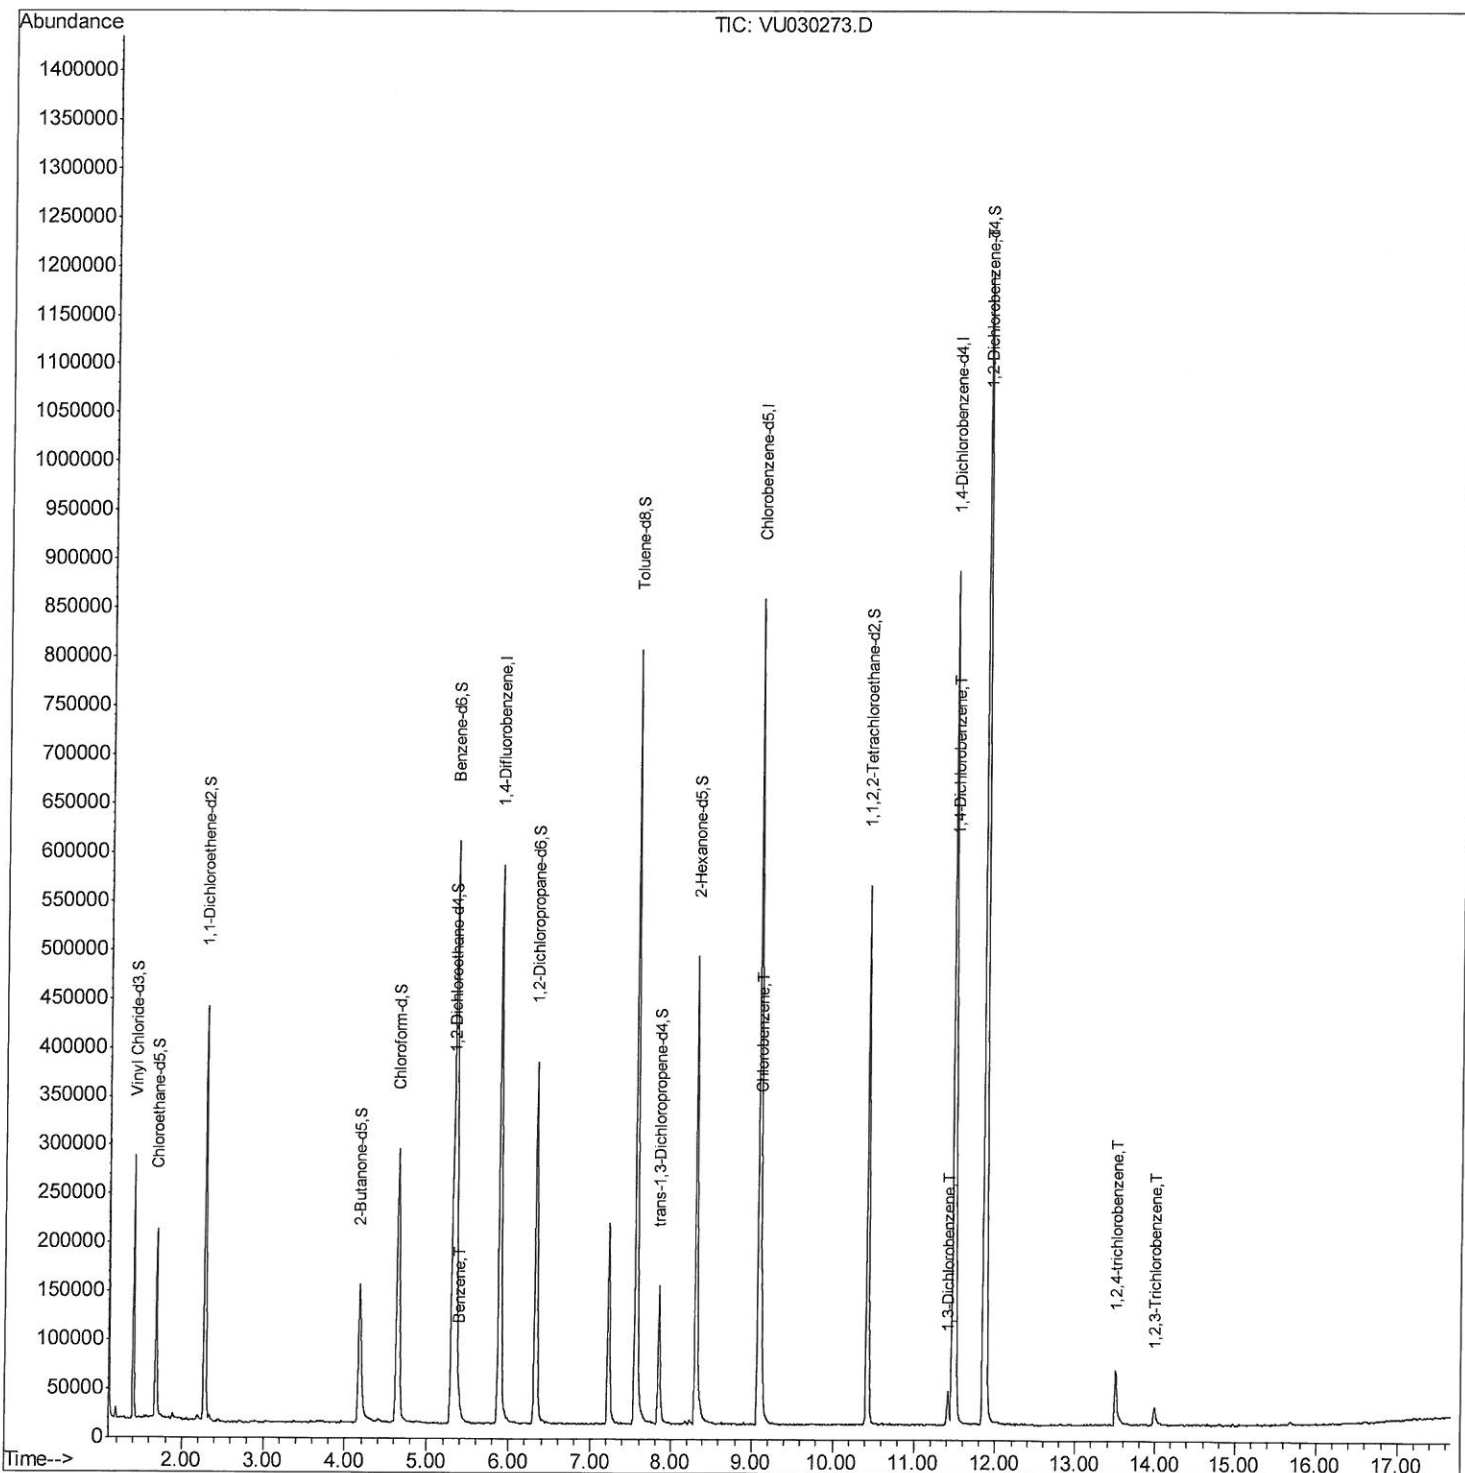

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (Qedit)




Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:18:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

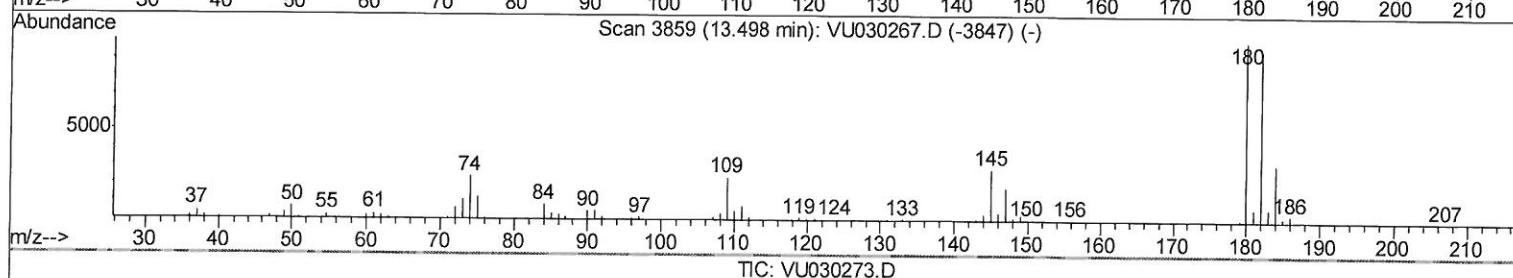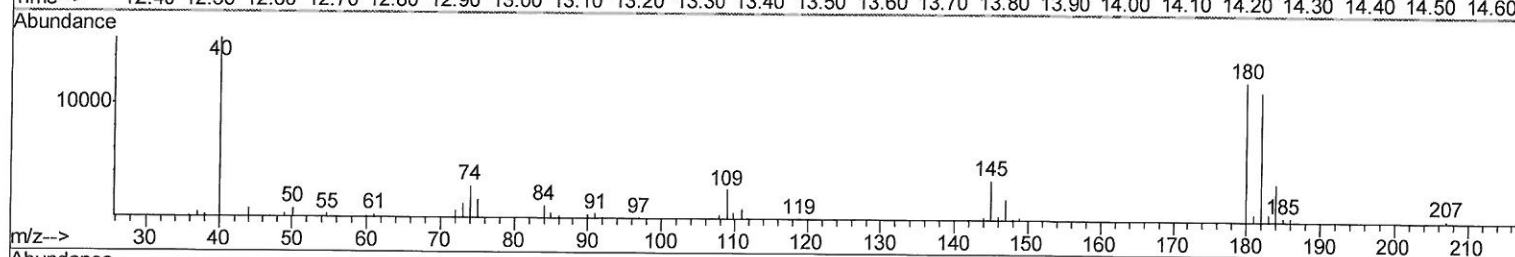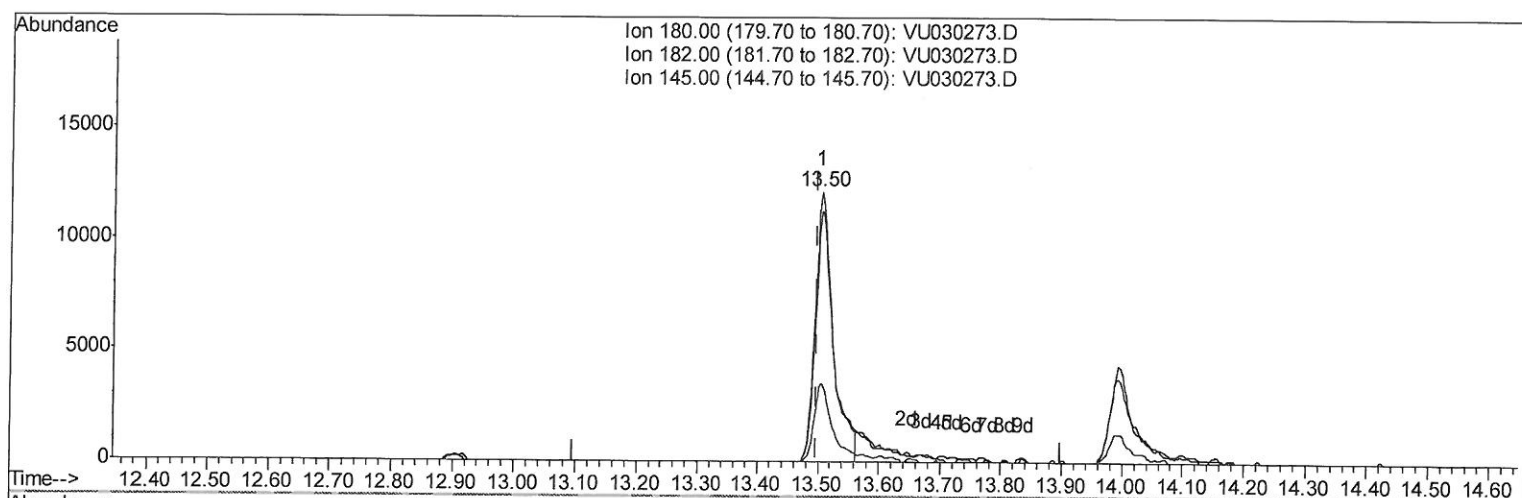

TIC: VU030273.D

(68) 1,2,4-trichlorobenzene (T)

13.504min (+0.006) 4.63ug/L

response 25053

Ion	Exp%	Act%
180.00	100	100
182.00	95.50	98.78
145.00	28.40	29.53
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (Qedit)




Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:18:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

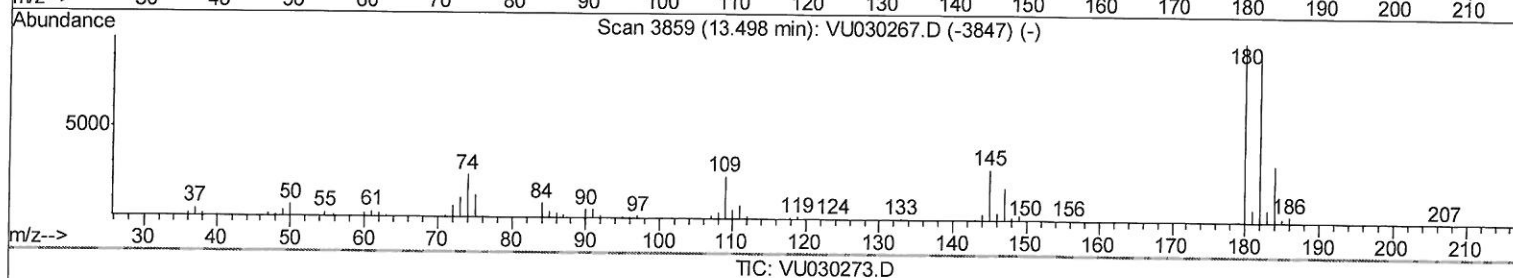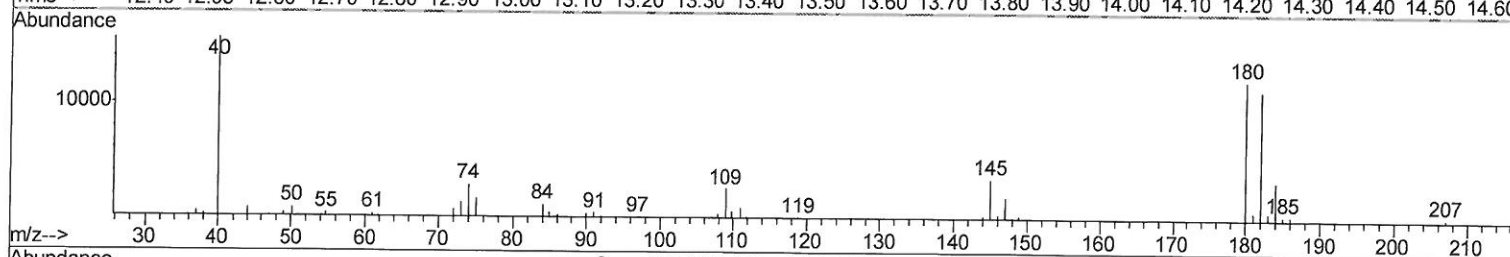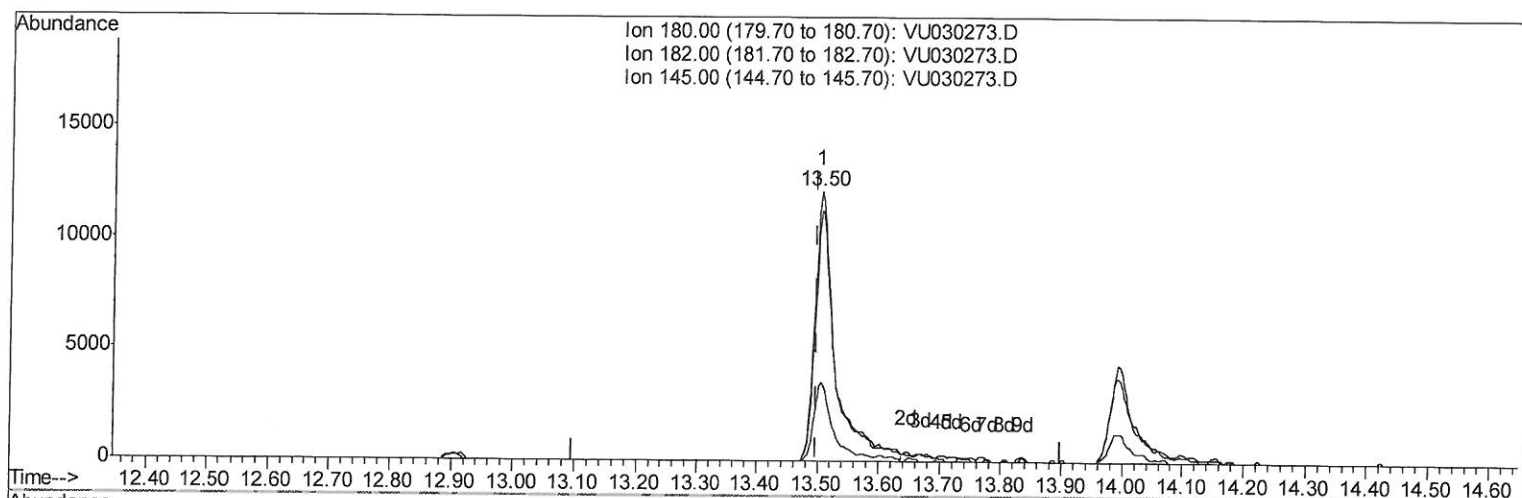

(68) 1,2,4-trichlorobenzene (T)

13.504min (+0.006) 5.27ug/L m

response 28533

Ion	Exp%	Act%
180.00	100	100
182.00	95.50	86.73
145.00	28.40	25.92
0.00	0.00	0.00

7 M
3/22/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (Qedit)




Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:18:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

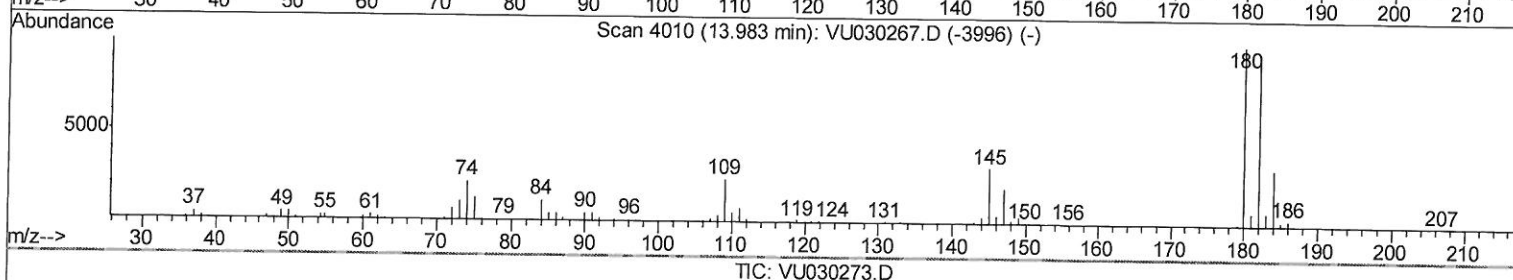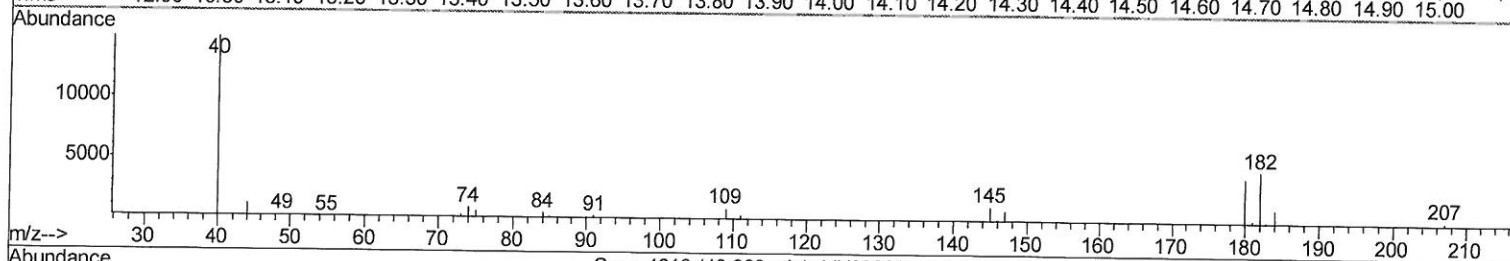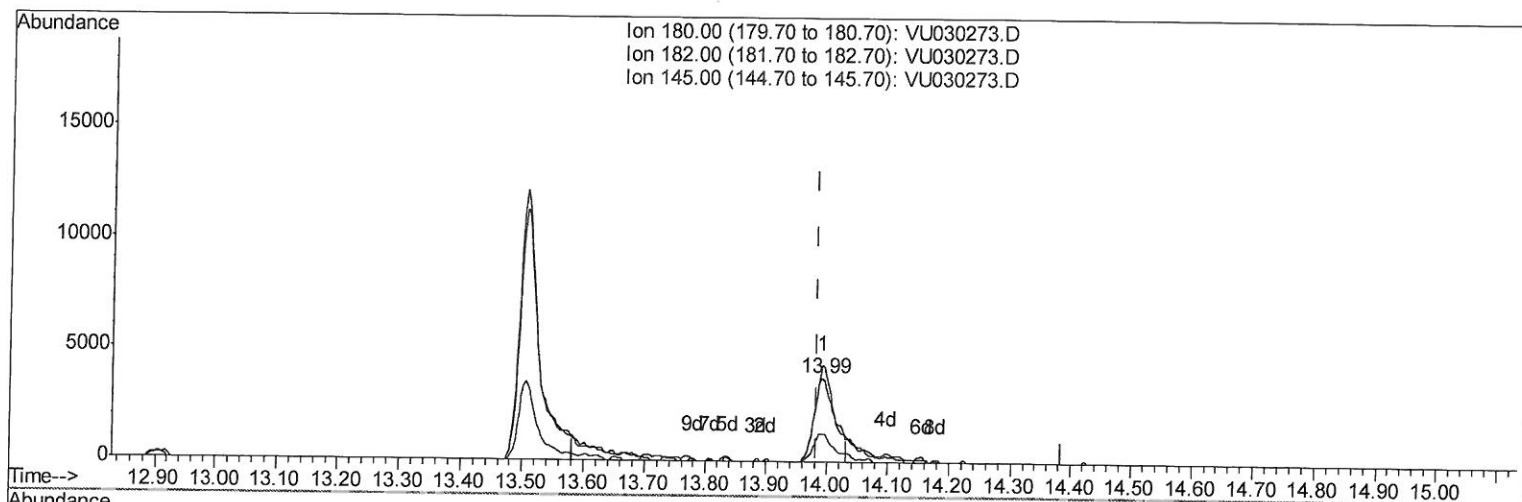

(70) 1,2,3-Trichlorobenzene (T)

13.993min (+0.010) 1.59ug/L

response 8973

Ion	Exp%	Act%
180.00	100	100
182.00	94.90	124.93#
145.00	30.10	15.87#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (Qedit)




Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:18:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

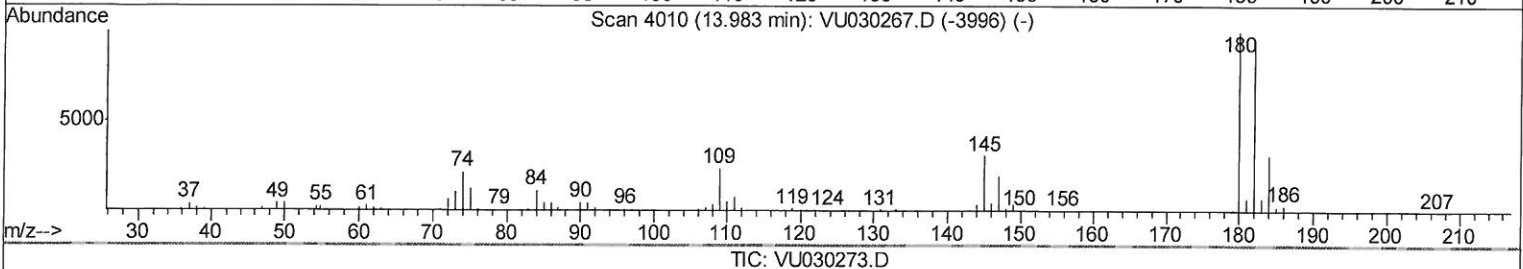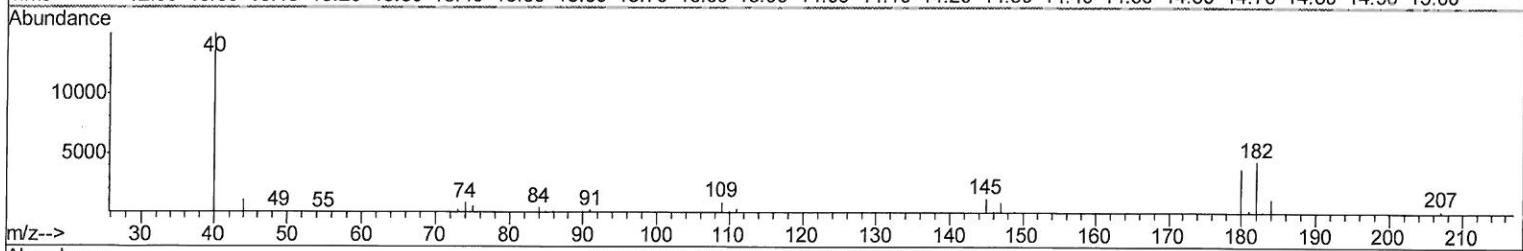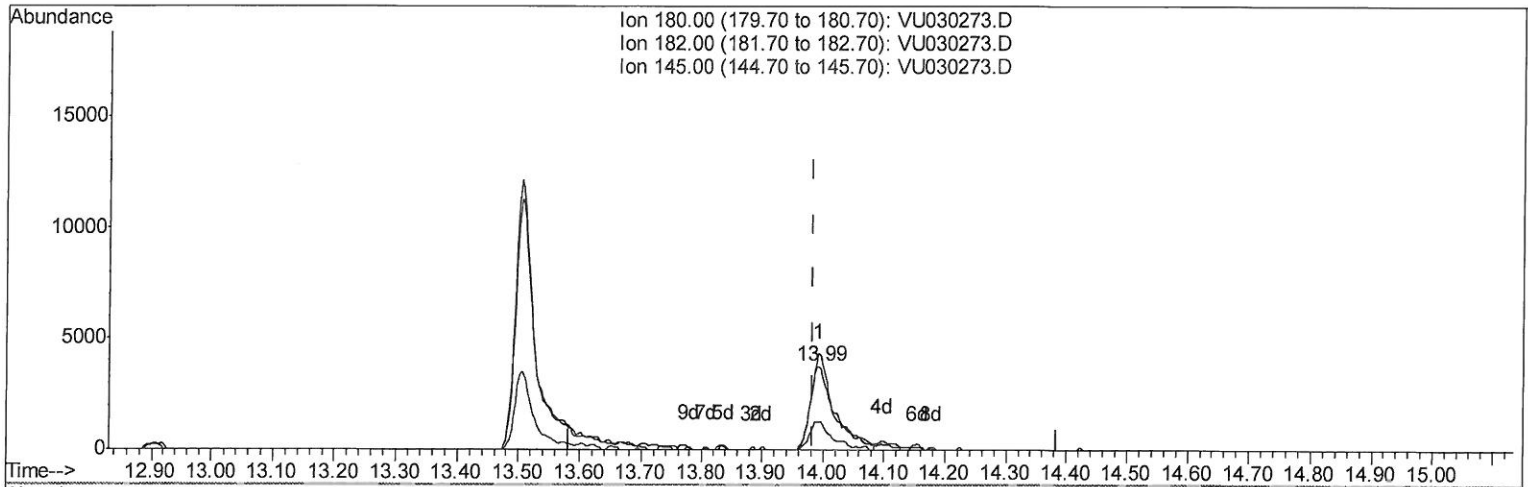

TIC: VU030273.D

(70) 1,2,3-Trichlorobenzene (T)

13.993min (+0.010) 1.91ug/L m

response 10798

Ion	Exp%	Act%
180.00	100	100
182.00	94.90	103.82
145.00	30.10	13.19#
0.00	0.00	0.00

7 MD
3/27/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Quantitation Report (QT Reviewed)

Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09A7DL

Manual Integrations
APPROVED

MMDadoda
3/22/2019 1:07:24 PM

Quant Time: Mar 22 05:38:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 05:14:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	534905	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	524923	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	245640	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	174947	48.37	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.74%
7) Chloroethane-d5	1.68	69	141145	48.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.27	63	233876	35.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.88%
21) 2-Butanone-d5	4.17	46	224744	83.76	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.76%
24) Chloroform-d	4.65	84	297887	44.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.76%
26) 1,2-Dichloroethane-d4	5.31	65	175350	46.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.62%
32) Benzene-d6	5.34	84	649642	46.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.92%
36) 1,2-Dichloropropane-d6	6.33	67	197840	46.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.44%
41) Toluene-d8	7.56	98	586999	45.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.26%
43) trans-1,3-Dichloropropene-	7.85	79	88797	42.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.22%
47) 2-Hexanone-d5	8.31	63	184805	83.26	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	285223	43.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	237368	48.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.26%

Target Compounds

					Qvalue
33) Benzene	5.39	78	23715	1.566	ug/L 100
51) Chlorobenzene	9.12	112	65033	5.963	ug/L 98
62) 1,3-Dichlorobenzene	11.42	146	16333	2.084	ug/L 98
63) 1,4-Dichlorobenzene	11.50	146	140832	17.324	ug/L 99
65) 1,2-Dichlorobenzene	11.87	146	436561	54.522	ug/L 97
68) 1,2,4-trichlorobenzene	13.50	180	28533m	5.268	ug/L
70) 1,2,3-Trichlorobenzene	13.99	180	10798m	1.911	ug/L

mmd
3/27/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed