

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030252.D
 Acq On : 21 Mar 2019 10:00
 Operator : JC/SP
 Sample : VU0321MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	11835	11913	0.65%	0.081%
2	1.399	89	96	109	rBV	266170	267058	14.68%	1.807%
3	1.679	175	183	197	rBV	199453	251773	13.84%	1.703%
4	2.270	357	367	380	rBV	436272	655077	36.01%	4.432%
5	2.601	467	470	472	rBV	1351	827	0.05%	0.006%
6	2.785	524	527	530	rVB2	1124	789	0.04%	0.005%
7	2.868	551	553	557	rVB	2159	1486	0.08%	0.010%
8	2.974	583	586	590	rBV3	1021	876	0.05%	0.006%
9	3.064	610	614	618	rBV	1479	1463	0.08%	0.010%
10	3.177	645	649	651	rBV	1241	937	0.05%	0.006%
11	3.190	651	653	657	rVV	1173	799	0.04%	0.005%
12	3.235	663	667	670	rBV	1401	1329	0.07%	0.009%
13	3.277	677	680	684	rVB	1158	898	0.05%	0.006%
14	3.360	702	706	712	rVB2	1555	1605	0.09%	0.011%
15	3.521	751	756	760	rBV	1956	1692	0.09%	0.011%
16	3.550	760	765	767	rBV	1418	1057	0.06%	0.007%
17	3.646	791	795	798	rBV	857	797	0.04%	0.005%
18	3.682	802	806	808	rBV	1228	1018	0.06%	0.007%
19	3.749	824	827	832	rVB	1525	1278	0.07%	0.009%
20	3.791	837	840	844	rVB	1416	1085	0.06%	0.007%
21	3.836	851	854	859	rVB	1342	876	0.05%	0.006%
22	3.875	863	866	873	rVB	2429	2586	0.14%	0.017%
23	3.916	873	879	881	rBV	1597	1540	0.08%	0.010%
24	3.997	900	904	908	rVB	1540	1115	0.06%	0.008%
25	4.174	947	959	979	rBV	166213	422686	23.23%	2.860%
26	4.379	1020	1023	1029	rBV	1241	1288	0.07%	0.009%
27	4.643	1085	1105	1130	rBV	299551	717826	39.46%	4.857%
28	4.785	1147	1149	1156	rVB	1641	1613	0.09%	0.011%
29	5.006	1215	1218	1223	rVB3	1179	889	0.05%	0.006%
30	5.132	1254	1257	1260	rVB	1103	768	0.04%	0.005%
31	5.170	1260	1269	1272	rBV2	2039	2258	0.12%	0.015%
32	5.196	1272	1277	1279	rBV2	1193	1114	0.06%	0.008%
33	5.248	1289	1293	1297	rBV2	1463	1515	0.08%	0.010%
34	5.334	1298	1320	1359	rVV3	617411	1819263	100.00%	12.309%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030252.D
 Acq On : 21 Mar 2019 10:00
 Operator : JC/SP
 Sample : VU0321MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	5.569	1389	1393	1399	rVB2	1449	1251	0.07%	0.008%
36	5.653	1416	1419	1422	rBV2	1517	1164	0.06%	0.008%
37	5.688	1427	1430	1434	rVB	2229	1828	0.10%	0.012%
38	5.727	1438	1442	1445	rBV	968	854	0.05%	0.006%
39	5.884	1474	1491	1535	rBV	572633	1173952	64.53%	7.943%
40	6.103	1556	1559	1564	rVB	1962	1581	0.09%	0.011%
41	6.132	1564	1568	1572	rBV	1569	1313	0.07%	0.009%
42	6.183	1577	1584	1587	rBV6	2235	3288	0.18%	0.022%
43	6.328	1615	1629	1653	rBV	393687	806759	44.35%	5.458%
44	6.482	1674	1677	1679	rBV2	1229	769	0.04%	0.005%
45	6.511	1683	1686	1690	rVB	1921	1290	0.07%	0.009%
46	6.572	1697	1705	1711	rBV	2080	2988	0.16%	0.020%
47	6.701	1740	1745	1747	rBV	1005	849	0.05%	0.006%
48	6.839	1785	1788	1792	rVB	1098	801	0.04%	0.005%
49	6.865	1792	1796	1800	rVB	1250	1036	0.06%	0.007%
50	6.891	1800	1804	1808	rBV	1429	1215	0.07%	0.008%
51	6.913	1808	1811	1820	rBV2	1185	1371	0.08%	0.009%
52	6.987	1829	1834	1835	rBV	1044	808	0.04%	0.005%
53	7.026	1842	1846	1848	rBV	2093	1320	0.07%	0.009%
54	7.148	1879	1884	1888	rVB2	829	748	0.04%	0.005%
55	7.225	1896	1908	1929	rBV	225891	419796	23.08%	2.840%
56	7.434	1970	1973	1977	rVB	1031	720	0.04%	0.005%
57	7.466	1977	1983	1991	rBV4	4363	7077	0.39%	0.048%
58	7.563	2000	2013	2049	rBV	840038	1513098	83.17%	10.237%
59	7.846	2090	2101	2123	rBV	155337	282794	15.54%	1.913%
60	8.009	2149	2152	2158	rVB	1880	1610	0.09%	0.011%
61	8.173	2199	2203	2209	rBV4	1718	2290	0.13%	0.015%
62	8.225	2215	2219	2223	rBV3	1788	1577	0.09%	0.011%
63	8.264	2229	2231	2234	rBV	1205	854	0.05%	0.006%
64	8.309	2234	2245	2282	rVV	553568	1022068	56.18%	6.915%
65	8.550	2316	2320	2325	rVB	2472	2042	0.11%	0.014%
66	8.588	2329	2332	2336	rVB	1557	1036	0.06%	0.007%
67	8.736	2375	2378	2382	rBV2	1063	914	0.05%	0.006%
68	8.781	2387	2392	2394	rBV	1662	1375	0.08%	0.009%
69	9.087	2473	2487	2509	rBV	843519	1432234	78.73%	9.690%
70	9.254	2536	2539	2547	rBV4	3187	4235	0.23%	0.029%
71	9.289	2547	2550	2553	rVB	1900	1091	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030252.D
 Acq On : 21 Mar 2019 10:00
 Operator : JC/SP
 Sample : VU0321MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	9.347	2565	2568	2572	rBV	1943	1780	0.10%	0.012%
73	9.379	2575	2578	2587	rVB2	2761	3630	0.20%	0.025%
74	9.447	2596	2599	2602	rBV	1503	1156	0.06%	0.008%
75	9.730	2683	2687	2691	rBV2	1424	1323	0.07%	0.009%
76	9.791	2699	2706	2707	rBV4	2495	2914	0.16%	0.020%
77	9.935	2746	2751	2755	rBV	2206	2626	0.14%	0.018%
78	10.164	2818	2822	2830	rVB3	3313	4694	0.26%	0.032%
79	10.427	2893	2904	2923	rBV	593618	966366	53.12%	6.538%
80	10.601	2956	2958	2961	rBV2	1795	997	0.05%	0.007%
81	10.688	2982	2985	2987	rBV	1348	787	0.04%	0.005%
82	10.775	3007	3012	3015	rBV	1826	2187	0.12%	0.015%
83	11.418	3201	3212	3220	rBV5	7513	14269	0.78%	0.097%
84	11.482	3220	3232	3259	rVV	839735	1393293	76.59%	9.427%
85	11.858	3334	3349	3373	rBV	817184	1391665	76.50%	9.416%
86	12.742	3621	3624	3627	rBV	1299	901	0.05%	0.006%
87	12.894	3662	3671	3678	rBV6	6267	11354	0.62%	0.077%
88	12.967	3691	3694	3696	rBV2	1342	826	0.05%	0.006%
89	13.270	3785	3788	3794	rVB	1829	1641	0.09%	0.011%
90	13.302	3794	3798	3802	rBV	1787	1596	0.09%	0.011%
91	13.511	3854	3863	3875	rBV5	13840	26532	1.46%	0.180%
92	13.752	3929	3938	3961	rBV	15857	43352	2.38%	0.293%
93	13.926	3989	3992	3997	rBV	1903	1367	0.08%	0.009%
94	13.996	4006	4014	4026	rBV5	8688	19107	1.05%	0.129%
95	14.164	4063	4066	4071	rBV	1554	1289	0.07%	0.009%
96	14.427	4145	4148	4151	rVB	1584	917	0.05%	0.006%
97	14.614	4203	4206	4208	rBV2	1362	1015	0.06%	0.007%
98	14.765	4251	4253	4257	rBV	1373	1157	0.06%	0.008%
99	15.131	4364	4367	4368	rBV	1493	925	0.05%	0.006%
100	16.032	4643	4647	4650	rBV3	1828	1768	0.10%	0.012%


Sum of corrected areas: 14780524

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030252.D
Acq On : 21 Mar 2019 10:00
Operator : JC/SP
Sample : VU0321MBL01
Misc : 5.00µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VBLK44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

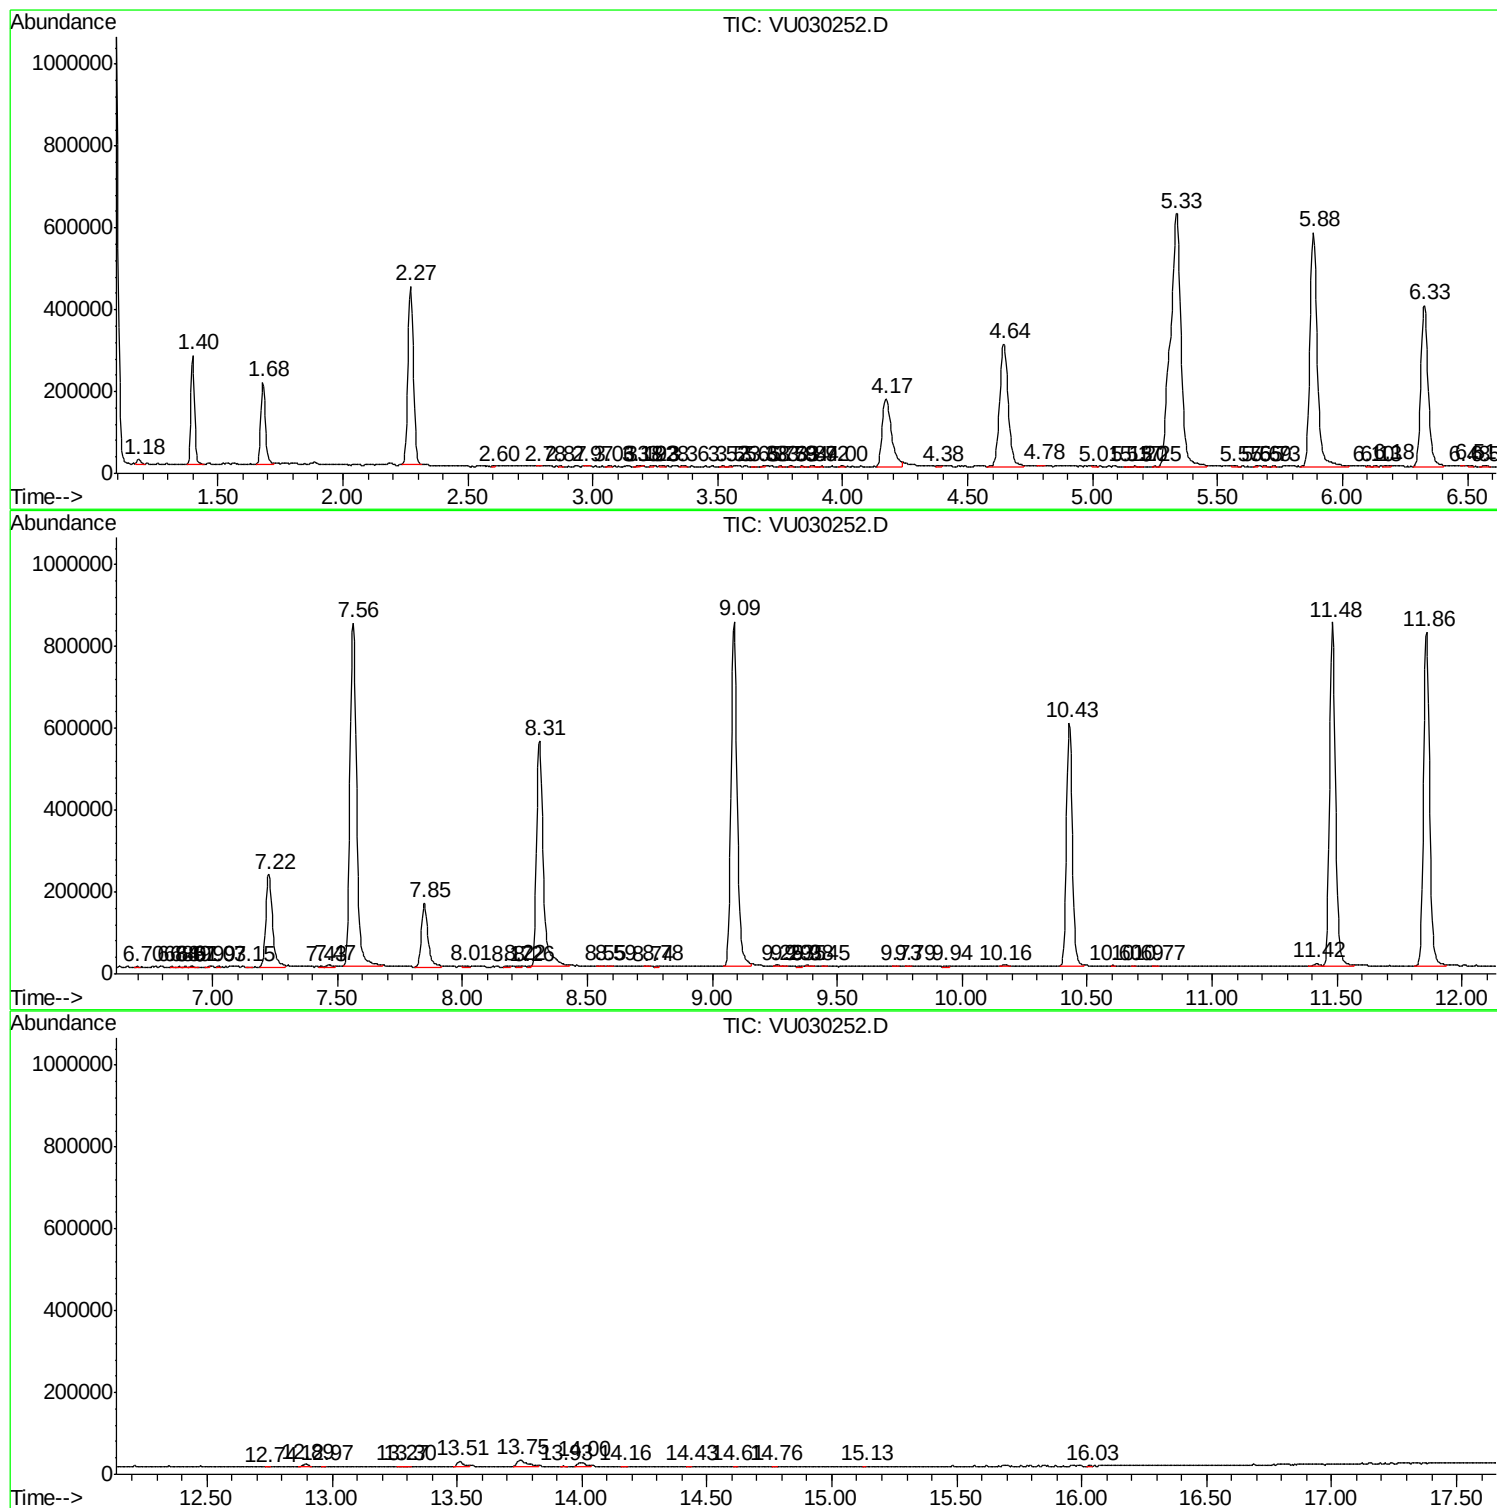

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030252.D
Acq On : 21 Mar 2019 10:00
Operator : JC/SP
Sample : VU0321MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030252.D
Acq On : 21 Mar 2019 10:00
Operator : JC/SP
Sample : VU0321MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc