

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030253.D
 Acq On : 21 Mar 2019 10:23
 Operator : JC/SP
 Sample : VU0321WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB3	11783	11899	0.66%	0.082%
2	1.399	89	96	106	rBV	262654	256535	14.14%	1.772%
3	1.678	175	183	196	rBV	189631	242339	13.36%	1.674%
4	2.273	357	368	383	rBV	416267	632453	34.86%	4.370%
5	2.463	423	427	428	rBV2	1716	1281	0.07%	0.009%
6	2.842	538	545	548	rBV	1995	2690	0.15%	0.019%
7	2.945	574	577	578	rBV	1359	884	0.05%	0.006%
8	3.048	604	609	610	rBV	1308	1187	0.07%	0.008%
9	3.116	625	630	635	rBV	1428	2273	0.13%	0.016%
10	3.260	672	675	677	rBV	1653	1110	0.06%	0.008%
11	3.305	681	689	691	rBV	1536	2077	0.11%	0.014%
12	3.540	758	762	765	rVB2	1571	1423	0.08%	0.010%
13	3.559	765	768	773	rVB	1187	909	0.05%	0.006%
14	3.707	809	814	815	rBV	1637	1442	0.08%	0.010%
15	3.752	824	828	832	rBV2	1264	1189	0.07%	0.008%
16	3.913	876	878	884	rVB	1526	1313	0.07%	0.009%
17	4.071	924	927	930	rBV	1456	1221	0.07%	0.008%
18	4.174	946	959	991	rBV	168590	453068	24.97%	3.130%
19	4.646	1091	1106	1137	rVB	287114	687779	37.91%	4.752%
20	4.990	1208	1213	1216	rBV	1922	2083	0.11%	0.014%
21	5.042	1226	1229	1237	rVB2	1640	1573	0.09%	0.011%
22	5.087	1237	1243	1244	rBV	1828	1804	0.10%	0.012%
23	5.225	1283	1286	1289	rBV	1268	980	0.05%	0.007%
24	5.337	1297	1321	1354	rBV2	612589	1814217	100.00%	12.535%
25	5.537	1380	1383	1387	rBV2	1203	1158	0.06%	0.008%
26	5.765	1450	1454	1460	rVB2	1808	2041	0.11%	0.014%
27	5.884	1477	1491	1519	rBV	550138	1121093	61.79%	7.746%
28	6.222	1592	1596	1598	rBV2	1263	1013	0.06%	0.007%
29	6.328	1614	1629	1662	rBV	390590	806186	44.44%	5.570%
30	6.794	1770	1774	1779	rBV	1645	1503	0.08%	0.010%
31	6.820	1779	1782	1787	rVB	1731	1428	0.08%	0.010%
32	6.958	1822	1825	1827	rBV2	1157	894	0.05%	0.006%
33	7.035	1845	1849	1855	rBV	935	984	0.05%	0.007%
34	7.225	1895	1908	1936	rBV	220792	414676	22.86%	2.865%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030253.D
 Acq On : 21 Mar 2019 10:23
 Operator : JC/SP
 Sample : VU0321WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.463	1979	1982	1985	rBV2	1607	1105	0.06%	0.008%
36	7.562	2000	2013	2046	rBV	825237	1488281	82.03%	10.283%
37	7.849	2089	2102	2128	rBV	154758	284363	15.67%	1.965%
38	7.942	2128	2131	2135	rVV	1163	1046	0.06%	0.007%
39	7.993	2144	2147	2150	rVB2	1498	858	0.05%	0.006%
40	8.038	2157	2161	2163	rBV3	1575	1321	0.07%	0.009%
41	8.151	2193	2196	2198	rBV	1341	887	0.05%	0.006%
42	8.167	2198	2201	2204	rVV2	1531	1360	0.07%	0.009%
43	8.247	2222	2226	2229	rBV	1466	1189	0.07%	0.008%
44	8.308	2234	2245	2275	rBV	569008	1022333	56.35%	7.063%
45	8.463	2290	2293	2299	rVB3	1751	1465	0.08%	0.010%
46	8.588	2330	2332	2342	rVB	1656	1636	0.09%	0.011%
47	8.630	2342	2345	2350	rVB	1711	1188	0.07%	0.008%
48	8.662	2351	2355	2359	rBV	1056	1187	0.07%	0.008%
49	8.804	2395	2399	2402	rBV	1492	1046	0.06%	0.007%
50	8.971	2447	2451	2453	rBV	1565	1134	0.06%	0.008%
51	9.016	2461	2465	2467	rBV	1241	877	0.05%	0.006%
52	9.035	2468	2471	2475	rVB	2001	1619	0.09%	0.011%
53	9.087	2475	2487	2513	rBV	823253	1405586	77.48%	9.711%
54	9.299	2550	2553	2557	rVB	1464	1082	0.06%	0.007%
55	9.334	2557	2564	2569	rBV4	1392	1829	0.10%	0.013%
56	9.408	2584	2587	2591	rVB	1737	1489	0.08%	0.010%
57	9.437	2591	2596	2598	rBV2	1243	1062	0.06%	0.007%
58	9.521	2619	2622	2629	rVB2	997	937	0.05%	0.006%
59	9.710	2677	2681	2684	rBV	1545	1231	0.07%	0.009%
60	9.781	2698	2703	2706	rVB2	1204	1048	0.06%	0.007%
61	9.816	2706	2714	2716	rBV3	1523	1740	0.10%	0.012%
62	9.861	2724	2728	2731	rBV	1317	1045	0.06%	0.007%
63	9.923	2741	2747	2750	rVB2	1663	1690	0.09%	0.012%
64	10.000	2766	2771	2775	rBV2	1427	1239	0.07%	0.009%
65	10.099	2798	2802	2805	rVV	1340	1065	0.06%	0.007%
66	10.177	2821	2826	2832	rVB2	1497	1651	0.09%	0.011%
67	10.215	2832	2838	2842	rBV	1438	1556	0.09%	0.011%
68	10.267	2852	2854	2859	rVB2	1438	1051	0.06%	0.007%
69	10.305	2862	2866	2869	rBV	1387	1302	0.07%	0.009%
70	10.347	2875	2879	2882	rBV	1343	1258	0.07%	0.009%
71	10.427	2889	2904	2929	rBV	613993	993153	54.74%	6.862%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030253.D
 Acq On : 21 Mar 2019 10:23
 Operator : JC/SP
 Sample : VU0321WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.604	2949	2959	2961	rBV3	2651	3777	0.21%	0.026%
73	10.768	3007	3010	3014	rVB	1844	1005	0.06%	0.007%
74	10.800	3018	3020	3024	rBV	1351	974	0.05%	0.007%
75	10.842	3030	3033	3036	rBV	1891	1381	0.08%	0.010%
76	10.884	3043	3046	3048	rBV2	1673	1103	0.06%	0.008%
77	10.919	3054	3057	3061	rBV	1485	1415	0.08%	0.010%
78	11.202	3142	3145	3153	rVB	902	1247	0.07%	0.009%
79	11.360	3188	3194	3196	rBV2	804	897	0.05%	0.006%
80	11.418	3206	3212	3219	rVB6	3512	4887	0.27%	0.034%
81	11.482	3219	3232	3255	rBV	805189	1344223	74.09%	9.287%
82	11.858	3335	3349	3376	rBV	809401	1376401	75.87%	9.510%
83	12.266	3472	3476	3478	rBV	1191	947	0.05%	0.007%
84	12.418	3519	3523	3529	rVB2	1550	1360	0.07%	0.009%
85	12.559	3564	3567	3570	rBV	1238	939	0.05%	0.006%
86	13.090	3725	3732	3736	rBV	2601	3058	0.17%	0.021%
87	13.131	3742	3745	3748	rBV2	1231	916	0.05%	0.006%
88	13.260	3782	3785	3790	rBV	1698	1767	0.10%	0.012%
89	13.514	3861	3864	3866	rBV3	2431	1824	0.10%	0.013%
90	13.768	3935	3943	3945	rBV4	2811	3937	0.22%	0.027%
91	14.070	4034	4037	4041	rBV	1286	1387	0.08%	0.010%
92	14.254	4091	4094	4097	rBV	1569	1022	0.06%	0.007%
93	14.453	4153	4156	4159	rBV2	1397	881	0.05%	0.006%
94	14.485	4163	4166	4170	rVV	1559	1350	0.07%	0.009%
95	14.524	4174	4178	4182	rBV	1746	1780	0.10%	0.012%
96	14.684	4225	4228	4233	rBV	1852	1898	0.10%	0.013%
97	14.993	4321	4324	4326	rBV2	1521	985	0.05%	0.007%
98	15.118	4360	4363	4368	rBV	1120	943	0.05%	0.007%
99	15.662	4529	4532	4535	rBV	1481	1208	0.07%	0.008%
100	15.745	4555	4558	4561	rBV	1752	1485	0.08%	0.010%


Sum of corrected areas: 14473611

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030253.D
Acq On : 21 Mar 2019 10:23
Operator : JC/SP
Sample : VU0321WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

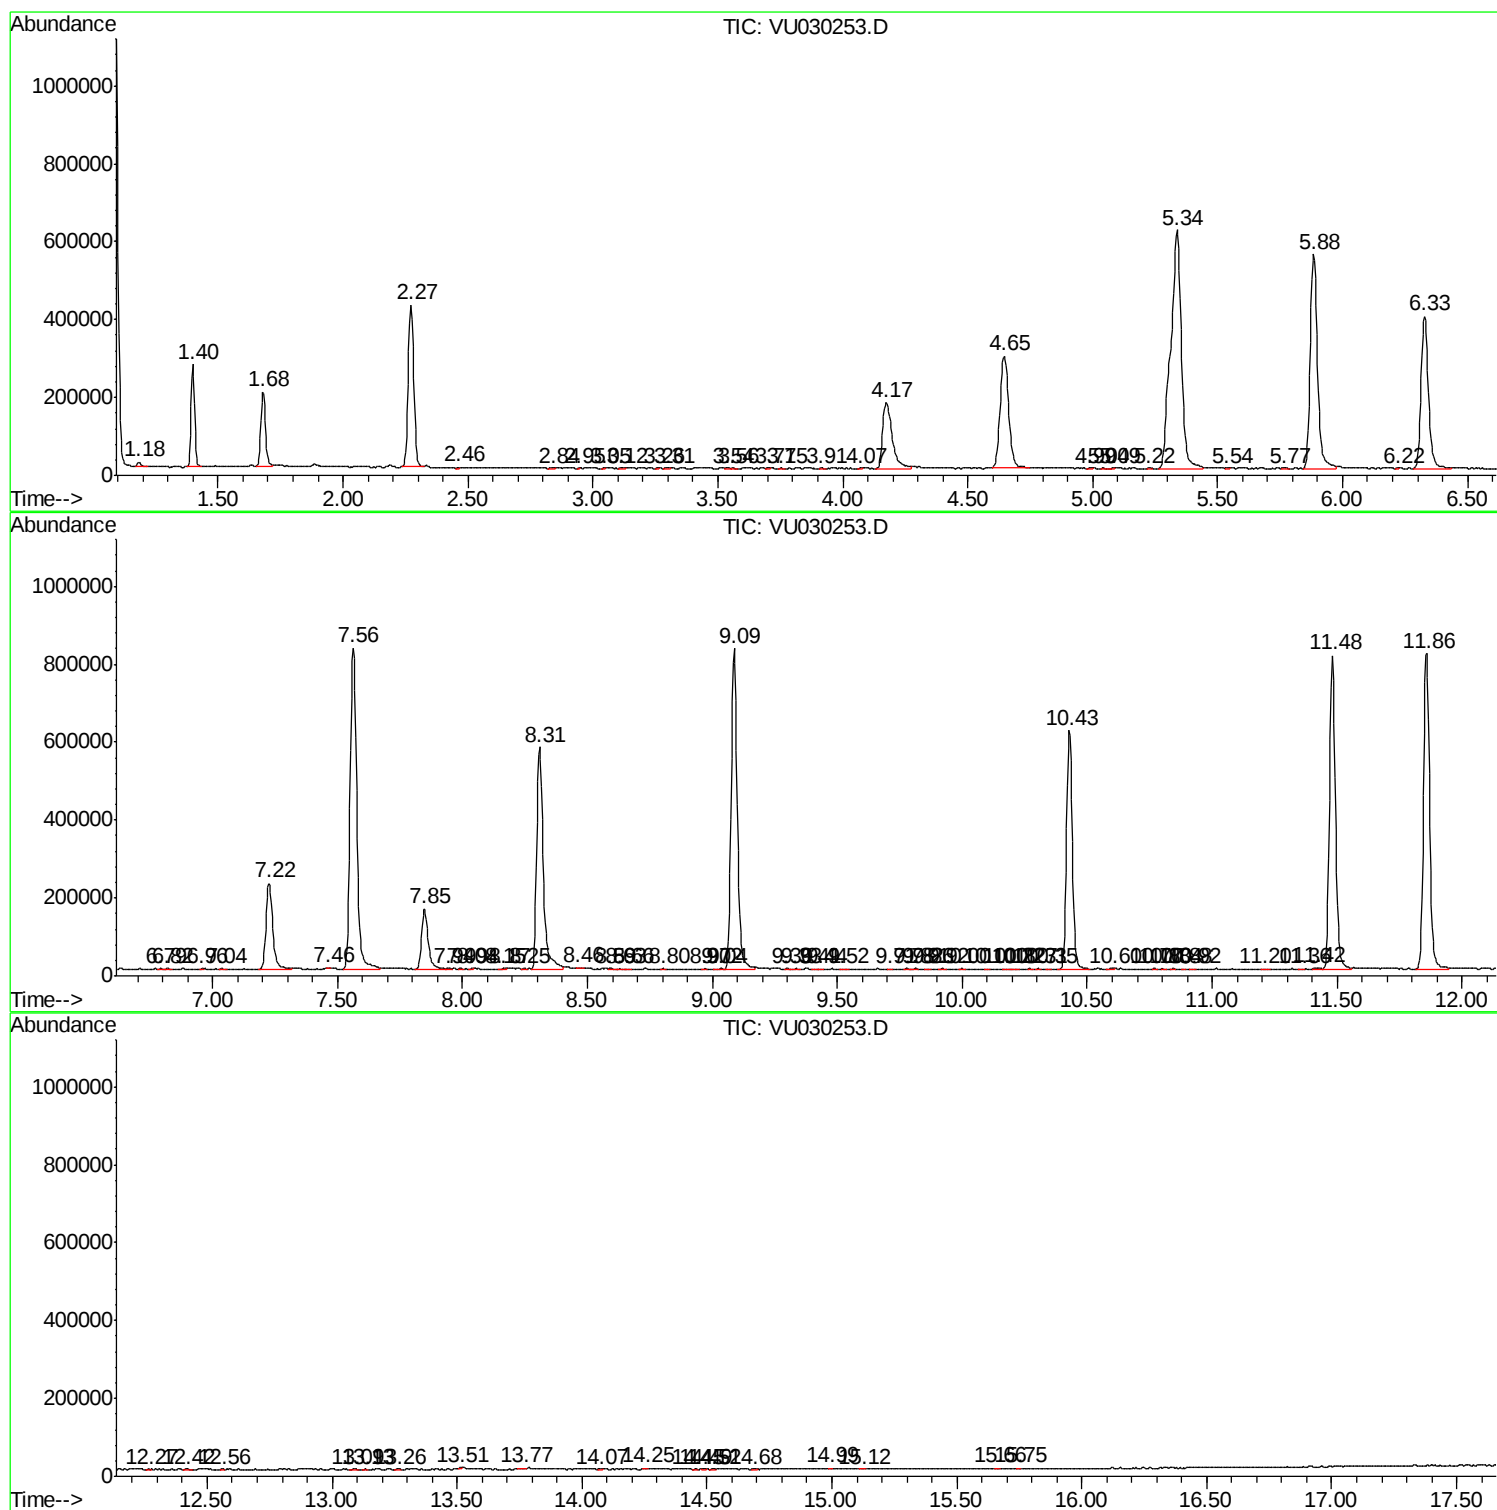

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030253.D
Acq On : 21 Mar 2019 10:23
Operator : JC/SP
Sample : VU0321WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030253.D
Acq On : 21 Mar 2019 10:23
Operator : JC/SP
Sample : VU0321WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc