

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030269.D
 Acq On : 21 Mar 2019 16:40
 Operator : JC/SP
 Sample : VU0321WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB2	11277	10428	0.59%	0.074%
2	1.399	89	96	107	rBV	247888	247163	14.03%	1.755%
3	1.559	143	146	149	rBV4	2830	2013	0.11%	0.014%
4	1.678	175	183	201	rBV	183778	236760	13.44%	1.681%
5	2.006	282	285	288	rBV	2188	1543	0.09%	0.011%
6	2.270	356	367	381	rBV	399803	612057	34.74%	4.346%
7	2.591	464	467	473	rVB	1781	1411	0.08%	0.010%
8	2.688	494	497	500	rBV2	1091	991	0.06%	0.007%
9	2.984	585	589	594	rBV3	1458	1719	0.10%	0.012%
10	3.042	603	607	610	rBV	1525	1072	0.06%	0.008%
11	3.077	615	618	624	rBV	1724	1812	0.10%	0.013%
12	3.444	729	732	738	rBV2	1107	1017	0.06%	0.007%
13	3.559	765	768	773	rVB	1337	1145	0.06%	0.008%
14	3.591	773	778	779	rBV	1463	1436	0.08%	0.010%
15	3.636	788	792	799	rVB	1785	2526	0.14%	0.018%
16	3.672	799	803	805	rBV	1379	1102	0.06%	0.008%
17	4.093	929	934	938	rBV	1890	1478	0.08%	0.010%
18	4.116	938	941	945	rBV	1152	1217	0.07%	0.009%
19	4.173	948	959	984	rBV	161237	418737	23.76%	2.973%
20	4.514	1062	1065	1069	rVB	1339	838	0.05%	0.006%
21	4.562	1077	1080	1083	rBV	1221	953	0.05%	0.007%
22	4.646	1088	1106	1128	rBV	285958	685330	38.89%	4.866%
23	4.797	1148	1153	1156	rVB2	1994	1854	0.11%	0.013%
24	4.878	1173	1178	1180	rBV3	1732	1576	0.09%	0.011%
25	4.974	1199	1208	1212	rBV3	2211	2698	0.15%	0.019%
26	5.035	1223	1227	1233	rVB2	1105	1188	0.07%	0.008%
27	5.103	1244	1248	1253	rBV	880	883	0.05%	0.006%
28	5.247	1286	1293	1296	rBV2	931	1006	0.06%	0.007%
29	5.337	1296	1321	1355	rBV2	597944	1762012	100.00%	12.512%
30	5.607	1402	1405	1416	rVB	1598	2134	0.12%	0.015%
31	5.884	1476	1491	1516	rBV	550669	1106168	62.78%	7.855%
32	6.077	1548	1551	1555	rVB	1572	1194	0.07%	0.008%
33	6.148	1570	1573	1576	rBV2	1178	977	0.06%	0.007%
34	6.180	1580	1583	1585	rBV2	1378	823	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030269.D
 Acq On : 21 Mar 2019 16:40
 Operator : JC/SP
 Sample : VU0321WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1614	1629	1656	rBV	381638	785303	44.57%	5.576%
36	6.524	1688	1690	1698	rVB2	1397	1271	0.07%	0.009%
37	6.566	1698	1703	1708	rBV2	994	1144	0.06%	0.008%
38	6.807	1775	1778	1782	rBV	1354	1013	0.06%	0.007%
39	6.890	1802	1804	1810	rVB2	1809	1306	0.07%	0.009%
40	6.987	1828	1834	1836	rBV	1137	1006	0.06%	0.007%
41	7.032	1845	1848	1851	rVB	1555	922	0.05%	0.007%
42	7.115	1869	1874	1877	rBV2	1483	1404	0.08%	0.010%
43	7.141	1877	1882	1884	rBV2	1209	1252	0.07%	0.009%
44	7.225	1897	1908	1931	rVV	215420	398596	22.62%	2.830%
45	7.456	1974	1980	1981	rBV	1938	1437	0.08%	0.010%
46	7.562	2000	2013	2033	rBV	796739	1423204	80.77%	10.106%
47	7.848	2090	2102	2133	rBV	148560	270707	15.36%	1.922%
48	8.148	2189	2195	2200	rBV	1582	2399	0.14%	0.017%
49	8.176	2201	2204	2207	rBV3	1688	1272	0.07%	0.009%
50	8.228	2215	2220	2226	rVB4	4251	5363	0.30%	0.038%
51	8.308	2234	2245	2284	rBV	539445	992292	56.32%	7.046%
52	8.910	2426	2432	2433	rBV	1275	1115	0.06%	0.008%
53	8.948	2439	2444	2447	rBV	1383	1469	0.08%	0.010%
54	9.086	2475	2487	2515	rBV	790533	1375010	78.04%	9.764%
55	9.334	2561	2564	2567	rBV	1441	1100	0.06%	0.008%
56	9.479	2604	2609	2612	rBV	1084	1022	0.06%	0.007%
57	9.778	2699	2702	2704	rVV	1345	1063	0.06%	0.008%
58	9.800	2706	2709	2713	rVV2	2760	2578	0.15%	0.018%
59	9.819	2713	2715	2719	rVB2	1379	869	0.05%	0.006%
60	9.858	2724	2727	2731	rVB	1425	986	0.06%	0.007%
61	9.897	2734	2739	2742	rVB2	1315	1346	0.08%	0.010%
62	10.186	2826	2829	2836	rVB	1718	1991	0.11%	0.014%
63	10.273	2850	2856	2858	rBV	1692	1507	0.09%	0.011%
64	10.427	2892	2904	2924	rBV	595464	961130	54.55%	6.825%
65	10.572	2944	2949	2953	rBV	1241	1324	0.08%	0.009%
66	10.607	2957	2960	2969	rVB5	2858	3228	0.18%	0.023%
67	10.717	2991	2994	2997	rBV	1130	992	0.06%	0.007%
68	10.768	3007	3010	3016	rVV3	1142	1082	0.06%	0.008%
69	10.848	3029	3035	3039	rVB	1378	1366	0.08%	0.010%
70	10.871	3039	3042	3047	rBV	1238	1280	0.07%	0.009%
71	10.954	3064	3068	3072	rBV	1311	1300	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030269.D
 Acq On : 21 Mar 2019 16:40
 Operator : JC/SP
 Sample : VU0321WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.244	3155	3158	3162	rVB	1914	1341	0.08%	0.010%
73	11.270	3162	3166	3167	rBV	1308	883	0.05%	0.006%
74	11.421	3202	3213	3220	rBV6	4026	6782	0.38%	0.048%
75	11.482	3220	3232	3254	rBV	793400	1315863	74.68%	9.344%
76	11.762	3316	3319	3321	rBV	1187	829	0.05%	0.006%
77	11.858	3337	3349	3375	rBV	799504	1346657	76.43%	9.562%
78	12.144	3431	3438	3442	rBV2	1174	1754	0.10%	0.012%
79	12.392	3510	3515	3519	rVB	1565	1738	0.10%	0.012%
80	12.430	3519	3527	3533	rBV2	2105	3381	0.19%	0.024%
81	12.475	3537	3541	3543	rBV3	1665	1462	0.08%	0.010%
82	12.819	3641	3648	3650	rBV2	1280	1487	0.08%	0.011%
83	13.112	3732	3739	3742	rBV	1768	2153	0.12%	0.015%
84	13.160	3748	3754	3757	rBV2	1105	1364	0.08%	0.010%
85	13.308	3797	3800	3803	rVB2	1831	1161	0.07%	0.008%
86	13.331	3803	3807	3810	rBV	1069	1056	0.06%	0.007%
87	13.401	3826	3829	3834	rVB2	1523	1140	0.06%	0.008%
88	13.514	3861	3864	3870	rBV4	1631	2223	0.13%	0.016%
89	13.765	3937	3942	3946	rBV3	4028	5090	0.29%	0.036%
90	14.003	4008	4016	4022	rBV4	3562	5593	0.32%	0.040%
91	14.257	4091	4095	4097	rBV	1656	1254	0.07%	0.009%
92	14.269	4097	4099	4102	rVV2	1328	876	0.05%	0.006%
93	14.337	4117	4120	4126	rBV2	907	880	0.05%	0.006%
94	14.662	4216	4221	4223	rBV	1919	1702	0.10%	0.012%
95	14.736	4239	4244	4247	rVB	1532	1461	0.08%	0.010%
96	14.761	4247	4252	4254	rBV2	910	902	0.05%	0.006%
97	15.028	4331	4335	4340	rBV	1814	1862	0.11%	0.013%
98	15.247	4398	4403	4406	rBV	2767	2695	0.15%	0.019%
99	15.366	4437	4440	4442	rBV2	1996	1470	0.08%	0.010%
100	15.466	4469	4471	4474	rBV	1346	1048	0.06%	0.007%


Sum of corrected areas: 14083017

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030269.D
Acq On : 21 Mar 2019 16:40
Operator : JC/SP
Sample : VU0321WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

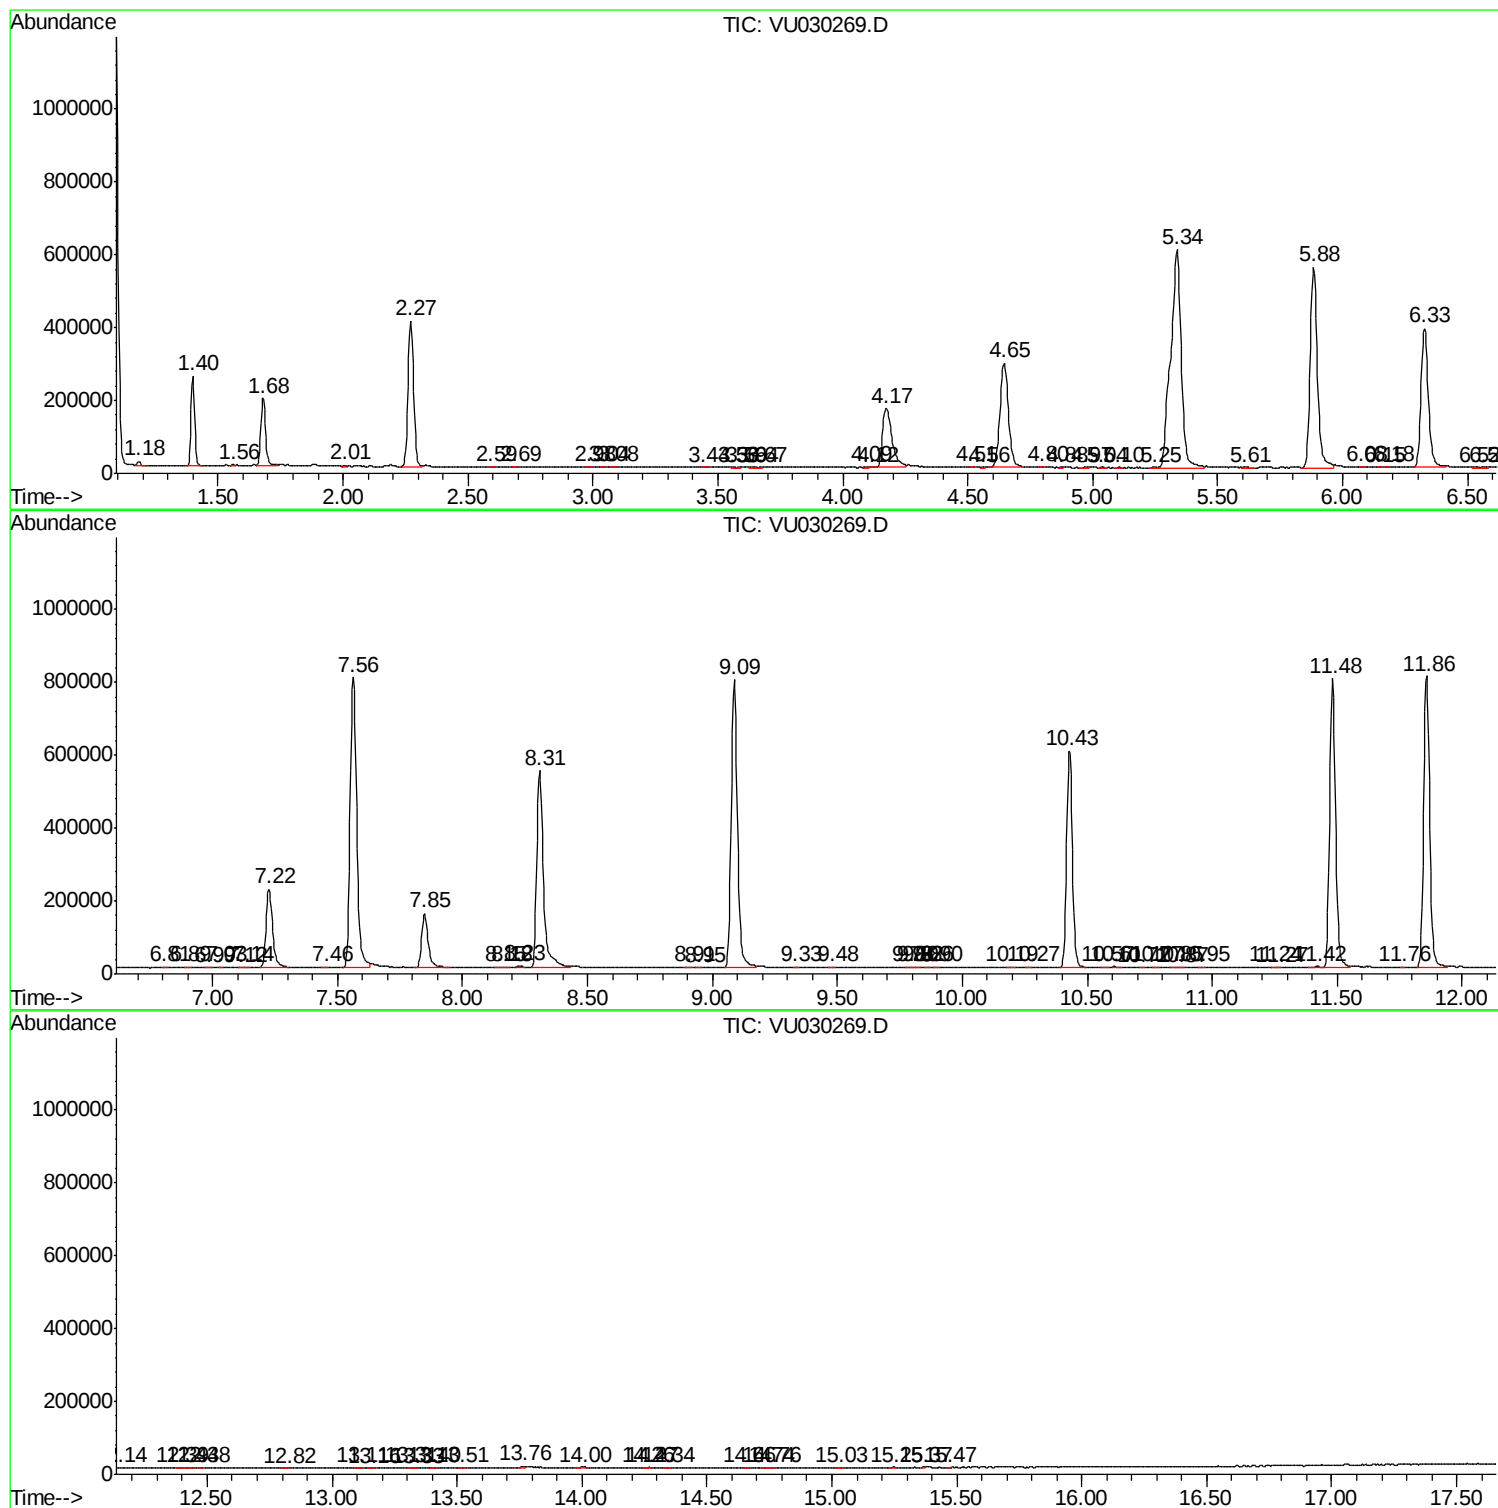

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030269.D
Acq On : 21 Mar 2019 16:40
Operator : JC/SP
Sample : VU0321WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030269.D
Acq On : 21 Mar 2019 16:40
Operator : JC/SP
Sample : VU0321WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK47

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc