

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030270.D
 Acq On : 21 Mar 2019 17:03
 Operator : JC/SP
 Sample : K2031-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	34	rVB	10244	8796	0.48%	0.060%
2	1.399	89	96	107	rBV	270592	271842	14.80%	1.859%
3	1.682	175	184	200	rBV	198097	253665	13.81%	1.734%
4	2.270	356	367	380	rBV	429729	660647	35.97%	4.517%
5	2.383	399	402	409	rVB	2220	2082	0.11%	0.014%
6	2.621	472	476	480	rBV2	1482	1269	0.07%	0.009%
7	2.775	520	524	526	rBV	1299	1033	0.06%	0.007%
8	2.836	540	543	546	rVB	2246	1494	0.08%	0.010%
9	3.112	624	629	632	rBV	1308	1368	0.07%	0.009%
10	3.302	683	688	691	rBV	1100	887	0.05%	0.006%
11	3.434	722	729	734	rVB	1545	2104	0.11%	0.014%
12	3.466	734	739	742	rBV2	1033	1148	0.06%	0.008%
13	3.508	749	752	757	rVB	1145	1081	0.06%	0.007%
14	3.617	781	786	790	rBV2	771	1096	0.06%	0.007%
15	3.717	812	817	819	rBV	1202	1106	0.06%	0.008%
16	3.881	864	868	872	rBV	1154	1233	0.07%	0.008%
17	3.952	886	890	893	rVB	1580	1245	0.07%	0.009%
18	3.981	893	899	902	rBV	1434	1781	0.10%	0.012%
19	4.055	917	922	924	rBV	1264	972	0.05%	0.007%
20	4.177	947	960	992	rBV	159187	430292	23.43%	2.942%
21	4.463	1045	1049	1057	rVB2	1632	1495	0.08%	0.010%
22	4.537	1069	1072	1076	rVB	1454	996	0.05%	0.007%
23	4.646	1085	1106	1132	rBV2	296714	717974	39.09%	4.909%
24	4.903	1184	1186	1192	rVB3	1513	1013	0.06%	0.007%
25	5.080	1238	1241	1249	rVB3	1149	1319	0.07%	0.009%
26	5.215	1279	1283	1286	rBV	1527	1181	0.06%	0.008%
27	5.247	1290	1293	1298	rVB	1514	1196	0.07%	0.008%
28	5.337	1298	1321	1354	rBV2	628616	1836836	100.00%	12.559%
29	5.518	1372	1377	1382	rVB	1975	2250	0.12%	0.015%
30	5.546	1382	1386	1391	rBV2	2063	2452	0.13%	0.017%
31	5.685	1424	1429	1434	rVB3	1318	1171	0.06%	0.008%
32	5.717	1434	1439	1444	rBV2	1309	1320	0.07%	0.009%
33	5.749	1444	1449	1455	rBV	1889	2308	0.13%	0.016%
34	5.884	1478	1491	1525	rVV	577422	1184597	64.49%	8.100%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030270.D
 Acq On : 21 Mar 2019 17:03
 Operator : JC/SP
 Sample : K2031-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1615	1629	1657	rBV	391978	804790	43.81%	5.503%
36	6.514	1683	1687	1690	rVB	1385	1054	0.06%	0.007%
37	6.604	1711	1715	1720	rBV	1364	1592	0.09%	0.011%
38	7.042	1848	1851	1857	rVB	1496	1344	0.07%	0.009%
39	7.074	1857	1861	1868	rBV2	1399	2088	0.11%	0.014%
40	7.225	1896	1908	1937	rBV	223012	416227	22.66%	2.846%
41	7.562	2001	2013	2035	rBV	824421	1486919	80.95%	10.167%
42	7.849	2091	2102	2124	rBV	153600	274949	14.97%	1.880%
43	8.029	2154	2158	2162	rBV	989	1055	0.06%	0.007%
44	8.122	2183	2187	2192	rBV3	895	1054	0.06%	0.007%
45	8.177	2195	2204	2212	rVV2	9573	16945	0.92%	0.116%
46	8.228	2216	2220	2226	rVB5	4242	4828	0.26%	0.033%
47	8.308	2234	2245	2277	rBV	536566	979019	53.30%	6.694%
48	8.620	2340	2342	2350	rVB	1355	1080	0.06%	0.007%
49	8.678	2355	2360	2363	rVB2	1506	1390	0.08%	0.010%
50	8.842	2407	2411	2416	rBV	1670	1733	0.09%	0.012%
51	9.029	2461	2469	2472	rBV	1464	1741	0.09%	0.012%
52	9.087	2474	2487	2508	rBV	841572	1436742	78.22%	9.824%
53	9.382	2574	2579	2585	rVV4	2221	2913	0.16%	0.020%
54	9.495	2611	2614	2620	rBV2	1085	951	0.05%	0.007%
55	9.681	2664	2672	2674	rBV2	1086	1198	0.07%	0.008%
56	9.755	2692	2695	2700	rBV2	979	972	0.05%	0.007%
57	9.791	2700	2706	2709	rBV4	1145	1453	0.08%	0.010%
58	9.942	2746	2753	2757	rBV	1466	2007	0.11%	0.014%
59	10.096	2798	2801	2806	rVB2	1134	1090	0.06%	0.007%
60	10.260	2849	2852	2855	rVB	1540	1007	0.05%	0.007%
61	10.283	2855	2859	2864	rBV3	1458	1694	0.09%	0.012%
62	10.427	2892	2904	2922	rBV	597425	970013	52.81%	6.632%
63	10.607	2951	2960	2966	rBV4	8798	12909	0.70%	0.088%
64	10.662	2974	2977	2981	rVV	1269	1025	0.06%	0.007%
65	10.685	2981	2984	2989	rVB2	1100	1027	0.06%	0.007%
66	10.942	3057	3064	3069	rVB2	1629	1764	0.10%	0.012%
67	11.012	3083	3086	3089	rBV	1321	971	0.05%	0.007%
68	11.115	3115	3118	3125	rVB	1581	1943	0.11%	0.013%
69	11.160	3125	3132	3133	rBV3	1267	1529	0.08%	0.010%
70	11.189	3138	3141	3144	rVV	2215	1630	0.09%	0.011%
71	11.212	3144	3148	3154	rVB	1265	1326	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030270.D
 Acq On : 21 Mar 2019 17:03
 Operator : JC/SP
 Sample : K2031-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.270	3161	3166	3167	rBV	1417	1274	0.07%	0.009%
73	11.324	3178	3183	3186	rBV2	1650	1707	0.09%	0.012%
74	11.411	3207	3210	3215	rVV4	1032	908	0.05%	0.006%
75	11.482	3220	3232	3257	rBV	831475	1377125	74.97%	9.416%
76	11.858	3336	3349	3377	rBV	812598	1363599	74.24%	9.324%
77	12.209	3455	3458	3463	rVB2	1072	974	0.05%	0.007%
78	12.250	3463	3471	3475	rVB2	2040	3084	0.17%	0.021%
79	12.276	3475	3479	3482	rBV	1512	1051	0.06%	0.007%
80	12.475	3538	3541	3549	rVB3	2244	2693	0.15%	0.018%
81	12.514	3549	3553	3560	rVB2	1631	2036	0.11%	0.014%
82	12.556	3560	3566	3568	rBV	1299	1436	0.08%	0.010%
83	12.826	3646	3650	3653	rBV	1102	930	0.05%	0.006%
84	12.877	3663	3666	3668	rBV	1471	902	0.05%	0.006%
85	12.951	3682	3689	3692	rVB	2158	2336	0.13%	0.016%
86	12.974	3692	3696	3698	rBV2	1535	1123	0.06%	0.008%
87	13.180	3758	3760	3767	rVV2	897	1010	0.05%	0.007%
88	13.231	3767	3776	3780	rVV2	1165	1775	0.10%	0.012%
89	13.514	3857	3864	3866	rBV3	2833	3178	0.17%	0.022%
90	13.864	3967	3973	3981	rBV2	1357	2068	0.11%	0.014%
91	13.996	4011	4014	4016	rBV2	1453	1086	0.06%	0.007%
92	14.045	4025	4029	4032	rBV2	1090	938	0.05%	0.006%
93	14.141	4053	4059	4063	rVV2	2161	2260	0.12%	0.015%
94	14.189	4072	4074	4078	rVB	1480	1061	0.06%	0.007%
95	14.273	4096	4100	4102	rBV2	1687	1368	0.07%	0.009%
96	14.446	4151	4154	4158	rBV	1178	906	0.05%	0.006%
97	14.707	4232	4235	4240	rBV2	1425	1231	0.07%	0.008%
98	15.054	4339	4343	4346	rBV2	1709	1548	0.08%	0.011%
99	15.308	4419	4422	4426	rVB	2210	1551	0.08%	0.011%
100	15.437	4459	4462	4466	rBV3	1606	987	0.05%	0.007%


Sum of corrected areas: 14625366

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030270.D
Acq On : 21 Mar 2019 17:03
Operator : JC/SP
Sample : K2031-13
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

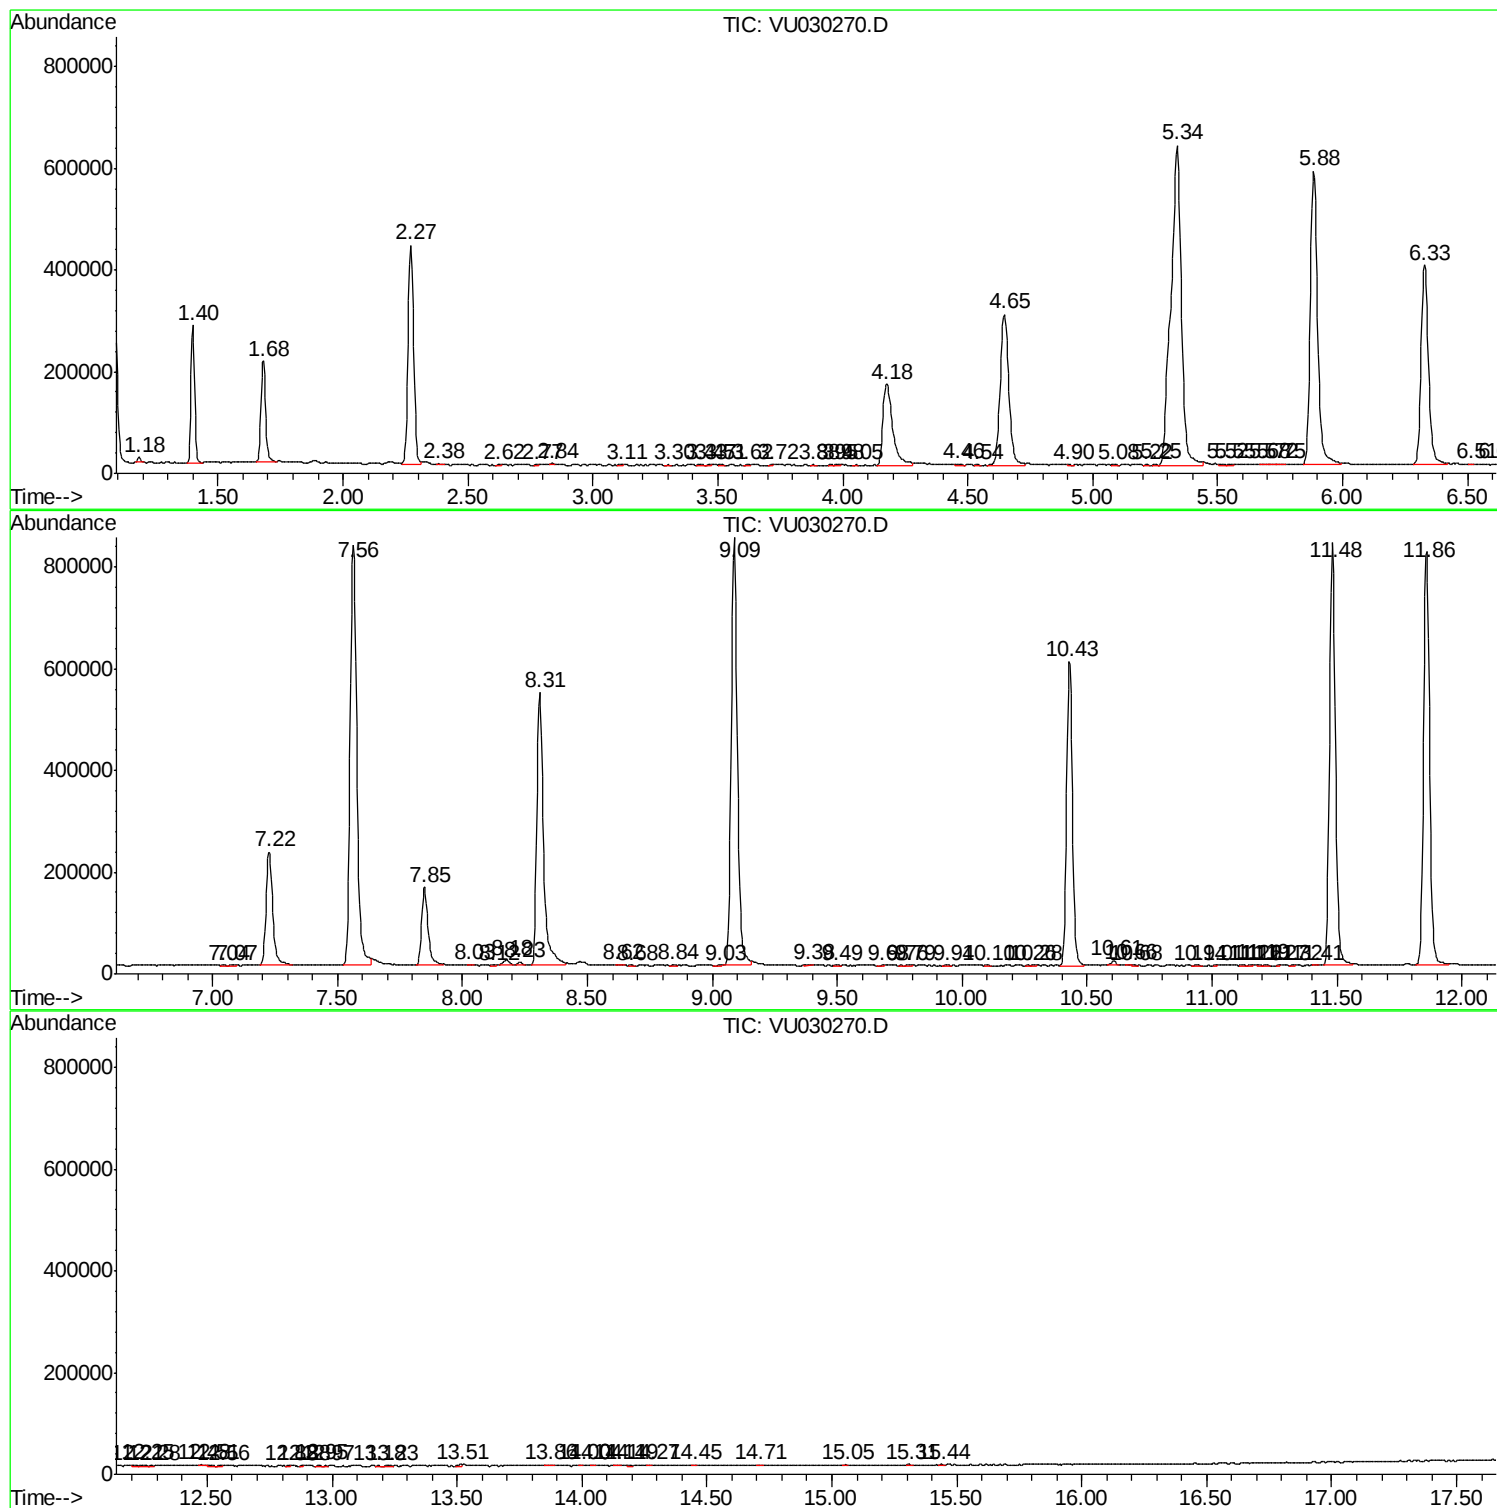

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030270.D
Acq On : 21 Mar 2019 17:03
Operator : JC/SP
Sample : K2031-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030270.D
Acq On : 21 Mar 2019 17:03
Operator : JC/SP
Sample : K2031-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc