

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030273.D
 Acq On : 21 Mar 2019 18:12
 Operator : JC/SP
 Sample : K2022-07DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	105	rBV	269006	269008	9.36%	1.646%
2	1.679	176	183	195	rVB	191149	237682	8.27%	1.454%
3	2.270	357	367	380	rBV	423663	644691	22.42%	3.944%
4	2.756	516	518	520	rBV	537	320	0.01%	0.002%
5	2.801	529	532	535	rVB	1733	1140	0.04%	0.007%
6	2.846	535	546	549	rBV2	1617	2913	0.10%	0.018%
7	2.952	577	579	582	rBV	732	363	0.01%	0.002%
8	3.019	597	600	602	rBV	1025	741	0.03%	0.005%
9	3.293	680	685	687	rBV2	1188	1071	0.04%	0.007%
10	3.370	705	709	712	rBV	1880	1485	0.05%	0.009%
11	3.489	742	746	749	rBV	1377	1304	0.05%	0.008%
12	3.910	874	877	879	rBV2	1155	704	0.02%	0.004%
13	3.952	886	890	892	rBV	1803	1583	0.06%	0.010%
14	4.174	948	959	983	rBV	141331	367563	12.78%	2.249%
15	4.646	1092	1106	1133	rBV	278225	653147	22.72%	3.996%
16	5.071	1235	1238	1241	rBV2	630	473	0.02%	0.003%
17	5.260	1294	1297	1298	rBV	1270	721	0.03%	0.004%
18	5.338	1299	1321	1351	rVV2	595732	1789859	62.25%	10.950%
19	5.620	1406	1409	1412	rBV	1178	949	0.03%	0.006%
20	5.723	1438	1441	1443	rBV2	1027	721	0.03%	0.004%
21	5.791	1460	1462	1463	rBV	452	158	0.01%	0.001%
22	5.884	1473	1491	1519	rBV	571920	1166876	40.58%	7.139%
23	6.328	1616	1629	1651	rBV	369514	747730	26.01%	4.574%
24	6.614	1714	1718	1719	rBV	936	767	0.03%	0.005%
25	6.665	1731	1734	1737	rBV3	769	579	0.02%	0.004%
26	6.698	1742	1744	1746	rBV2	688	395	0.01%	0.002%
27	6.714	1746	1749	1752	rBV	1211	792	0.03%	0.005%
28	6.768	1763	1766	1771	rBV	741	882	0.03%	0.005%
29	6.817	1778	1781	1785	rBV	1222	729	0.03%	0.004%
30	6.865	1789	1796	1803	rBV2	1530	2255	0.08%	0.014%
31	6.936	1815	1818	1820	rBV2	735	464	0.02%	0.003%
32	6.952	1820	1823	1827	rVB2	1085	744	0.03%	0.005%
33	7.055	1852	1855	1858	rBV	1405	772	0.03%	0.005%
34	7.071	1858	1860	1861	rBV	1190	568	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030273.D
 Acq On : 21 Mar 2019 18:12
 Operator : JC/SP
 Sample : K2022-07DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.116	1872	1874	1879	rVB3	872	634	0.02%	0.004%
36	7.145	1879	1883	1884	rBV2	624	380	0.01%	0.002%
37	7.157	1884	1887	1889	rBV	687	430	0.01%	0.003%
38	7.225	1896	1908	1926	rBV	206512	379510	13.20%	2.322%
39	7.563	2000	2013	2050	rBV	792213	1456432	50.65%	8.910%
40	7.849	2088	2102	2121	rBV	142409	256366	8.92%	1.568%
41	8.228	2213	2220	2223	rBV2	4427	5065	0.18%	0.031%
42	8.308	2234	2245	2275	rBV	478769	883878	30.74%	5.407%
43	8.575	2325	2328	2331	rBV2	1011	789	0.03%	0.005%
44	8.656	2351	2353	2355	rBV	958	565	0.02%	0.003%
45	8.890	2423	2426	2428	rBV	1013	760	0.03%	0.005%
46	8.990	2453	2457	2461	rBV	1586	1368	0.05%	0.008%
47	9.087	2475	2487	2528	rBV	843875	1639956	57.04%	10.033%
48	9.386	2574	2580	2586	rBV3	1381	2149	0.07%	0.013%
49	9.434	2592	2595	2599	rVB	1048	647	0.02%	0.004%
50	9.511	2616	2619	2620	rBV2	636	350	0.01%	0.002%
51	9.527	2621	2624	2630	rVB	1718	1429	0.05%	0.009%
52	9.556	2630	2633	2634	rBV	479	276	0.01%	0.002%
53	9.607	2646	2649	2651	rBV	1274	879	0.03%	0.005%
54	9.672	2666	2669	2671	rBV2	1173	734	0.03%	0.004%
55	9.816	2710	2714	2718	rBV2	1212	1341	0.05%	0.008%
56	9.852	2723	2725	2730	rVB2	1495	1083	0.04%	0.007%
57	9.890	2730	2737	2744	rBV2	1419	2000	0.07%	0.012%
58	9.942	2749	2753	2758	rBV	1266	1231	0.04%	0.008%
59	9.984	2762	2766	2772	rVB	826	857	0.03%	0.005%
60	10.122	2807	2809	2812	rVB	977	489	0.02%	0.003%
61	10.154	2812	2819	2822	rBV	1338	1211	0.04%	0.007%
62	10.173	2822	2825	2828	rVB	1235	780	0.03%	0.005%
63	10.199	2828	2833	2836	rBV	1462	1410	0.05%	0.009%
64	10.244	2845	2847	2850	rBV	774	386	0.01%	0.002%
65	10.296	2857	2863	2867	rBV2	1542	1894	0.07%	0.012%
66	10.386	2888	2891	2892	rBV	1291	719	0.03%	0.004%
67	10.427	2893	2904	2927	rVB	551130	890460	30.97%	5.448%
68	10.578	2948	2951	2953	rBV	1544	925	0.03%	0.006%
69	10.595	2953	2956	2957	rBV	1134	683	0.02%	0.004%
70	10.736	2996	3000	3003	rBV2	1264	997	0.03%	0.006%
71	10.775	3009	3012	3015	rBV	1267	1041	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030273.D
 Acq On : 21 Mar 2019 18:12
 Operator : JC/SP
 Sample : K2022-07DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.939	3061	3063	3066	rBV	827	493	0.02%	0.003%
73	10.977	3071	3075	3077	rBV2	945	722	0.03%	0.004%
74	11.035	3090	3093	3105	rBV2	1333	2309	0.08%	0.014%
75	11.077	3105	3106	3108	rBV	747	382	0.01%	0.002%
76	11.157	3126	3131	3132	rBV2	1211	1163	0.04%	0.007%
77	11.292	3170	3173	3174	rBV	596	306	0.01%	0.002%
78	11.369	3194	3197	3200	rBV2	1088	940	0.03%	0.006%
79	11.418	3204	3212	3220	rVV3	34256	52709	1.83%	0.322%
80	11.482	3221	3232	3259	rVB2	870314	1849857	64.34%	11.317%
81	11.871	3337	3353	3386	rBV2	1178474	2875287	100.00%	17.590%
82	12.591	3571	3577	3580	rBV	1374	1749	0.06%	0.011%
83	13.504	3852	3861	3881	rBV2	56973	117248	4.08%	0.717%
84	14.974	4312	4318	4320	rBV2	2353	2575	0.09%	0.016%


Sum of corrected areas: 16345993

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09A7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

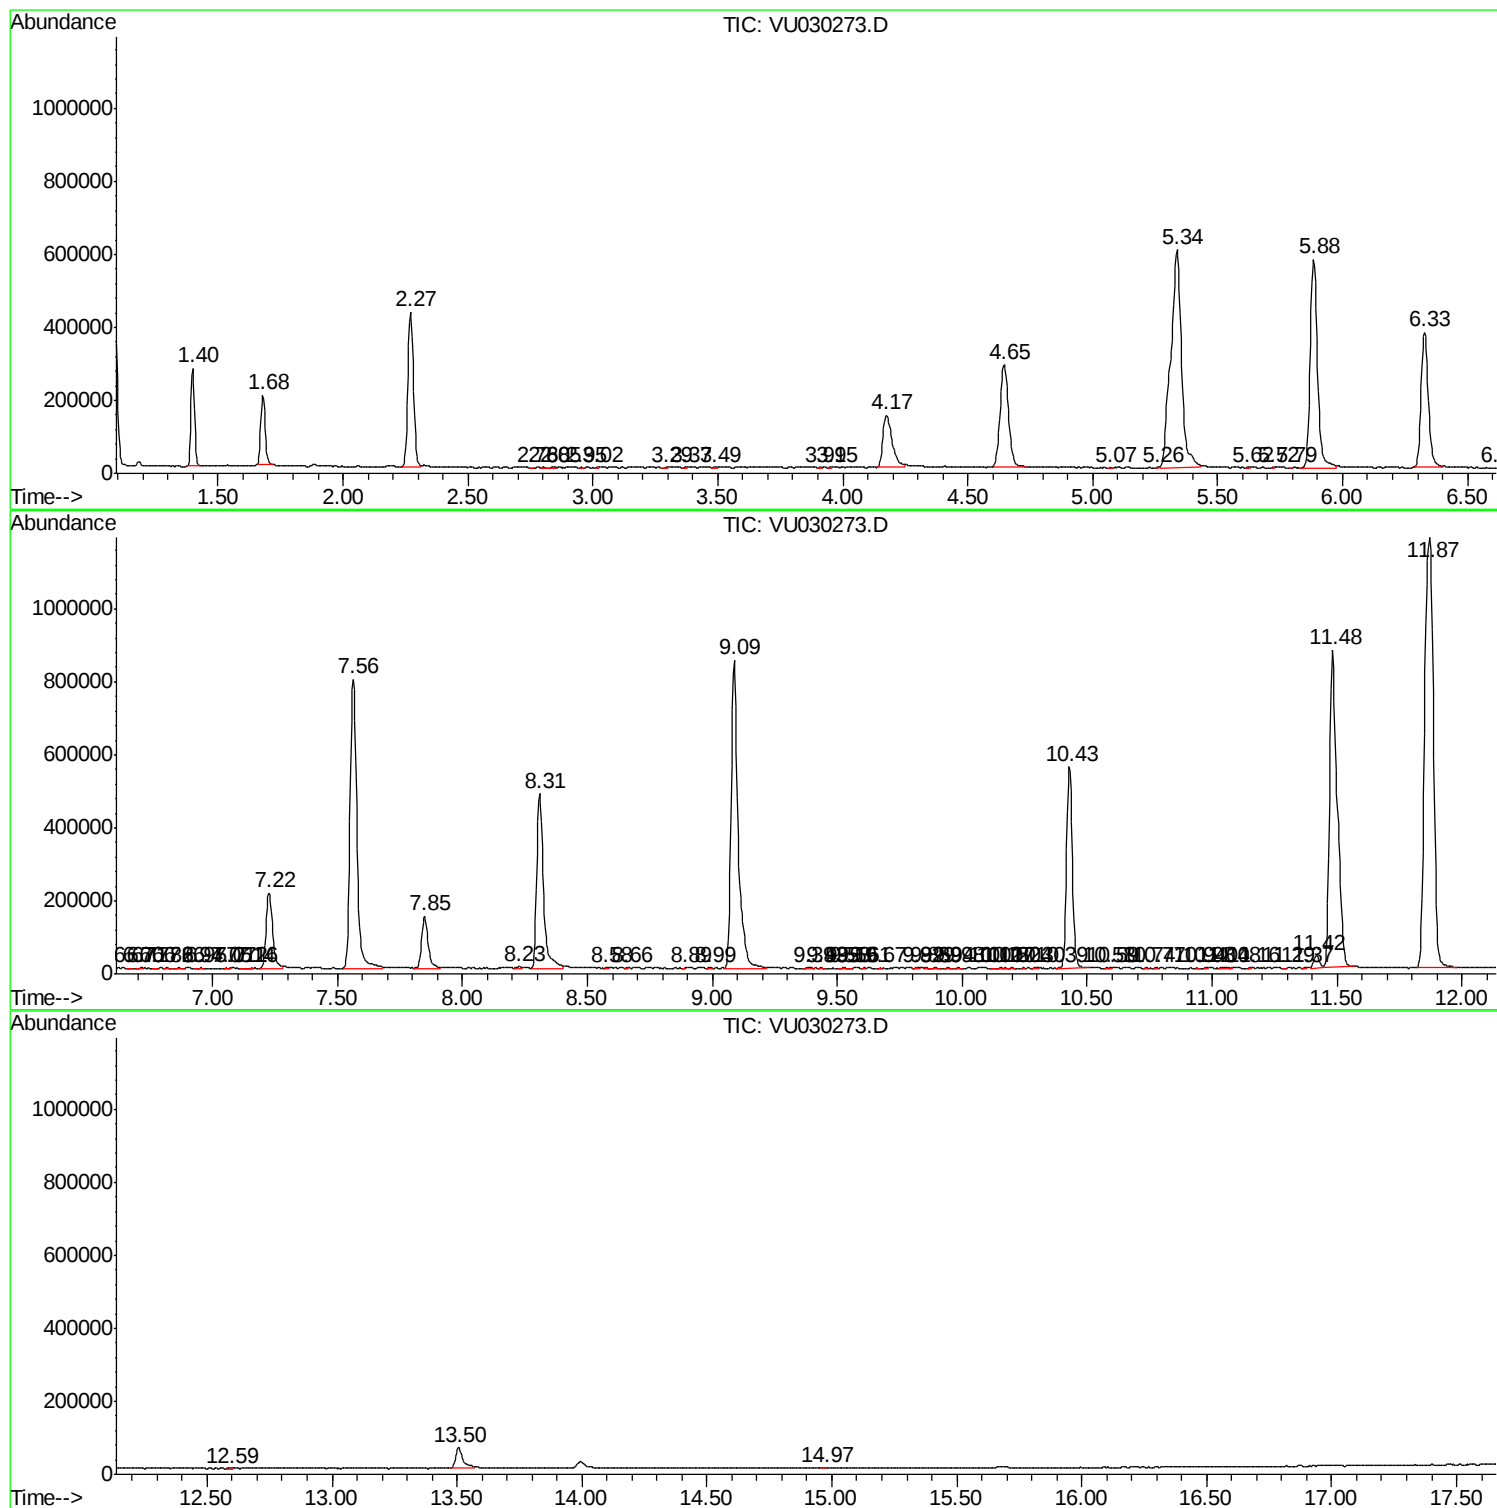

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030273.D
Acq On : 21 Mar 2019 18:12
Operator : JC/SP
Sample : K2022-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc