

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030275.D
 Acq On : 21 Mar 2019 18:58
 Operator : JC/SP
 Sample : K1967-18DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0967DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	39	rVB	13475	13658	0.24%	0.058%
2	1.399	89	96	109	rBV	275581	277979	4.89%	1.181%
3	1.678	175	183	197	rBV	198538	251102	4.42%	1.066%
4	2.270	357	367	380	rBV	431131	653611	11.49%	2.776%
5	2.575	460	462	466	rVB	1716	875	0.02%	0.004%
6	2.698	497	500	502	rBV2	1710	1073	0.02%	0.005%
7	2.749	513	516	520	rBV	1334	877	0.02%	0.004%
8	2.788	524	528	532	rBV	1536	1180	0.02%	0.005%
9	2.817	532	537	538	rBV	1135	1015	0.02%	0.004%
10	2.884	555	558	562	rVB	1269	937	0.02%	0.004%
11	3.148	637	640	642	rBV	1198	903	0.02%	0.004%
12	3.289	679	684	687	rVV	2060	2120	0.04%	0.009%
13	3.321	691	694	699	rVB	1407	1026	0.02%	0.004%
14	3.350	699	703	706	rVB	1353	872	0.02%	0.004%
15	3.450	730	734	737	rBV	1476	1136	0.02%	0.005%
16	3.636	786	792	795	rBV	1393	1399	0.02%	0.006%
17	3.743	820	825	830	rVV2	1274	1543	0.03%	0.007%
18	3.990	899	902	905	rBV	1512	1196	0.02%	0.005%
19	4.177	947	960	990	rBV	154044	408298	7.18%	1.734%
20	4.646	1090	1106	1134	rBV	291615	706351	12.42%	3.000%
21	4.800	1151	1154	1159	rBV	1187	926	0.02%	0.004%
22	4.926	1189	1193	1196	rBV2	1484	1062	0.02%	0.005%
23	4.974	1203	1208	1211	rVV	1047	1140	0.02%	0.005%
24	5.212	1278	1282	1286	rBV	1249	1143	0.02%	0.005%
25	5.234	1286	1289	1292	rBV	1325	930	0.02%	0.004%
26	5.337	1296	1321	1330	rBV2	618047	1772864	31.17%	7.529%
27	5.681	1426	1428	1432	rVB	1743	1070	0.02%	0.005%
28	5.726	1432	1442	1448	rBV	2300	4908	0.09%	0.021%
29	5.775	1454	1457	1461	rVB2	1343	1138	0.02%	0.005%
30	5.807	1461	1467	1472	rBV2	1668	2217	0.04%	0.009%
31	5.884	1478	1491	1530	rVV	574751	1157947	20.36%	4.918%
32	6.045	1538	1541	1545	rVB3	1021	882	0.02%	0.004%
33	6.074	1545	1550	1555	rVB	1563	1559	0.03%	0.007%
34	6.109	1558	1561	1568	rVB2	1178	1289	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030275.D
 Acq On : 21 Mar 2019 18:58
 Operator : JC/SP
 Sample : K1967-18DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0967DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.154	1572	1575	1582	rBV2	855	948	0.02%	0.004%
36	6.193	1582	1587	1591	rBV2	1583	1726	0.03%	0.007%
37	6.328	1615	1629	1657	rVV	384424	784259	13.79%	3.331%
38	6.521	1686	1689	1693	rVB	1399	1082	0.02%	0.005%
39	6.556	1693	1700	1703	rBV2	1586	2037	0.04%	0.009%
40	6.730	1751	1754	1759	rVB2	1209	1082	0.02%	0.005%
41	6.820	1779	1782	1786	rBV	1376	1184	0.02%	0.005%
42	6.919	1811	1813	1819	rVV	874	940	0.02%	0.004%
43	6.974	1827	1830	1833	rBV2	1327	938	0.02%	0.004%
44	7.067	1856	1859	1864	rBV	1410	1329	0.02%	0.006%
45	7.141	1876	1882	1888	rBV	1335	1982	0.03%	0.008%
46	7.225	1894	1908	1929	rBV	214135	399461	7.02%	1.696%
47	7.379	1953	1956	1962	rVB2	1760	1743	0.03%	0.007%
48	7.456	1977	1980	1984	rVV2	1000	886	0.02%	0.004%
49	7.562	2000	2013	2061	rVV	809580	1497770	26.34%	6.361%
50	7.762	2071	2075	2084	rVB	2258	2470	0.04%	0.010%
51	7.848	2091	2102	2116	rBV	147418	258619	4.55%	1.098%
52	8.012	2151	2153	2158	rVB	2059	1428	0.03%	0.006%
53	8.112	2178	2184	2188	rVB2	1162	1223	0.02%	0.005%
54	8.225	2215	2219	2227	rVB4	3030	4495	0.08%	0.019%
55	8.308	2234	2245	2279	rBV	507043	930971	16.37%	3.954%
56	8.617	2335	2341	2342	rBV3	1113	1222	0.02%	0.005%
57	8.649	2347	2351	2354	rBV2	919	920	0.02%	0.004%
58	8.794	2390	2396	2400	rVB	1039	981	0.02%	0.004%
59	8.820	2400	2404	2405	rBV2	1260	871	0.02%	0.004%
60	9.086	2472	2487	2491	rBV	877021	1377649	24.22%	5.851%
61	9.305	2551	2555	2556	rBV	1377	954	0.02%	0.004%
62	9.453	2598	2601	2606	rVB2	1194	1069	0.02%	0.005%
63	9.485	2607	2611	2615	rVB	1381	1243	0.02%	0.005%
64	9.578	2633	2640	2644	rBV	1027	1548	0.03%	0.007%
65	9.633	2652	2657	2659	rBV	1156	1023	0.02%	0.004%
66	9.758	2693	2696	2702	rVB2	1707	1723	0.03%	0.007%
67	9.797	2702	2708	2710	rBV2	1418	1354	0.02%	0.006%
68	10.025	2773	2779	2781	rBV3	1199	1230	0.02%	0.005%
69	10.106	2798	2804	2806	rBV2	1059	1209	0.02%	0.005%
70	10.138	2811	2814	2820	rBV	989	1170	0.02%	0.005%
71	10.167	2820	2823	2829	rVB2	1588	1376	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030275.D
 Acq On : 21 Mar 2019 18:58
 Operator : JC/SP
 Sample : K1967-18DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0967DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.199	2829	2833	2836	rBV2	1278	1222	0.02%	0.005%
73	10.305	2862	2866	2870	rBV	917	890	0.02%	0.004%
74	10.427	2892	2904	2926	rBV	567211	923503	16.24%	3.922%
75	10.591	2952	2955	2961	rVB2	1199	1115	0.02%	0.005%
76	10.810	3018	3023	3026	rBV	1206	1138	0.02%	0.005%
77	10.964	3066	3071	3074	rBV	1514	1149	0.02%	0.005%
78	11.006	3082	3084	3088	rVB	1424	858	0.02%	0.004%
79	11.215	3147	3149	3159	rVB	1320	1226	0.02%	0.005%
80	11.337	3184	3187	3194	rBV2	1326	1106	0.02%	0.005%
81	11.414	3199	3211	3221	rBV	455453	728997	12.82%	3.096%
82	11.504	3221	3239	3265	rVB2	2273945	4872347	85.68%	20.692%
83	11.749	3312	3315	3325	rVB3	1350	1422	0.03%	0.006%
84	11.874	3334	3354	3379	rBV2	2896557	5686990	100.00%	24.152%
85	12.080	3415	3418	3423	rBV6	1122	1036	0.02%	0.004%
86	12.298	3482	3486	3488	rBV3	1147	917	0.02%	0.004%
87	12.427	3523	3526	3531	rVB2	1402	1146	0.02%	0.005%
88	12.543	3559	3562	3565	rBV	1345	1067	0.02%	0.005%
89	12.649	3589	3595	3597	rBV3	1828	1940	0.03%	0.008%
90	12.761	3626	3630	3634	rBV2	1369	1125	0.02%	0.005%
91	12.819	3644	3648	3651	rBV	1137	918	0.02%	0.004%
92	12.884	3659	3668	3680	rVB5	3730	7992	0.14%	0.034%
93	13.343	3808	3811	3815	rVB2	1230	877	0.02%	0.004%
94	13.453	3839	3845	3848	rBV	921	1101	0.02%	0.005%
95	13.501	3848	3860	3884	rBV	282254	496796	8.74%	2.110%
96	13.986	3999	4011	4033	rBV2	121344	234781	4.13%	0.997%
97	14.366	4123	4129	4132	rBV2	1690	2119	0.04%	0.009%
98	14.469	4156	4161	4164	rBV2	2046	2165	0.04%	0.009%
99	15.221	4393	4395	4401	rBV2	1405	1194	0.02%	0.005%
100	15.324	4424	4427	4430	rBV	1564	1191	0.02%	0.005%


Sum of corrected areas: 23546669

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030275.D
Acq On : 21 Mar 2019 18:58
Operator : JC/SP
Sample : K1967-18DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0967DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

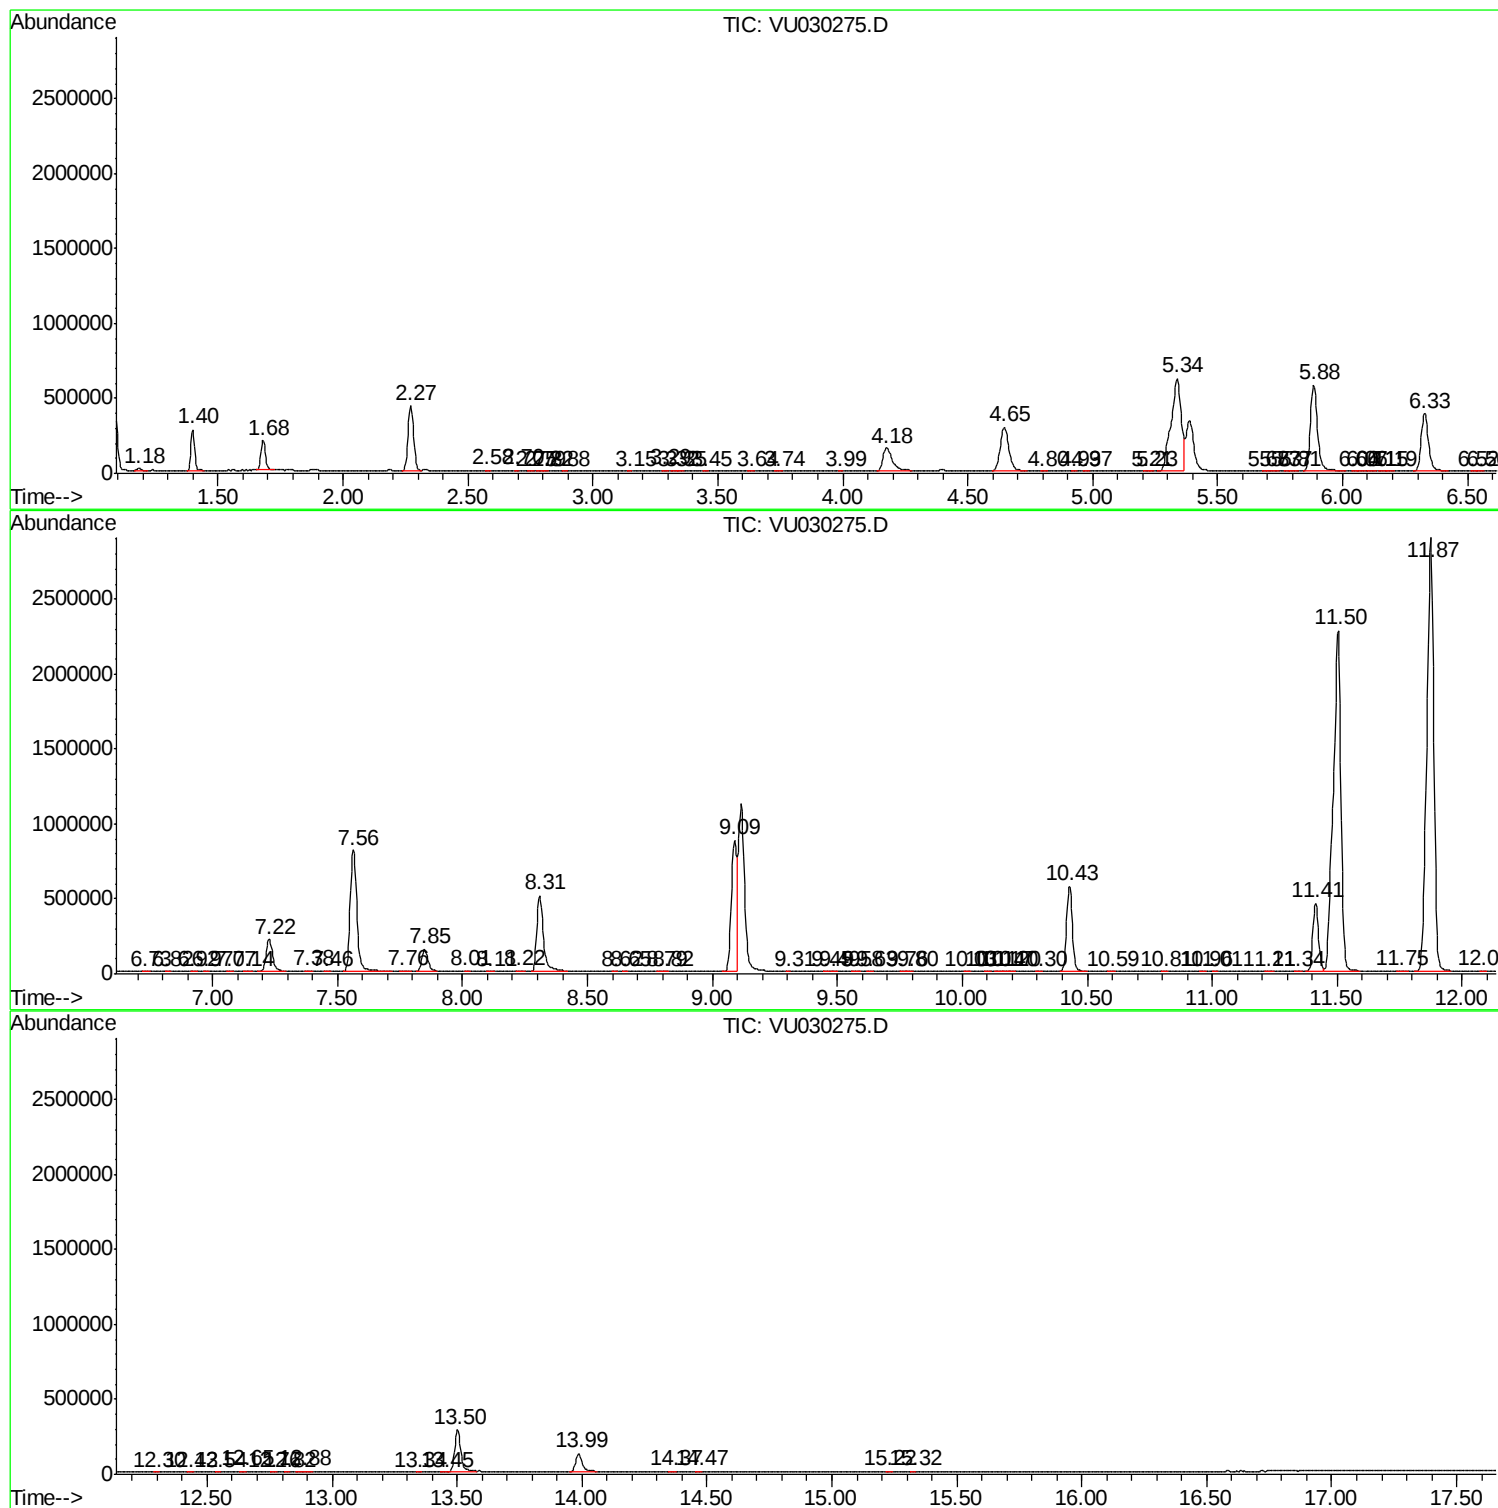

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030275.D
Acq On : 21 Mar 2019 18:58
Operator : JC/SP
Sample : K1967-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0967DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030275.D
Acq On : 21 Mar 2019 18:58
Operator : JC/SP
Sample : K1967-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0967DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc