

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030276.D
 Acq On : 21 Mar 2019 19:21
 Operator : JC/SP
 Sample : K1967-17DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0966DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.184	24	29	35	rBV3	12101	11201	0.24%	0.048%
2	1.399	89	96	108	rBV	279888	273036	5.89%	1.176%
3	1.679	176	183	198	rVB	196296	245181	5.29%	1.056%
4	2.270	356	367	381	rBV	436728	664214	14.32%	2.862%
5	2.656	481	487	492	rBV	1744	2451	0.05%	0.011%
6	2.804	530	533	537	rBV	1446	1301	0.03%	0.006%
7	3.103	624	626	631	rVB	1027	776	0.02%	0.003%
8	3.274	676	679	683	rVB	1092	951	0.02%	0.004%
9	3.309	683	690	692	rBV	1950	1965	0.04%	0.008%
10	3.428	724	727	731	rVB	1563	1171	0.03%	0.005%
11	3.537	757	761	763	rBV	1265	1007	0.02%	0.004%
12	3.666	795	801	804	rBV	1478	1860	0.04%	0.008%
13	3.794	838	841	847	rVB	1757	1463	0.03%	0.006%
14	3.868	860	864	868	rBV	1888	1608	0.03%	0.007%
15	4.036	911	916	918	rVB2	948	796	0.02%	0.003%
16	4.074	925	928	931	rVB2	1214	802	0.02%	0.003%
17	4.093	931	934	938	rBV2	949	883	0.02%	0.004%
18	4.177	948	960	987	rBV2	155208	404818	8.73%	1.744%
19	4.486	1048	1056	1060	rBV3	1364	2014	0.04%	0.009%
20	4.521	1064	1067	1069	rBV	1362	962	0.02%	0.004%
21	4.572	1079	1083	1087	rBV	1223	1200	0.03%	0.005%
22	4.646	1090	1106	1134	rVV	296417	745766	16.08%	3.213%
23	4.920	1188	1191	1194	rBV3	1039	801	0.02%	0.003%
24	5.064	1233	1236	1241	rVB	1361	1341	0.03%	0.006%
25	5.193	1272	1276	1283	rBV	1355	1945	0.04%	0.008%
26	5.338	1299	1321	1328	rBV2	623751	1732142	37.34%	7.463%
27	5.386	1330	1336	1373	rVB	1003138	2049997	44.19%	8.832%
28	5.659	1417	1421	1426	rBV3	1606	1541	0.03%	0.007%
29	5.682	1426	1428	1430	rBV	1285	795	0.02%	0.003%
30	5.794	1459	1463	1464	rBV2	1337	838	0.02%	0.004%
31	5.884	1477	1491	1522	rBV	579487	1179961	25.44%	5.084%
32	6.193	1581	1587	1591	rBV4	1090	1402	0.03%	0.006%
33	6.241	1598	1602	1606	rVB2	1352	1228	0.03%	0.005%
34	6.261	1606	1608	1612	rVB	1178	780	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030276.D
 Acq On : 21 Mar 2019 19:21
 Operator : JC/SP
 Sample : K1967-17DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 C0966DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1615	1629	1660	rBV	385285	786373	16.95%	3.388%
36	6.563	1691	1702	1711	rBV2	1769	4110	0.09%	0.018%
37	6.923	1810	1814	1817	rBV3	1386	1368	0.03%	0.006%
38	6.994	1832	1836	1838	rBV	1197	870	0.02%	0.004%
39	7.087	1861	1865	1871	rBV	1266	1376	0.03%	0.006%
40	7.183	1890	1895	1897	rBV	1063	1005	0.02%	0.004%
41	7.225	1897	1908	1932	rBV	210984	392242	8.46%	1.690%
42	7.441	1971	1975	1978	rBV2	1436	1182	0.03%	0.005%
43	7.563	2000	2013	2039	rBV	818467	1485371	32.02%	6.400%
44	7.849	2090	2102	2128	rBV	145218	265993	5.73%	1.146%
45	8.154	2193	2197	2199	rBV	1411	1075	0.02%	0.005%
46	8.177	2199	2204	2205	rBV2	1886	1401	0.03%	0.006%
47	8.222	2215	2218	2221	rBV2	2708	2026	0.04%	0.009%
48	8.264	2227	2231	2234	rBV	1219	1092	0.02%	0.005%
49	8.309	2234	2245	2276	rBV	507267	940377	20.27%	4.052%
50	8.585	2329	2331	2335	rBV	1074	796	0.02%	0.003%
51	8.662	2352	2355	2357	rVB	1708	1028	0.02%	0.004%
52	8.711	2366	2370	2374	rVB3	1433	1122	0.02%	0.005%
53	9.042	2469	2473	2475	rBV	1306	1056	0.02%	0.005%
54	9.090	2475	2488	2490	rBV	900198	1295291	27.92%	5.581%
55	9.437	2593	2596	2599	rBV	1306	1063	0.02%	0.005%
56	9.563	2629	2635	2639	rBV3	1170	1115	0.02%	0.005%
57	9.649	2659	2662	2668	rVB3	1495	1618	0.03%	0.007%
58	9.678	2668	2671	2676	rBV2	1467	1574	0.03%	0.007%
59	9.730	2684	2687	2693	rVB	2497	1864	0.04%	0.008%
60	9.765	2693	2698	2700	rBV2	1636	1599	0.03%	0.007%
61	9.781	2701	2703	2707	rVV	1675	1609	0.03%	0.007%
62	9.865	2725	2729	2733	rBV	1072	867	0.02%	0.004%
63	9.971	2756	2762	2766	rBV2	969	1159	0.02%	0.005%
64	10.125	2807	2810	2813	rBV2	908	782	0.02%	0.003%
65	10.231	2837	2843	2846	rBV2	1734	2169	0.05%	0.009%
66	10.270	2851	2855	2857	rVV	1402	1111	0.02%	0.005%
67	10.376	2883	2888	2892	rVB	1271	1268	0.03%	0.005%
68	10.428	2892	2904	2928	rBV	580177	936543	20.19%	4.035%
69	10.601	2951	2958	2962	rBV2	2573	2727	0.06%	0.012%
70	10.649	2969	2973	2975	rBV	1259	984	0.02%	0.004%
71	10.765	3005	3009	3017	rVB2	1187	930	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032119\
 Data File : VU030276.D
 Acq On : 21 Mar 2019 19:21
 Operator : JC/SP
 Sample : K1967-17DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0966DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.871	3037	3042	3046	rBV2	913	1195	0.03%	0.005%
73	10.997	3078	3081	3082	rBV	1314	831	0.02%	0.004%
74	11.022	3086	3089	3093	rVB	1648	1242	0.03%	0.005%
75	11.055	3093	3099	3102	rBV	1154	1247	0.03%	0.005%
76	11.174	3129	3136	3144	rBV2	1619	3017	0.07%	0.013%
77	11.235	3152	3155	3158	rBV	1350	1015	0.02%	0.004%
78	11.415	3200	3211	3221	rBV	316181	506715	10.92%	2.183%
79	11.501	3221	3238	3268	rVB2	1647240	3903774	84.15%	16.819%
80	11.874	3336	3354	3381	rBV2	2208967	4639075	100.00%	19.987%
81	12.135	3428	3435	3440	rBV	2262	2957	0.06%	0.013%
82	12.280	3477	3480	3483	rBV2	1106	860	0.02%	0.004%
83	12.437	3520	3529	3532	rBV3	1215	2144	0.05%	0.009%
84	12.685	3603	3606	3610	rVB	1078	813	0.02%	0.004%
85	12.707	3610	3613	3614	rBV	1720	1108	0.02%	0.005%
86	12.820	3643	3648	3651	rBV2	995	900	0.02%	0.004%
87	12.874	3657	3665	3679	rBV6	5881	13930	0.30%	0.060%
88	13.251	3778	3782	3785	rBV2	1363	938	0.02%	0.004%
89	13.379	3816	3822	3824	rBV3	1223	1143	0.02%	0.005%
90	13.399	3825	3828	3830	rBV2	1392	832	0.02%	0.004%
91	13.501	3848	3860	3888	rBV	238833	430683	9.28%	1.856%
92	13.714	3921	3926	3928	rBV	1627	1613	0.03%	0.007%
93	13.897	3980	3983	3989	rBV	1241	953	0.02%	0.004%
94	13.987	4000	4011	4039	rBV2	100897	204744	4.41%	0.882%
95	14.469	4159	4161	4164	rVB2	1914	1050	0.02%	0.005%
96	14.575	4191	4194	4199	rBV	1451	1578	0.03%	0.007%
97	14.630	4208	4211	4213	rBV2	1134	813	0.02%	0.004%
98	14.781	4255	4258	4260	rBV2	1431	962	0.02%	0.004%
99	14.942	4305	4308	4311	rBV3	1268	1155	0.02%	0.005%
100	15.263	4405	4408	4410	rBV	1251	848	0.02%	0.004%


Sum of corrected areas: 23210468

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032119\
Data File : VU030276.D
Acq On : 21 Mar 2019 19:21
Operator : JC/SP
Sample : K1967-17DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0966DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

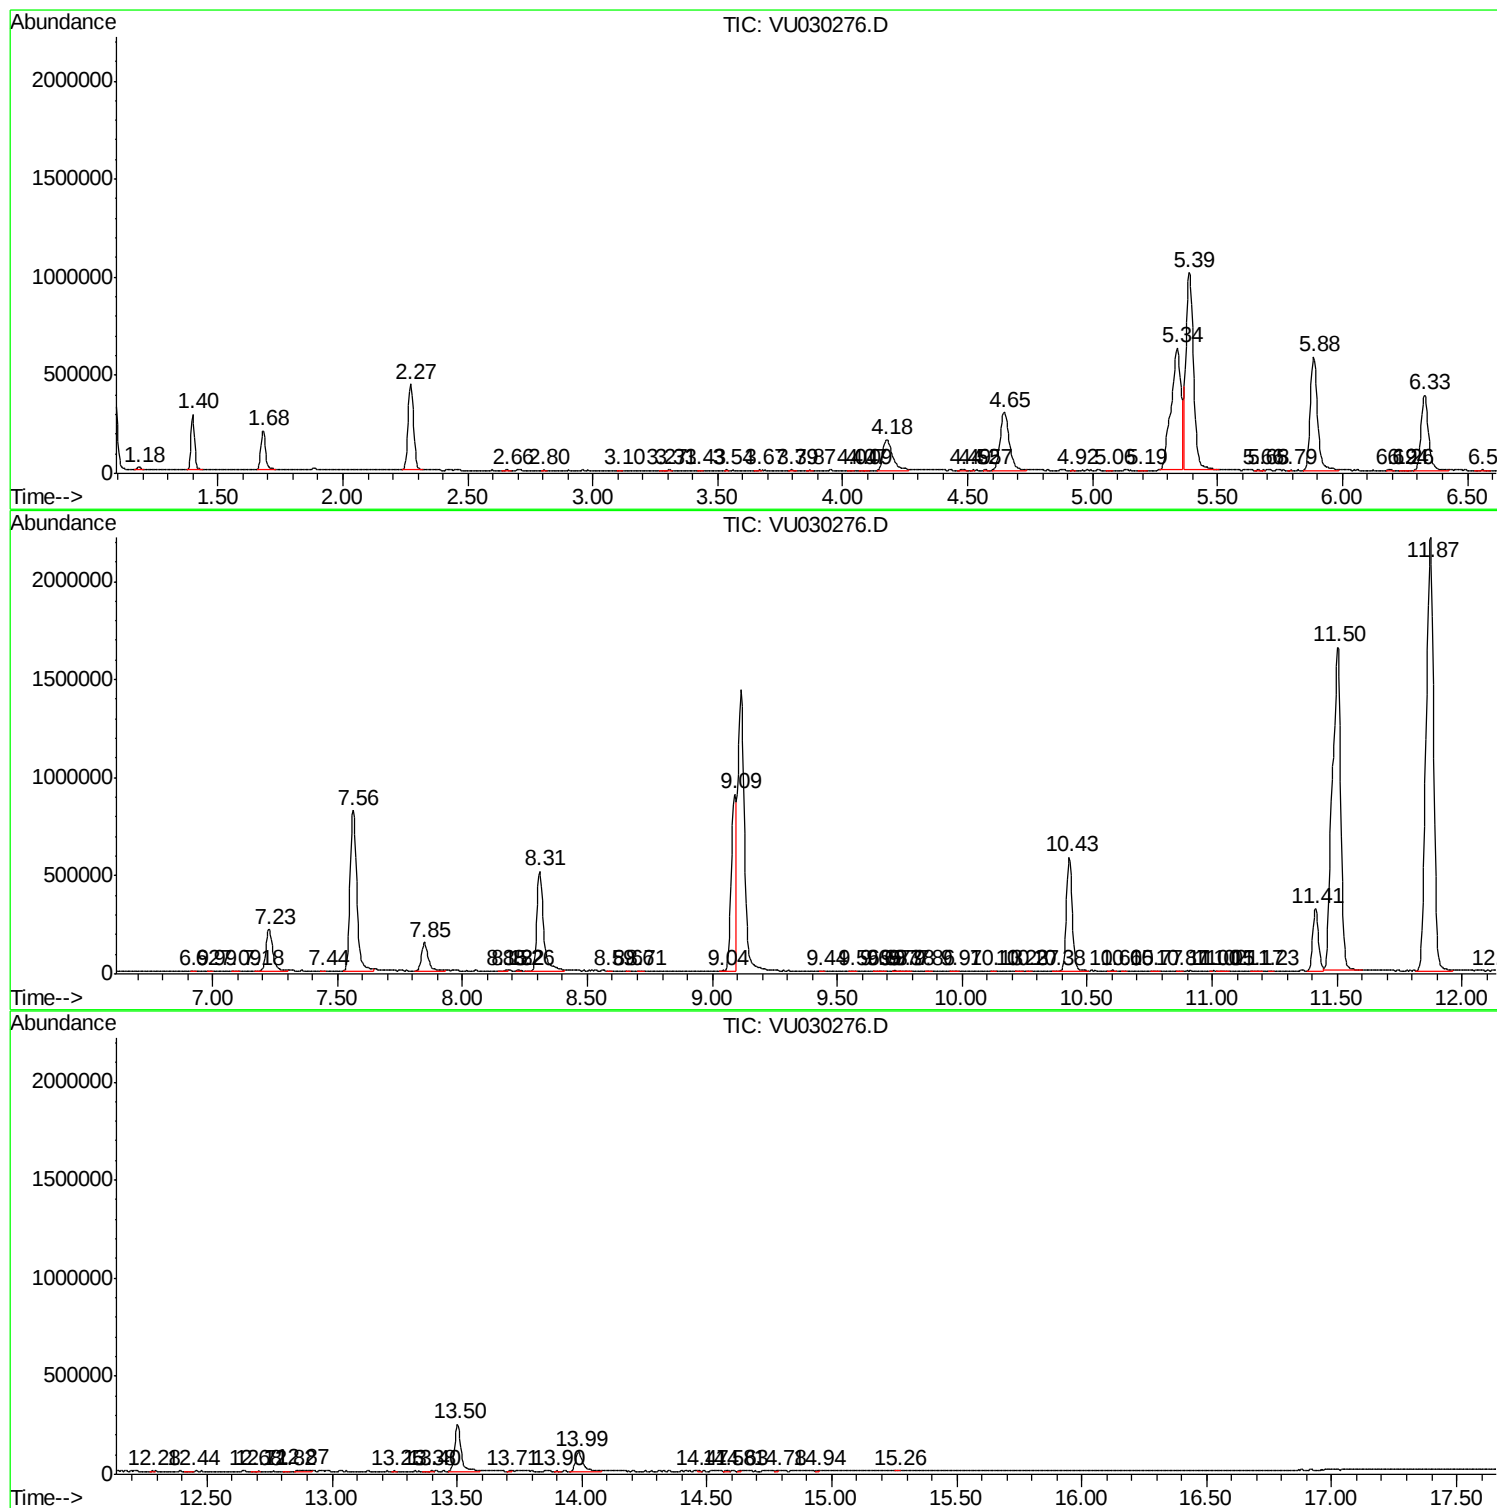

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030276.D
Acq On : 21 Mar 2019 19:21
Operator : JC/SP
Sample : K1967-17DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0966DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032119\
Data File : VU030276.D
Acq On : 21 Mar 2019 19:21
Operator : JC/SP
Sample : K1967-17DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0966DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc