


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032119\
 Data File : VU030250.D
 Acq On : 21 Mar 2019 08:59
 Operator : JC/SP
 Sample : BFB39
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 25 12:01:39 2019

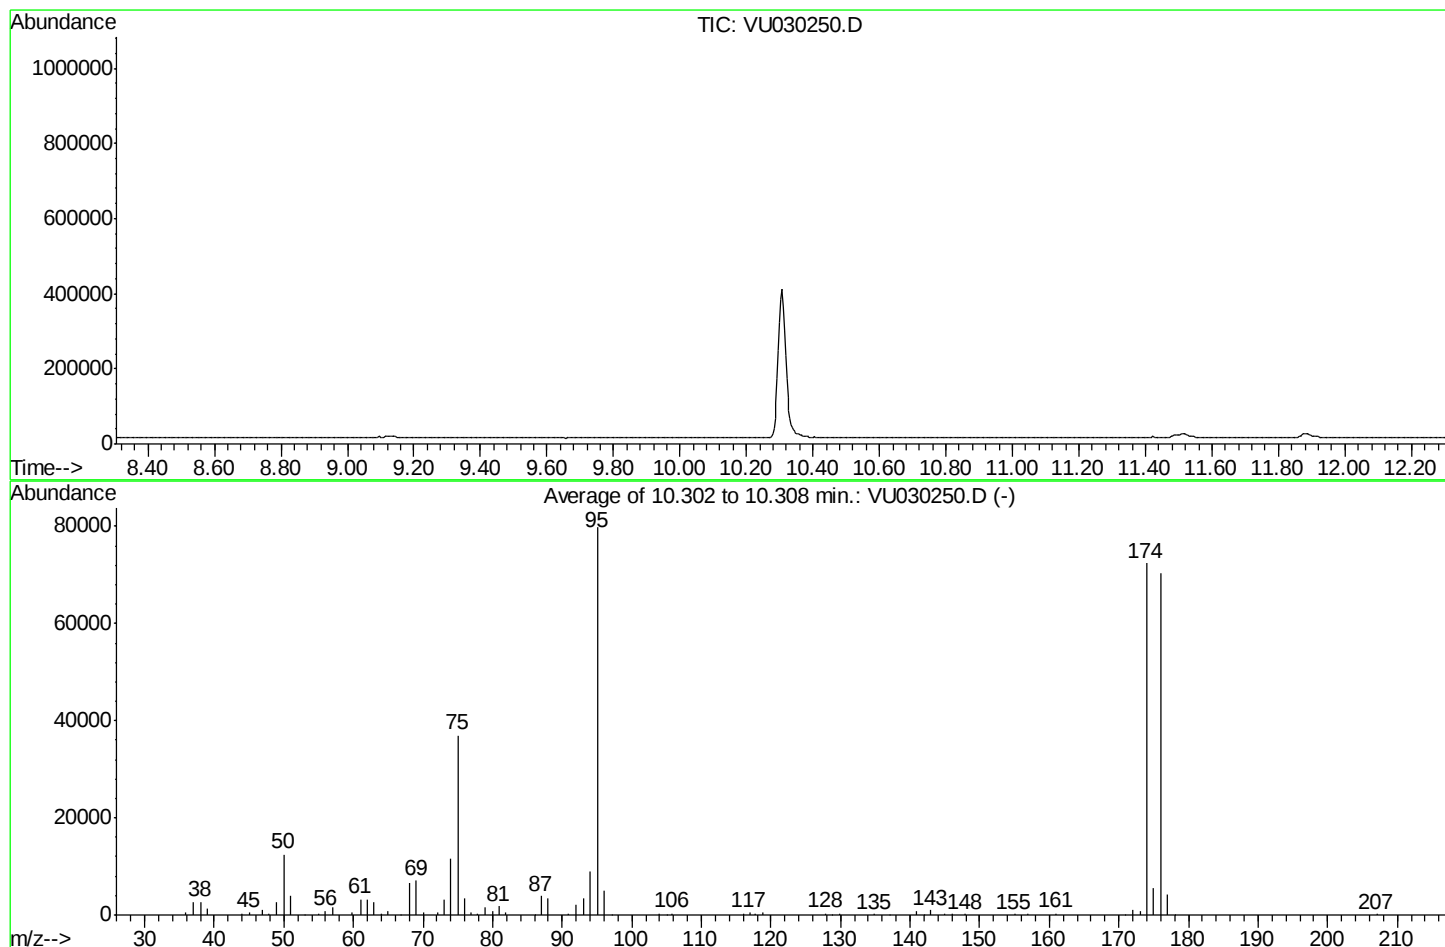

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	12465	PASS
75	95	30	80	46.3	36952	PASS
95	95	100	100	100.0	79816	PASS
96	95	5	9	6.2	4985	PASS
173	174	0.00	2	1.0	752	PASS
174	95	50	120	90.7	72410	PASS
175	174	5	9	7.6	5499	PASS
176	174	95	101	97.2	70352	PASS
177	176	5	9	6.1	4311	PASS

Scan 2854 (10.266 min): VU030250.D
BFB39

m/z	Abundance
40.00	17168.0
43.90	580.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	561.0
37.00	2547.0
38.00	2542.0
39.00	1142.0
40.00	17240.0
44.00	930.0
45.00	473.0
47.00	856.0
47.80	315.0
49.00	2574.0
50.00	12253.0
51.00	3899.0
55.00	139.0
56.00	844.0
57.00	1675.0
59.90	422.0
61.00	2975.0
62.00	3028.0
63.00	2580.0
64.10	282.0
65.00	663.0
66.80	105.0
68.00	6505.0
69.00	6840.0
70.00	506.0
72.10	415.0
73.00	2945.0
74.00	11464.0
75.00	36104.0
76.00	3182.0
77.00	459.0
77.80	324.0
79.00	1694.0
80.00	662.0
80.90	1656.0
81.90	536.0
86.10	102.0
87.00	3695.0
88.00	3349.0
90.90	220.0
92.00	1947.0
93.00	3365.0
94.00	8699.0
95.10	76080.0
96.00	4866.0
103.90	199.0
104.90	135.0
105.90	209.0
116.10	217.0
116.90	596.0
117.80	234.0
118.90	510.0
127.90	294.0
128.80	138.0
130.00	237.0
134.90	191.0
140.90	810.0
142.90	1047.0
145.00	197.0
146.00	115.0
147.90	173.0
155.00	208.0
156.90	156.0
161.00	246.0
170.90	122.0
172.00	824.0
173.00	758.0
174.00	68056.0
175.00	5230.0
176.00	65504.0
177.00	4139.0
207.10	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.00	604.0
37.00	2721.0
38.00	2796.0
39.00	1253.0
40.00	16816.0
44.00	967.0
45.00	495.0
47.00	968.0
47.90	312.0
49.00	2833.0
50.00	12931.0
51.00	4107.0
52.90	129.0
54.90	143.0
56.00	867.0
57.00	1525.0
59.80	523.0
61.00	3296.0
62.00	3200.0
63.00	2749.0
64.00	288.0
65.00	747.0
68.00	6763.0
69.00	7267.0
70.00	473.0
72.10	435.0
73.00	3257.0
74.00	11974.0
75.00	38224.0
76.00	3473.0
76.80	414.0
77.90	268.0
78.90	1597.0
80.00	748.0
80.90	1883.0
81.90	583.0
86.00	139.0
87.00	4067.0
88.00	3454.0
90.90	219.0
92.00	2137.0
93.00	3565.0
94.00	9203.0
95.10	82128.0
96.00	5151.0
97.10	110.0
103.90	202.0
104.90	141.0
105.80	312.0
116.00	297.0
116.90	506.0
117.80	285.0
118.90	526.0
127.90	315.0
128.80	143.0
129.90	231.0
134.90	212.0
136.90	136.0
140.90	830.0
142.00	112.0
143.00	989.0
145.00	178.0
146.00	168.0
147.90	173.0
155.00	194.0
156.90	164.0
161.00	306.0
170.90	134.0
172.00	986.0
173.00	788.0
174.00	74712.0
175.00	5730.0
176.00	72512.0
177.00	4450.0
178.00	105.0
207.00	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.00	674.0
37.00	2586.0
38.00	2900.0
39.00	1253.0
40.00	16488.0
44.00	844.0
45.00	507.0
47.00	1037.0
48.00	317.0
49.00	2813.0
50.00	12212.0
51.00	3951.0
52.90	110.0
54.90	157.0
56.00	853.0
57.00	1426.0
59.90	549.0
61.00	3230.0
62.00	3081.0
63.00	2665.0
64.00	325.0
65.00	729.0
68.10	6495.0
69.00	7220.0
70.00	476.0
72.00	422.0
73.00	3174.0
74.00	11247.0
75.00	36528.0
76.00	3315.0
76.90	392.0
78.00	258.0
78.90	1530.0
80.00	708.0
80.90	1905.0
81.90	556.0
86.00	141.0
86.90	3953.0
88.00	3239.0
90.90	182.0
92.00	2075.0
93.00	3341.0
94.00	8972.0
95.10	81240.0
96.10	4940.0
97.10	155.0
104.00	188.0
105.00	142.0
105.80	331.0
116.00	333.0
117.00	448.0
117.80	286.0
118.90	443.0
127.90	287.0
128.90	132.0
129.90	237.0
134.80	169.0
137.00	140.0
140.90	710.0
142.00	102.0
143.00	853.0
145.00	177.0
146.00	186.0
148.00	192.0
155.00	163.0
156.90	134.0
161.00	259.0
170.90	156.0
172.00	1028.0
173.00	710.0
174.00	74464.0
175.00	5538.0
176.00	73040.0
177.00	4345.0
207.00	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39